

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012425\
Data File : FF015317.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2025 17:52
Operator : YP\AJ
Sample : PB166221BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB166221BL

Integration File: autoint1.e
Quant Time: Jan 24 23:32:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011425.M
Quant Title :
QLast Update : Tue Jan 14 11:12:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.020	1746403	13.337 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012425\
Data File : FF015317.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2025 17:52
Operator : YP\AJ
Sample : PB166221BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB166221BL

Integration File: autoint1.e
Quant Time: Jan 24 23:32:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011425.M
Quant Title :
QLast Update : Tue Jan 14 11:12:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

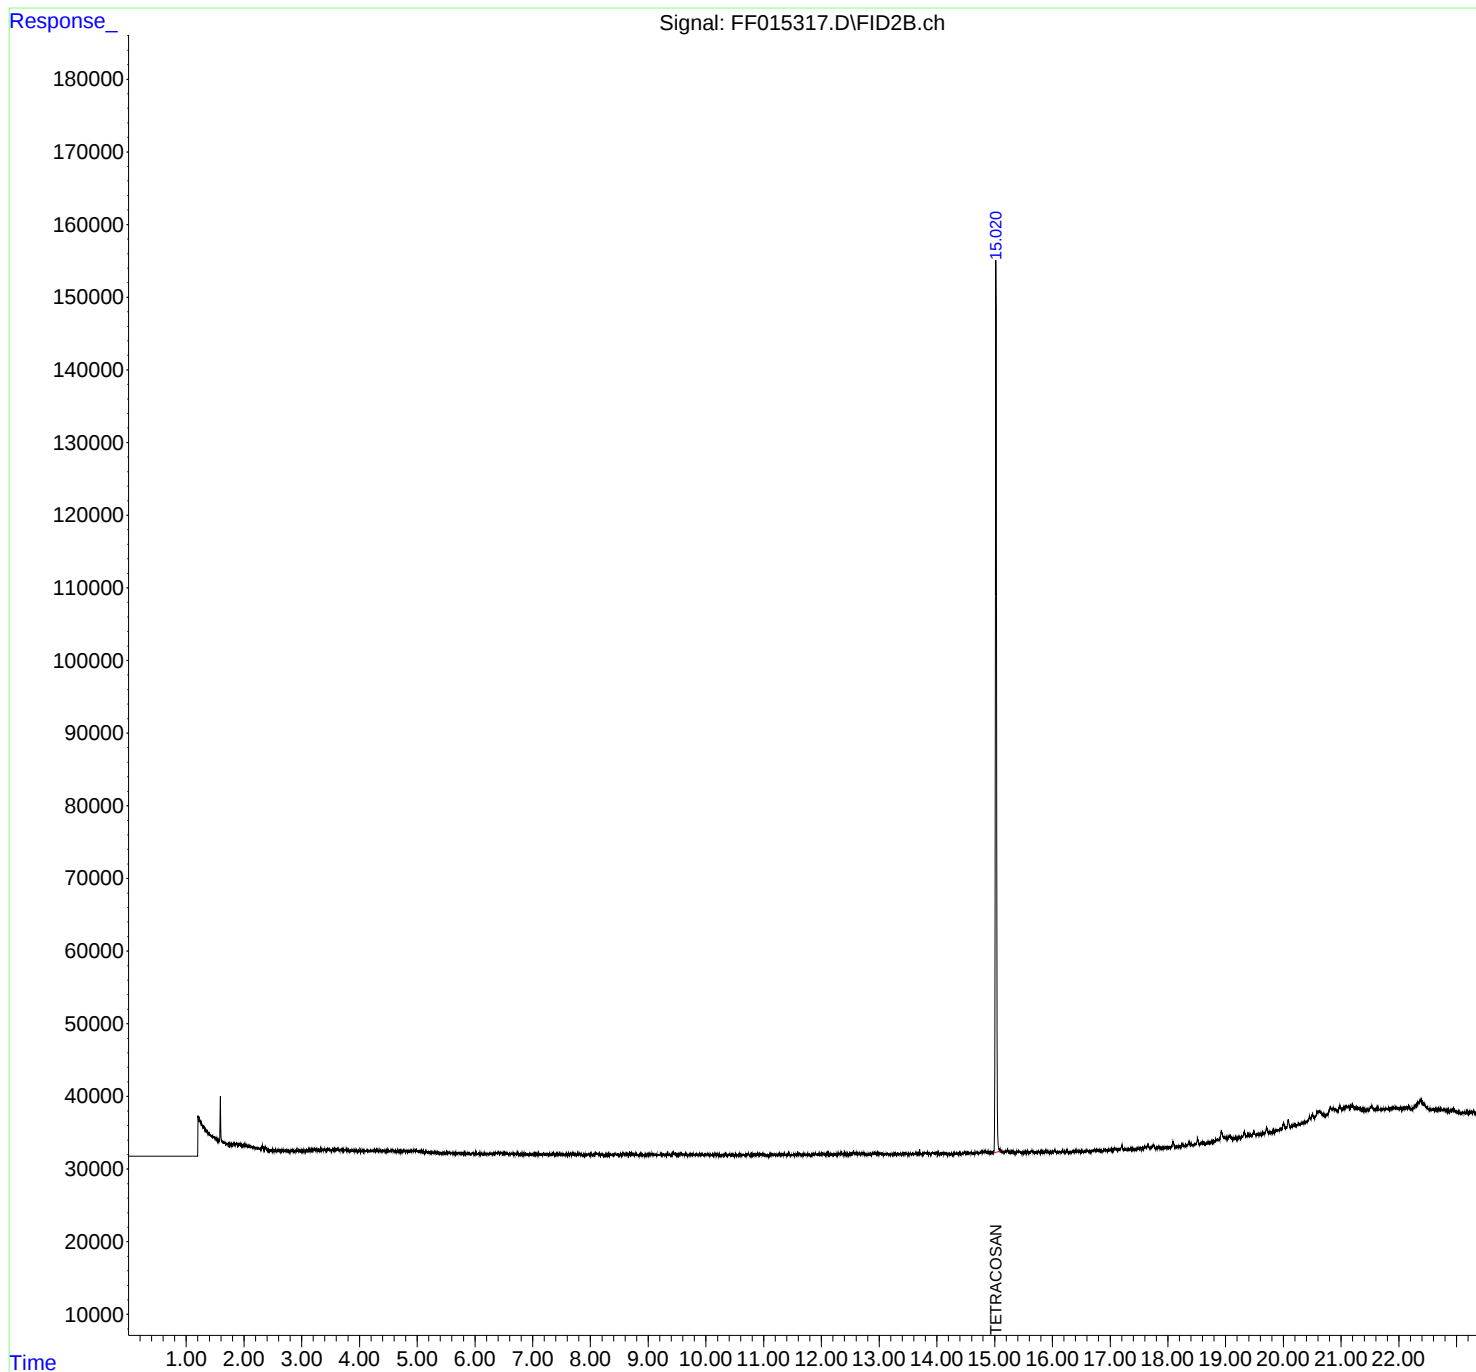

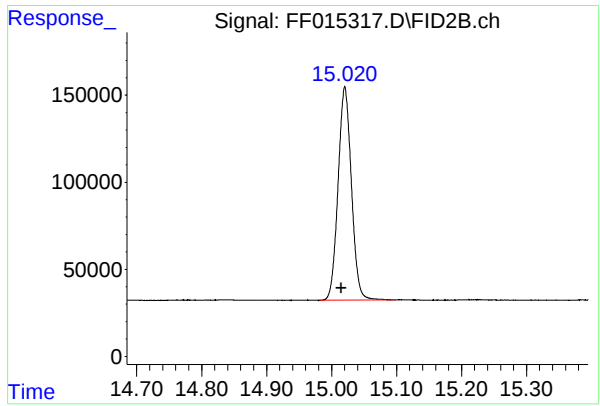

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.020 min
Delta R.T.: 0.006 min
Response: 1746403
Conc: 13.34 ug/ml

Instrument :
FID_F
ClientSampleId :
PB166221BL