

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012622\
Data File : FF009784.D
Signal(s) : FID2B.ch
Acq On : 26 Jan 2022 09:33
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 27 00:11:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.332	224487	1.650 ug/ml
16)	N-HEXATRIACONTANE	19.876	513264	4.978 ug/ml
18)	N-TETRACONTANE	21.388	398750	4.390 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012622\
Data File : FF009784.D
Signal(s) : FID2B.ch
Acq On : 26 Jan 2022 09:33
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 27 00:11:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

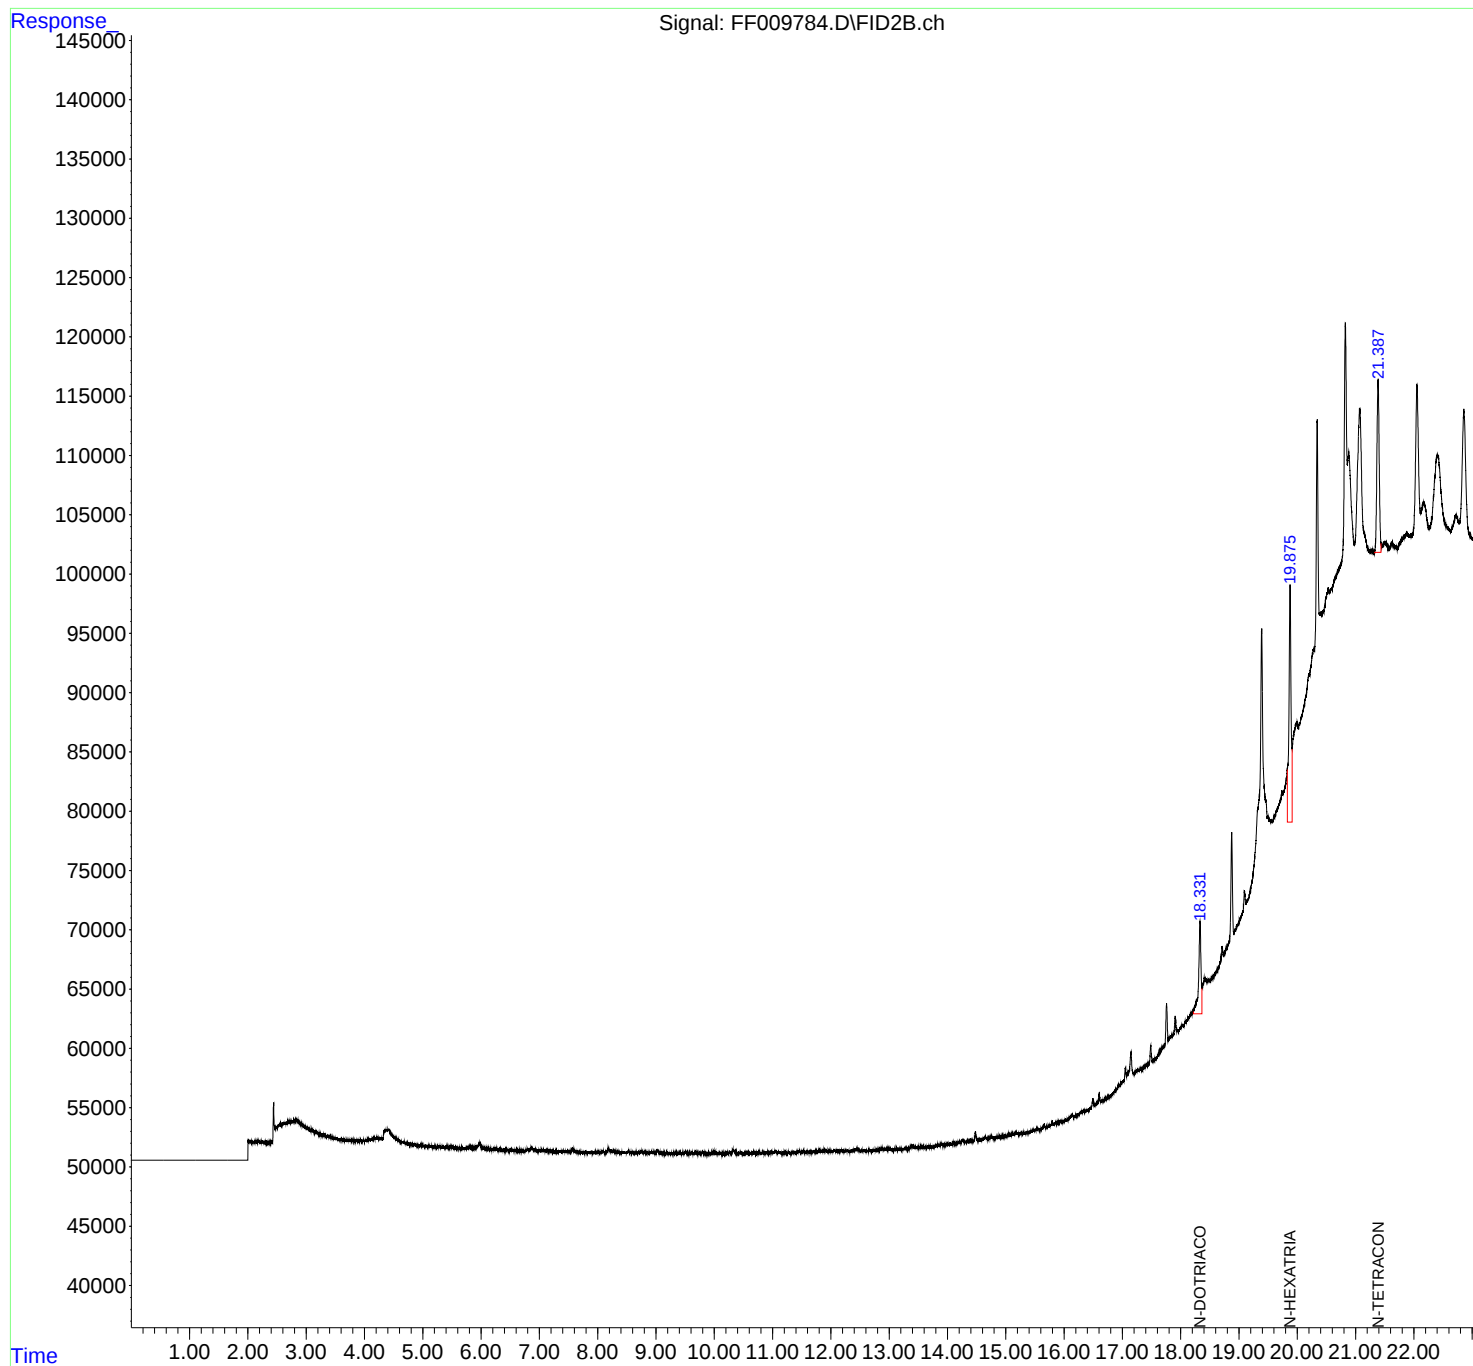


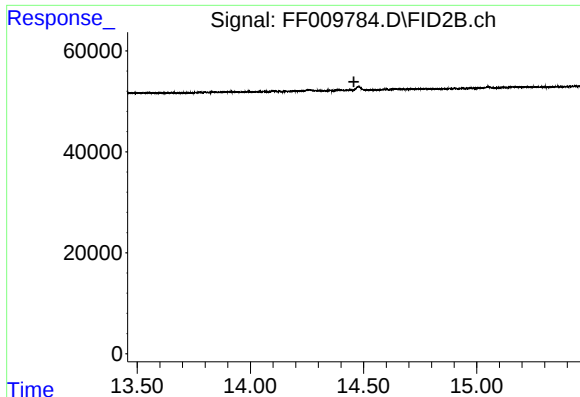

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.457 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

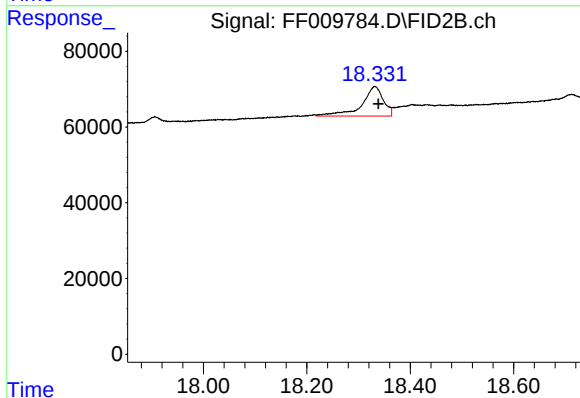


#14 N-DOTRIACONTANE

R.T.: 18.332 min
Delta R.T.: -0.007 min
Response: 224487
Conc: 1.65 ug/ml

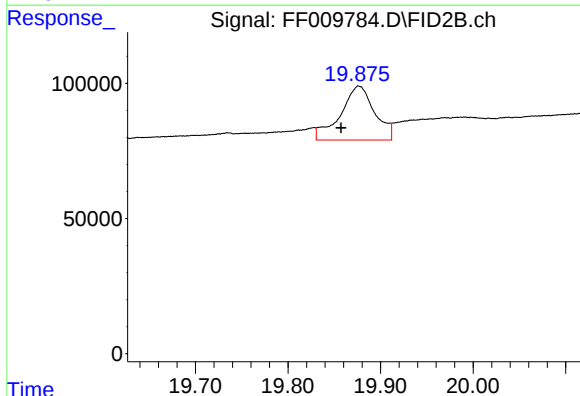

#16 N-HEXATRIACONTANE

R.T.: 19.876 min
Delta R.T.: 0.019 min
Response: 513264
Conc: 4.98 ug/ml

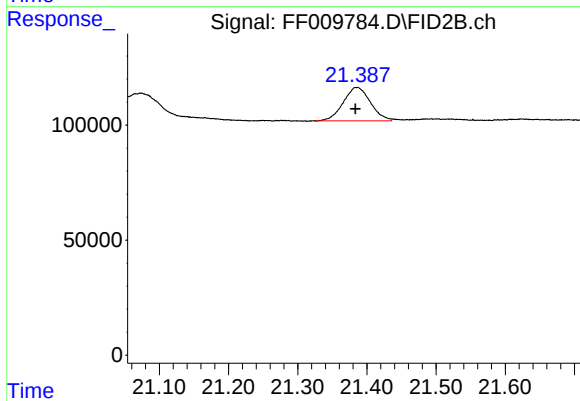

#18 N-TETRACONTANE

R.T.: 21.388 min
Delta R.T.: 0.004 min
Response: 398750
Conc: 4.39 ug/ml