

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012622\
 Data File : FF009796.D
 Signal(s) : FID2B.ch
 Acq On : 26 Jan 2022 17:49
 Operator : AJ\MA
 Sample : N1266-05
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 27 00:14:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.436	733181	5.611 ug/ml
Target Compounds			
4) N-TETRADECANE	8.016	59555	0.405 ug/ml
7) N-EICOSANE	12.411	326725	2.161 ug/ml
11) N-HEXACOSANE	15.686	85952	0.588 ug/ml
12) N-OCTACOSANE	16.601	92495	0.637 ug/ml
13) N-TRIACONTANE	17.484	86679	0.606 ug/ml
14) N-DOTRIACONTANE	18.344	448917	3.299 ug/ml
15) N-TETRATRIACONTANE	19.095	550094	4.631 ug/ml
16) N-HEXATRIACONTANE	19.875	450433	4.369 ug/ml
17) N-OCTATRIACONTANE	20.535	56581	0.635 ug/ml
18) N-TETRACONTANE	21.384	260293	2.865 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012622\
Data File : FF009796.D
Signal(s) : FID2B.ch
Acq On : 26 Jan 2022 17:49
Operator : AJ\MA
Sample : N1266-05
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 27 00:14:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

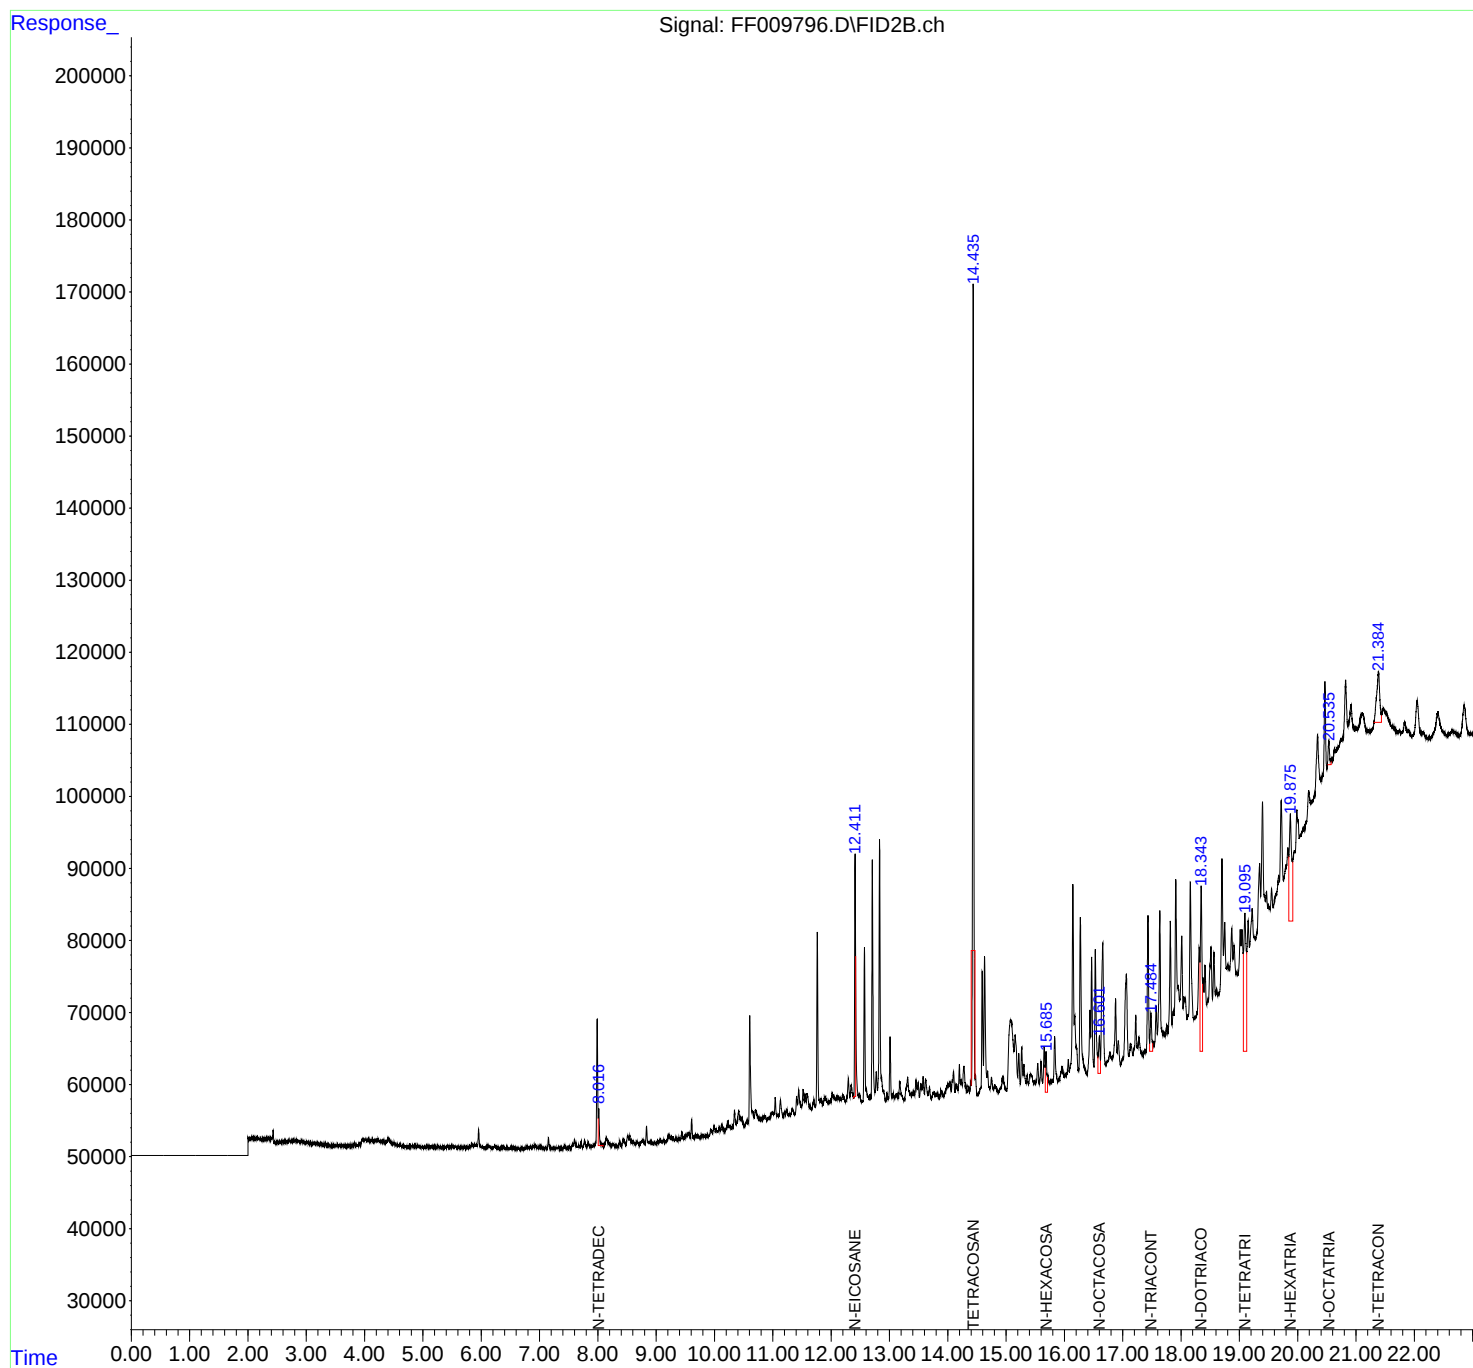


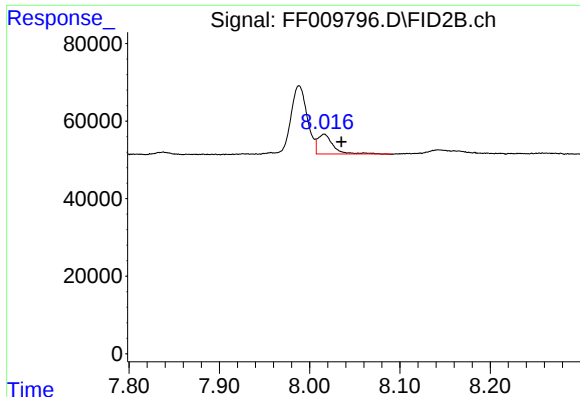

#4 N-TETRADECANE


R.T.: 8.016 min
Delta R.T.: -0.019 min
Response: 59555
Conc: 0.41 ug/ml

Instrument :
FID_F
ClientSampleId :

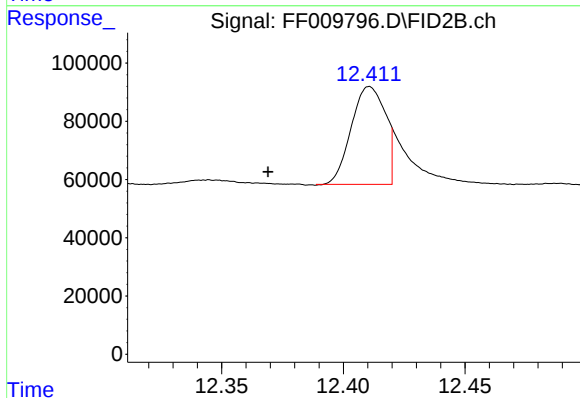


#7 N-EICOSANE

R.T.: 12.411 min
Delta R.T.: 0.042 min
Response: 326725
Conc: 2.16 ug/ml

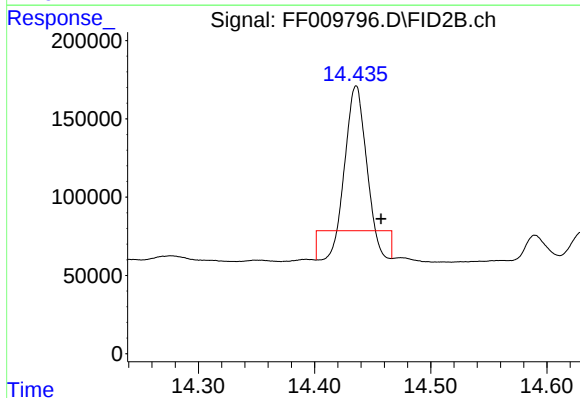


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.436 min
Delta R.T.: -0.021 min
Response: 733181
Conc: 5.61 ug/ml

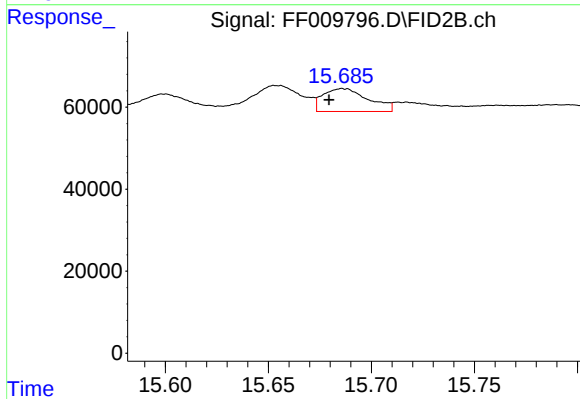

#11 N-HEXACOSANE


R.T.: 15.686 min
Delta R.T.: 0.006 min
Response: 85952
Conc: 0.59 ug/ml

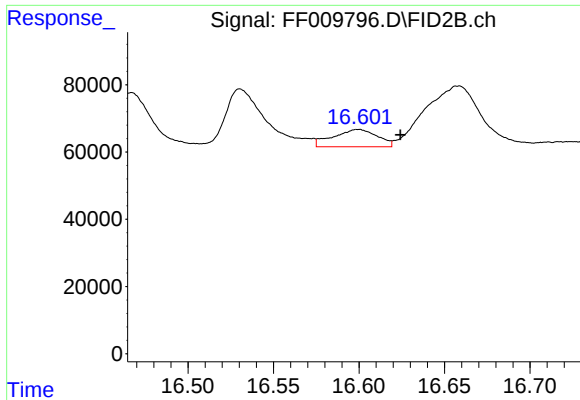

#12 N-OCTACOSANE


R.T.: 16.601 min
Delta R.T.: -0.024 min
Response: 92495
Conc: 0.64 ug/ml

Instrument :
FID_F
ClientSampleId :

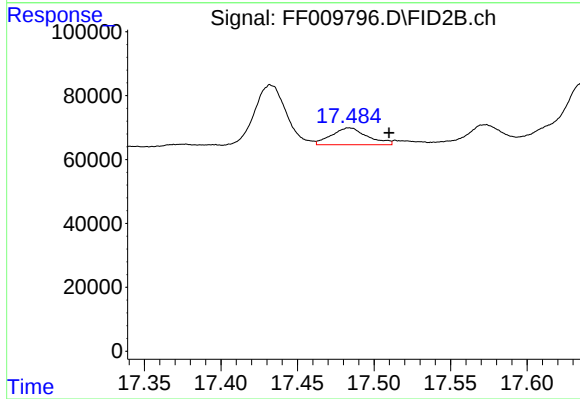


#13 N-TRIACONTANE

R.T.: 17.484 min
Delta R.T.: -0.026 min
Response: 86679
Conc: 0.61 ug/ml

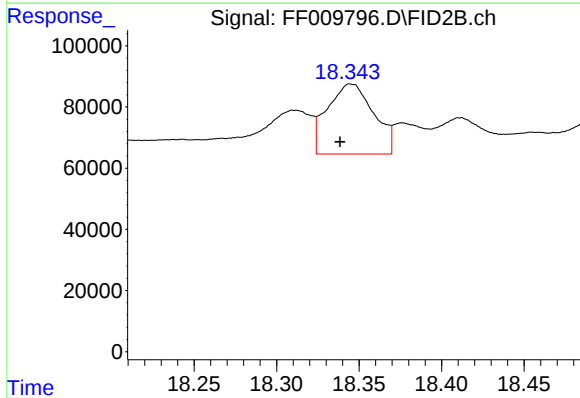


#14 N-DOTRIACONTANE

R.T.: 18.344 min
Delta R.T.: 0.006 min
Response: 448917
Conc: 3.30 ug/ml

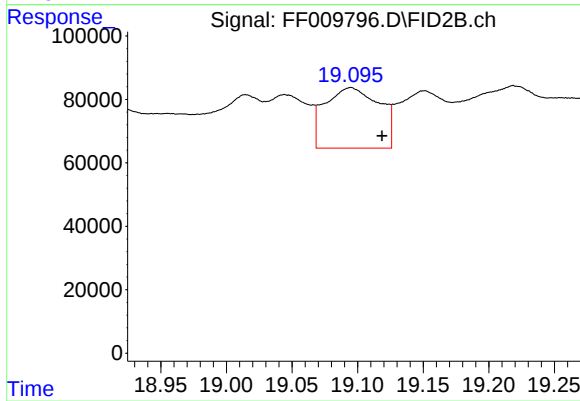

#15 N-TETRATRIACONTANE


R.T.: 19.095 min
Delta R.T.: -0.023 min
Response: 550094
Conc: 4.63 ug/ml

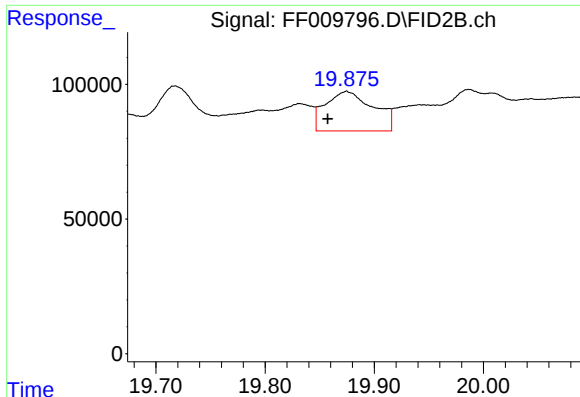

#16 N-HEXATRIACONTANE


R.T.: 19.875 min
Delta R.T.: 0.018 min
Response: 450433
Conc: 4.37 ug/ml

Instrument :
FID_F
ClientSampleId :

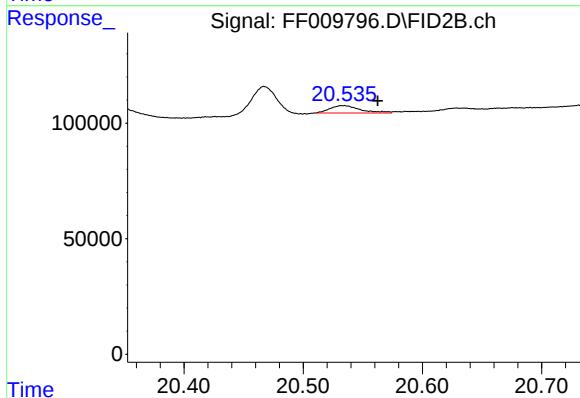

#17 N-OCTATRIACONTANE

R.T.: 20.535 min
Delta R.T.: -0.028 min
Response: 56581
Conc: 0.63 ug/ml

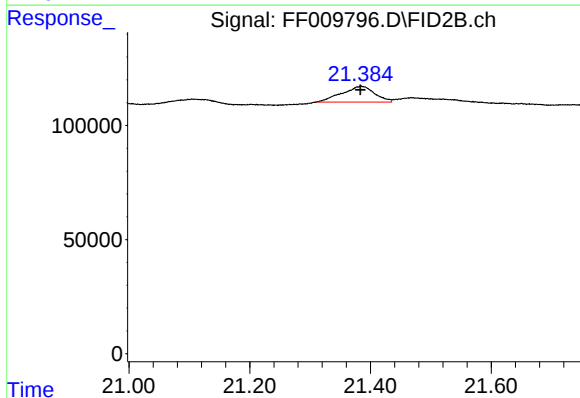

#18 N-TETRACONTANE

R.T.: 21.384 min
Delta R.T.: 0.001 min
Response: 260293
Conc: 2.87 ug/ml