

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012622\
 Data File : FF009797.D
 Signal(s) : FID2B.ch
 Acq On : 26 Jan 2022 18:18
 Operator : AJ\MA
 Sample : N1266-06
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 27 00:14:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.435	1741558	13.327 ug/ml
Target Compounds			
4) N-TETRADECANE	8.016	74646	0.508 ug/ml
6) N-OCTADECANE	11.127f	147311	0.956 ug/ml
7) N-EICOSANE	12.409	439947	2.910 ug/ml
10) N-TETRACOSANE	14.628	435874	2.939 ug/ml
11) N-HEXACOSANE	15.655	208306	1.425 ug/ml
12) N-OCTACOSANE	16.600	183293	1.263 ug/ml
13) N-TRIACONTANE	17.484	117780	0.823 ug/ml
14) N-DOTRIACONTANE	18.340	279727	2.056 ug/ml
15) N-TETRATRIACONTANE	19.093	509138	4.287 ug/ml
16) N-HEXATRIACONTANE	19.875	506292	4.911 ug/ml
18) N-TETRACONTANE	21.384	283838	3.125 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012622\
Data File : FF009797.D
Signal(s) : FID2B.ch
Acq On : 26 Jan 2022 18:18
Operator : AJ\MA
Sample : N1266-06
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 27 00:14:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

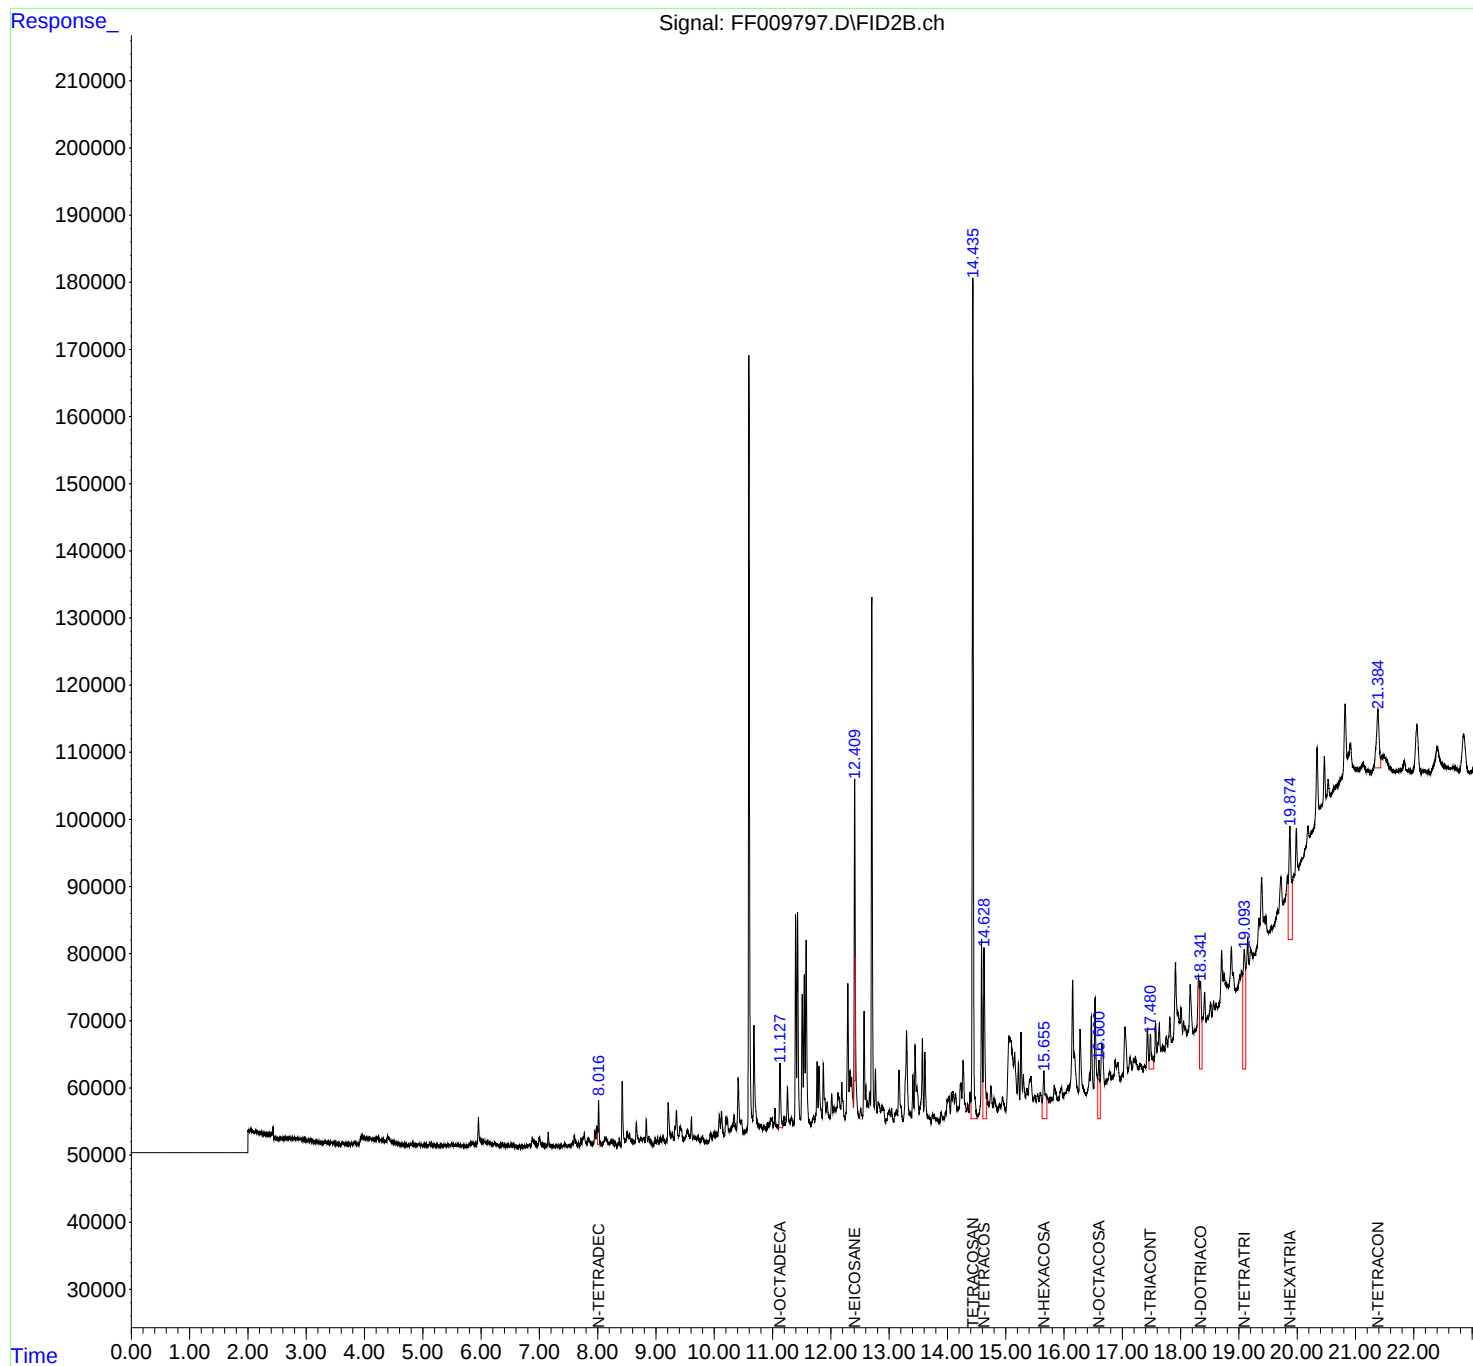


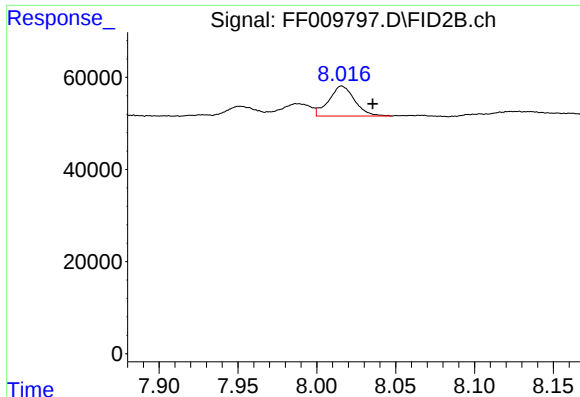

#4 N-TETRADECANE


R.T.: 8.016 min
Delta R.T.: -0.019 min
Response: 74646
Conc: 0.51 ug/ml

Instrument :
FID_F
ClientSampleId :

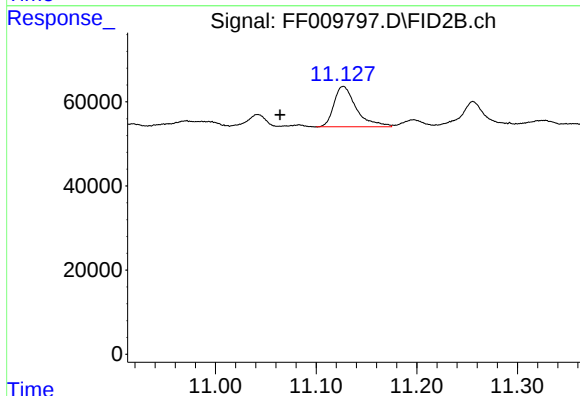


#6 N-OCTADECANE

R.T.: 11.127 min
Delta R.T.: 0.063 min
Response: 147311
Conc: 0.96 ug/ml

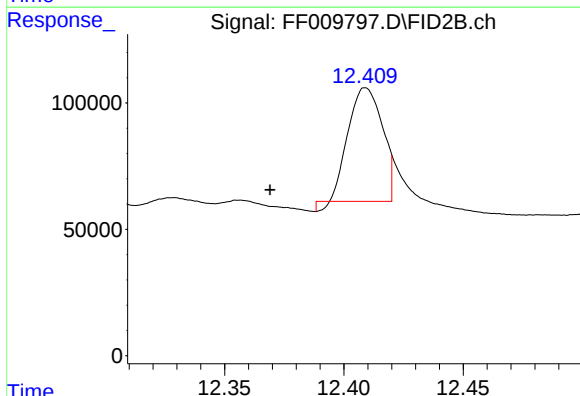


#7 N-EICOSANE

R.T.: 12.409 min
Delta R.T.: 0.040 min
Response: 439947
Conc: 2.91 ug/ml

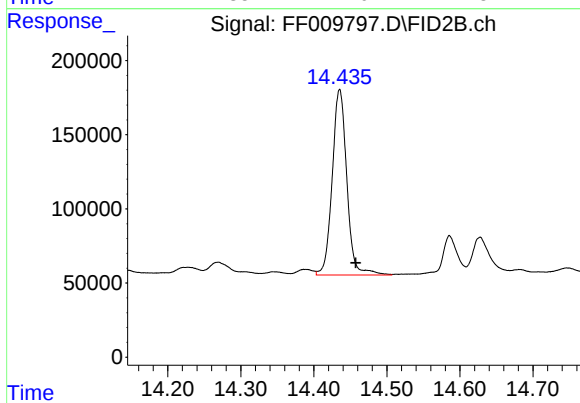

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.435 min
Delta R.T.: -0.022 min
Response: 1741558
Conc: 13.33 ug/ml

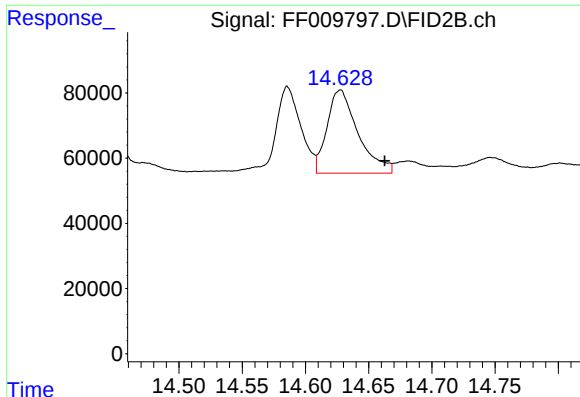

#10 N-TETRACOSANE


R.T.: 14.628 min
Delta R.T.: -0.035 min
Response: 435874
Conc: 2.94 ug/ml

Instrument :
FID_F
ClientSampleId :

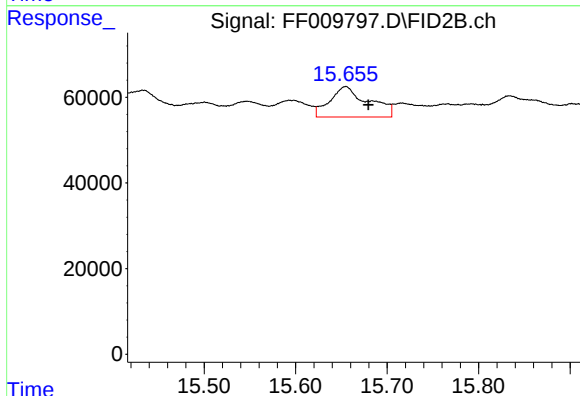


#11 N-HEXACOSANE

R.T.: 15.655 min
Delta R.T.: -0.025 min
Response: 208306
Conc: 1.42 ug/ml

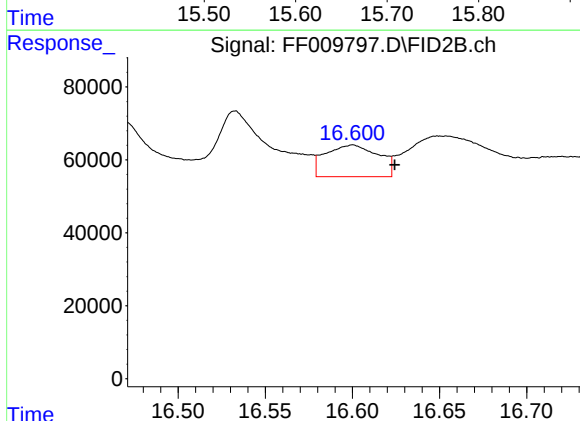


#12 N-OCTACOSANE

R.T.: 16.600 min
Delta R.T.: -0.024 min
Response: 183293
Conc: 1.26 ug/ml

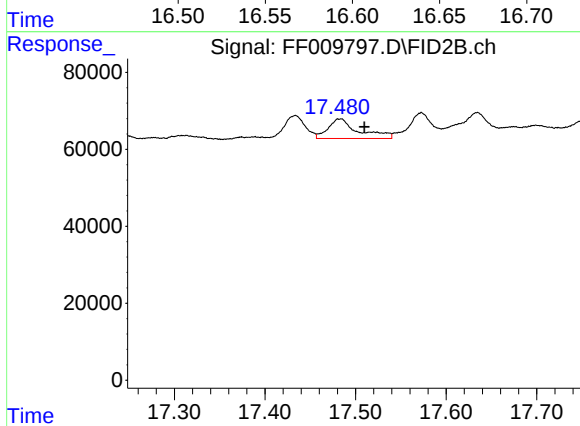

#13 N-TRIACONTANE


R.T.: 17.484 min
Delta R.T.: -0.026 min
Response: 117780
Conc: 0.82 ug/ml

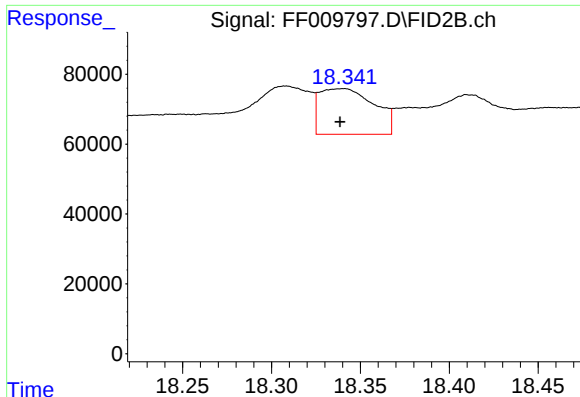

#14 N-DOTRIACONTANE


R.T.: 18.340 min
Delta R.T.: 0.002 min
Response: 279727
Conc: 2.06 ug/ml

Instrument :
FID_F
ClientSampleId :

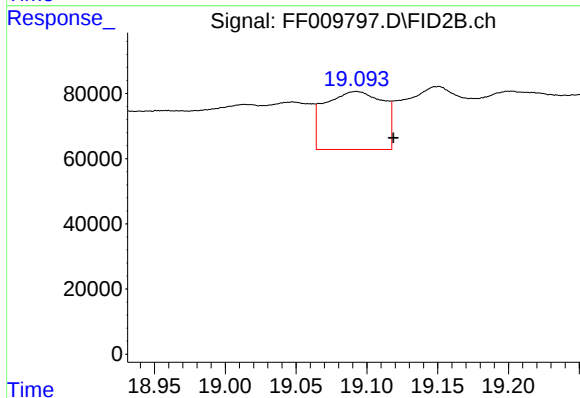


#15 N-TETRATRIACONTANE

R.T.: 19.093 min
Delta R.T.: -0.026 min
Response: 509138
Conc: 4.29 ug/ml

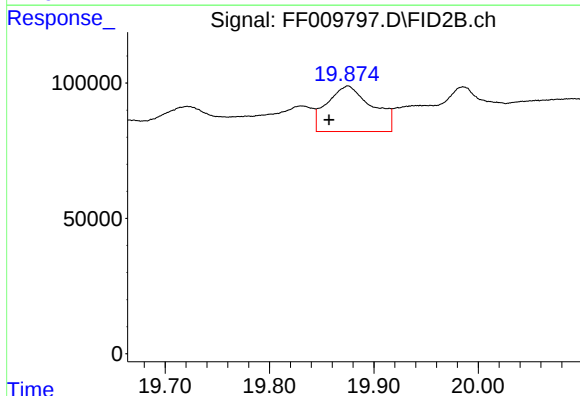

#16 N-HEXATRIACONTANE

R.T.: 19.875 min
Delta R.T.: 0.018 min
Response: 506292
Conc: 4.91 ug/ml

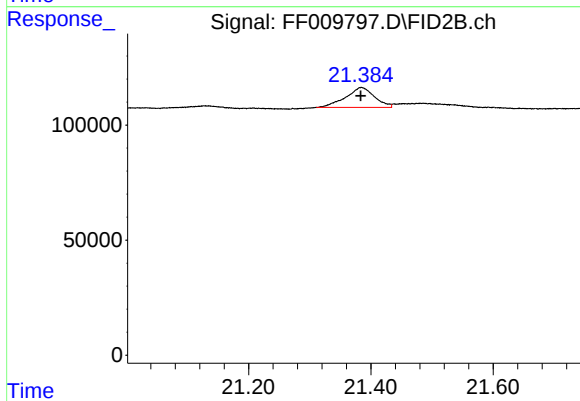

#18 N-TETRACONTANE

R.T.: 21.384 min
Delta R.T.: 0.001 min
Response: 283838
Conc: 3.12 ug/ml