

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012622\
 Data File : FF009798.D
 Signal(s) : FID2B.ch
 Acq On : 26 Jan 2022 18:47
 Operator : AJ\MA
 Sample : N1266-07
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 27 00:15:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.435	2214302	16.945 ug/ml
Target Compounds			
4) N-TETRADECANE	8.016	97139	0.661 ug/ml
5) N-HEXADECANE	9.631	173437	1.159 ug/ml
6) N-OCTADECANE	11.041	84555	0.548 ug/ml
10) N-TETRACOSANE	14.620	1268741	8.555 ug/ml
11) N-HEXACOSANE	15.654	169328	1.158 ug/ml
12) N-OCTACOSANE	16.636	303387	2.090 ug/ml
13) N-TRIACONTANE	17.486	554435	3.875 ug/ml
14) N-DOTRIACONTANE	18.304	1831518	13.459 ug/ml
15) N-TETRATRIACONTANE	19.095	1582649	13.325 ug/ml
16) N-HEXATRIACONTANE	19.875	309562	3.002 ug/ml
18) N-TETRACONTANE	21.390	98061	1.080 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012622\
Data File : FF009798.D
Signal(s) : FID2B.ch
Acq On : 26 Jan 2022 18:47
Operator : AJ\MA
Sample : N1266-07
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 27 00:15:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

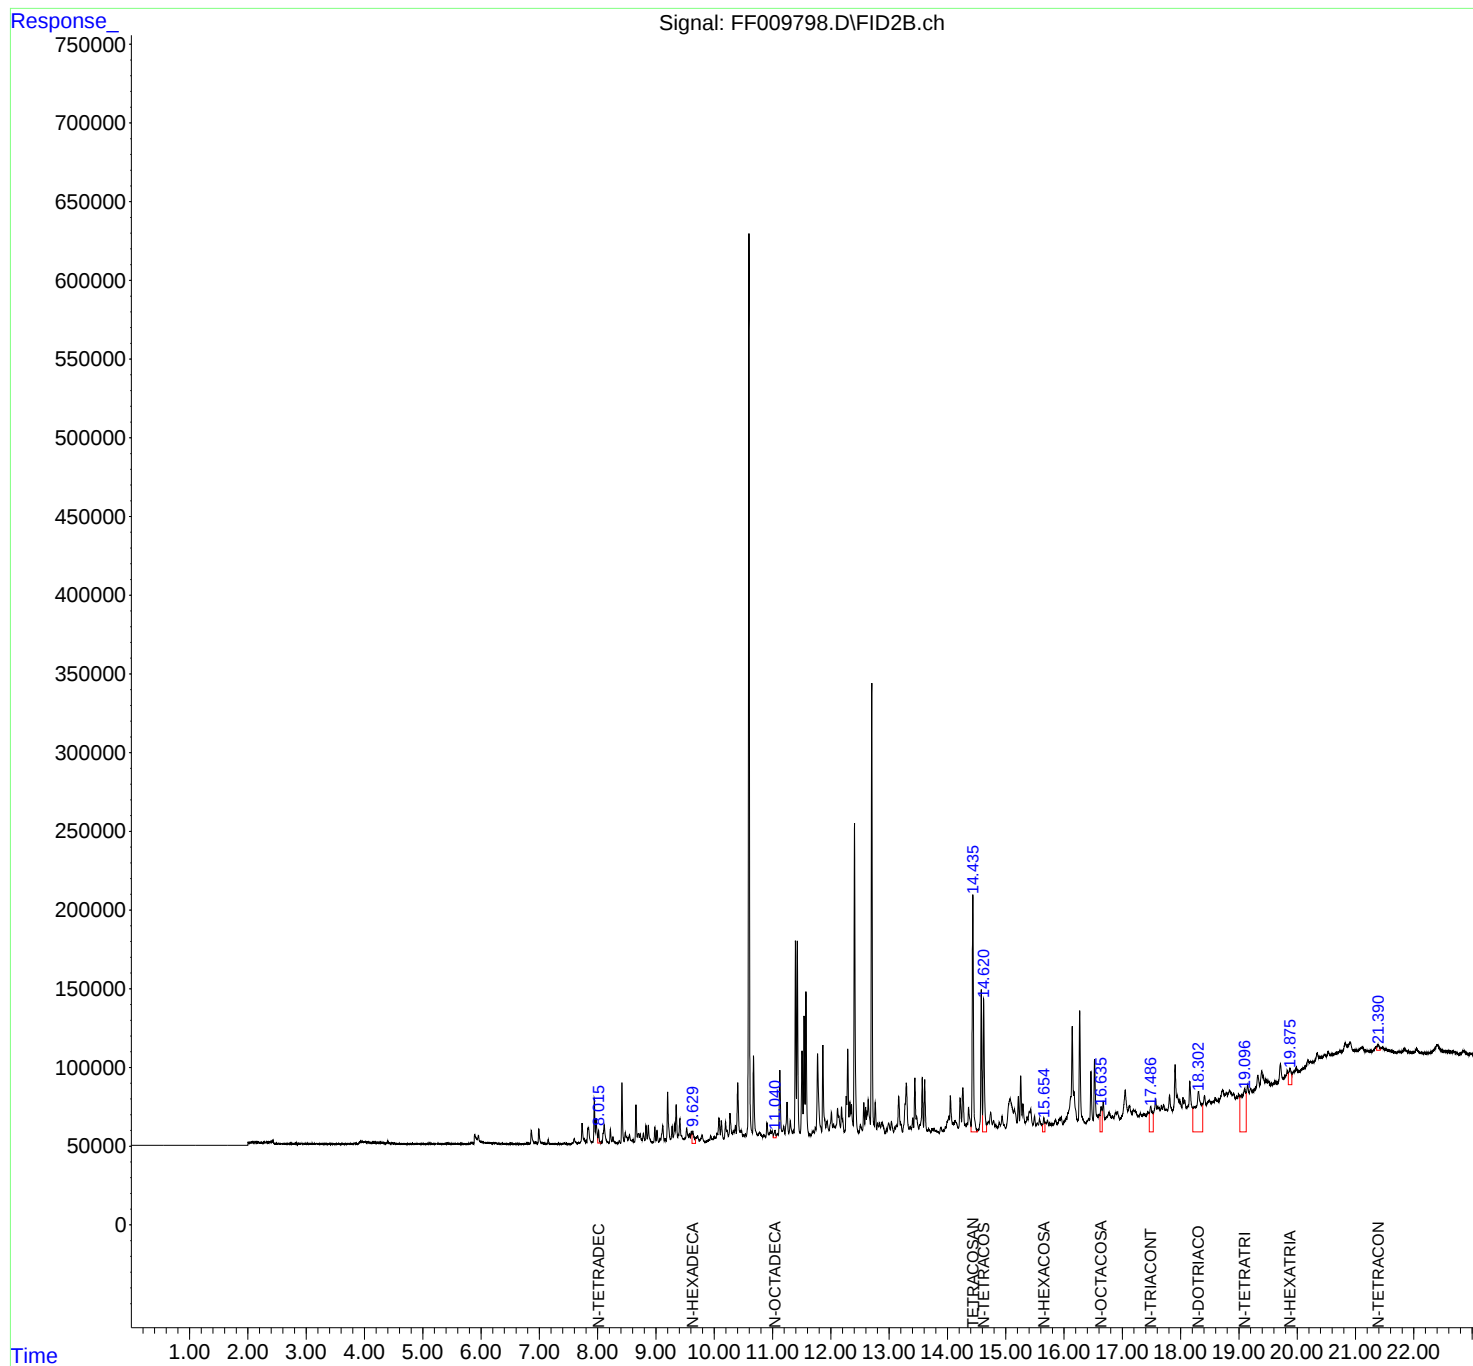


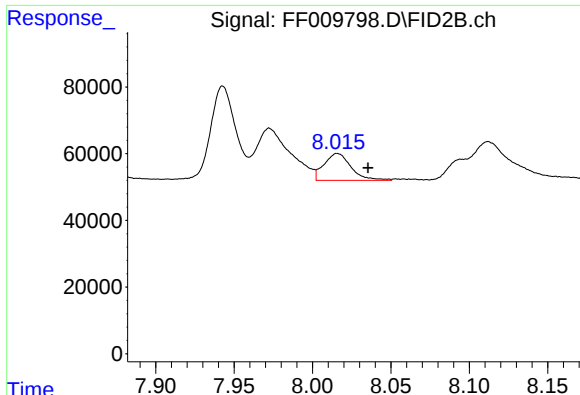

#4 N-TETRADECANE


R.T.: 8.016 min
Delta R.T.: -0.020 min
Response: 97139
Conc: 0.66 ug/ml

Instrument :
FID_F
ClientSampleId :

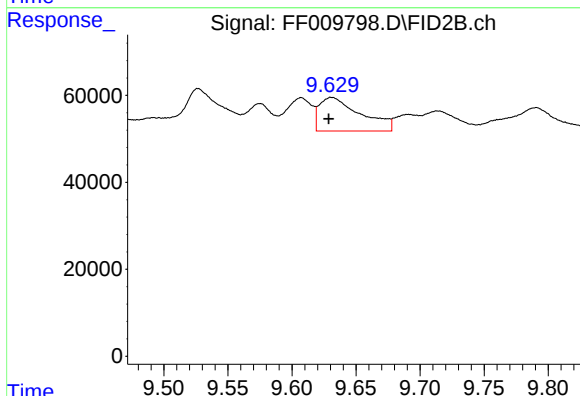


#5 N-HEXADECANE

R.T.: 9.631 min
Delta R.T.: 0.002 min
Response: 173437
Conc: 1.16 ug/ml

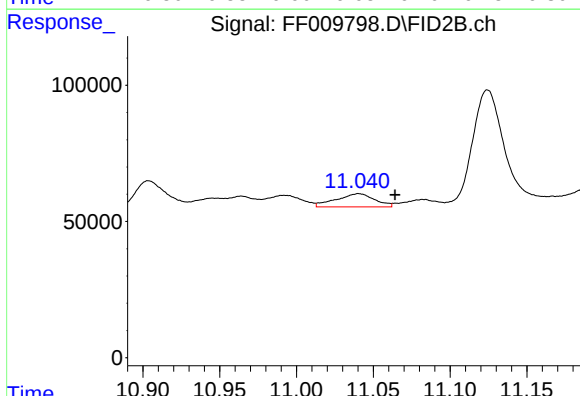


#6 N-OCTADECANE

R.T.: 11.041 min
Delta R.T.: -0.024 min
Response: 84555
Conc: 0.55 ug/ml

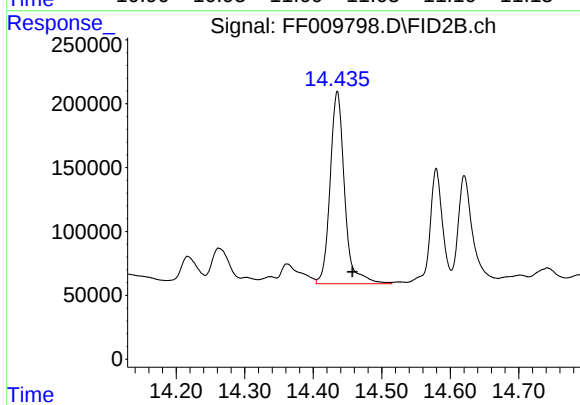

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.435 min
Delta R.T.: -0.022 min
Response: 2214302
Conc: 16.94 ug/ml

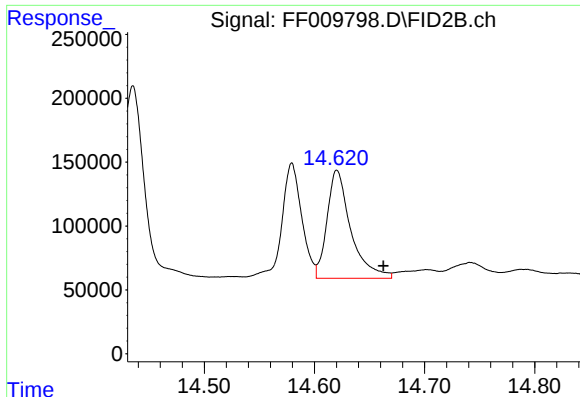

#10 N-TETRACOSANE


R.T.: 14.620 min
Delta R.T.: -0.042 min
Response: 1268741
Conc: 8.56 ug/ml

Instrument :
FID_F
ClientSampleId :

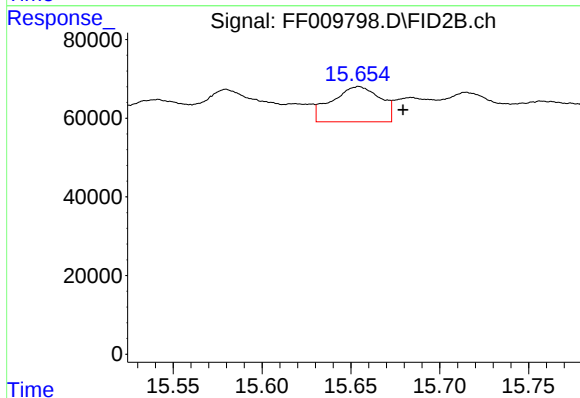


#11 N-HEXACOSANE

R.T.: 15.654 min
Delta R.T.: -0.025 min
Response: 169328
Conc: 1.16 ug/ml

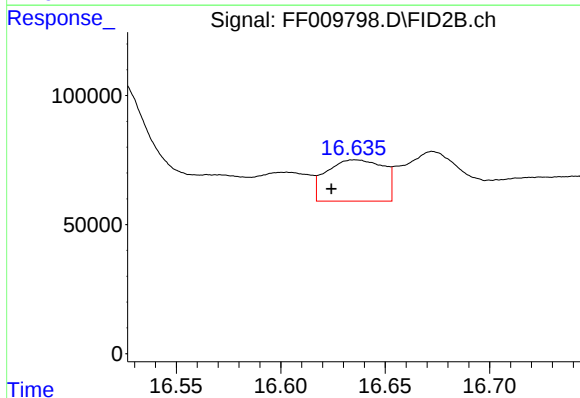


#12 N-OCTACOSANE

R.T.: 16.636 min
Delta R.T.: 0.011 min
Response: 303387
Conc: 2.09 ug/ml

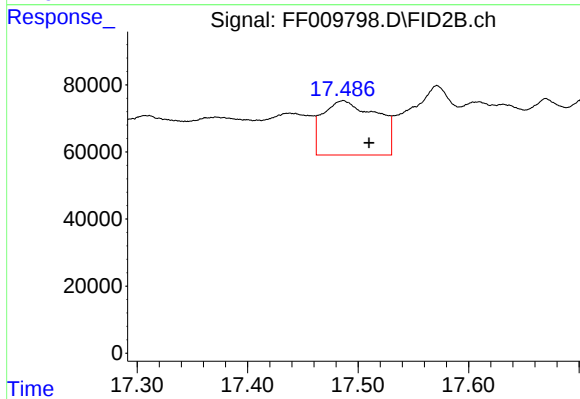

#13 N-TRIACONTANE


R.T.: 17.486 min
Delta R.T.: -0.023 min
Response: 554435
Conc: 3.87 ug/ml

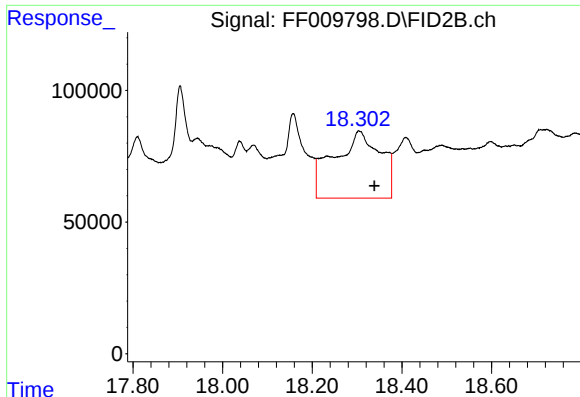

#14 N-DOTRIACONTANE


R.T.: 18.304 min
Delta R.T.: -0.035 min
Response: 1831518
Conc: 13.46 ug/ml

Instrument :
FID_F
ClientSampleId :

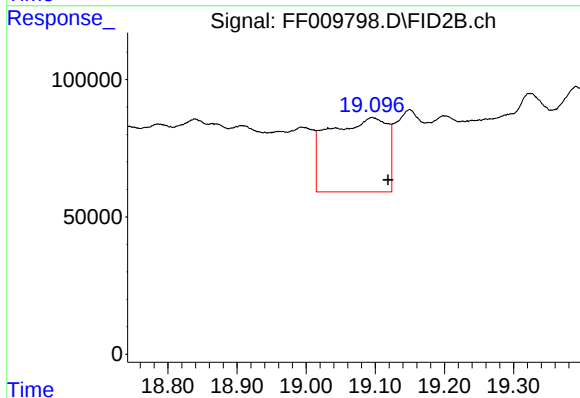


#15 N-TETRATRIACONTANE

R.T.: 19.095 min
Delta R.T.: -0.023 min
Response: 1582649
Conc: 13.32 ug/ml

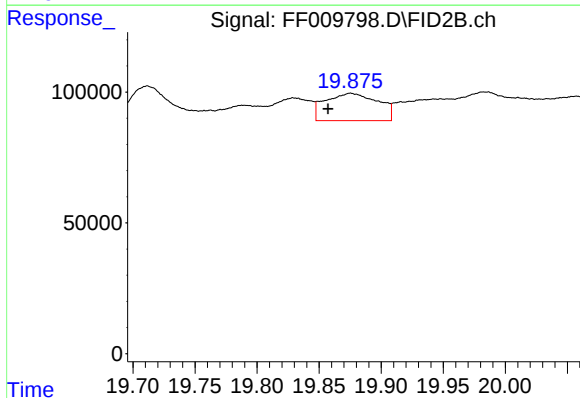

#16 N-HEXATRIACONTANE

R.T.: 19.875 min
Delta R.T.: 0.018 min
Response: 309562
Conc: 3.00 ug/ml

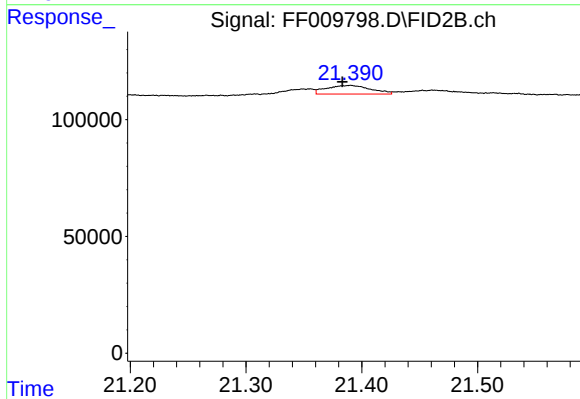

#18 N-TETRACONTANE

R.T.: 21.390 min
Delta R.T.: 0.007 min
Response: 98061
Conc: 1.08 ug/ml