

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012622\
 Data File : FF009799.D
 Signal(s) : FID2B.ch
 Acq On : 26 Jan 2022 19:16
 Operator : AJ\MA
 Sample : N1266-08
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 27 00:15:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.434	1117640	8.553 ug/ml
Target Compounds			
4) N-TETRADECANE	8.017	108652	0.739 ug/ml
6) N-OCTADECANE	11.040	39122	0.254 ug/ml
7) N-EICOSANE	12.408	417070	2.759 ug/ml
10) N-TETRACOSANE	14.622	76933	0.519 ug/ml
13) N-TRIACONTANE	17.484	125218	0.875 ug/ml
14) N-DOTRIACONTANE	18.306	712429	5.235 ug/ml
15) N-TETRATRIACONTANE	19.093	421219	3.546 ug/ml
16) N-HEXATRIACONTANE	19.875	667171	6.471 ug/ml
18) N-TETRACONTANE	21.381	252086	2.775 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012622\
Data File : FF009799.D
Signal(s) : FID2B.ch
Acq On : 26 Jan 2022 19:16
Operator : AJ\MA
Sample : N1266-08
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 27 00:15:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

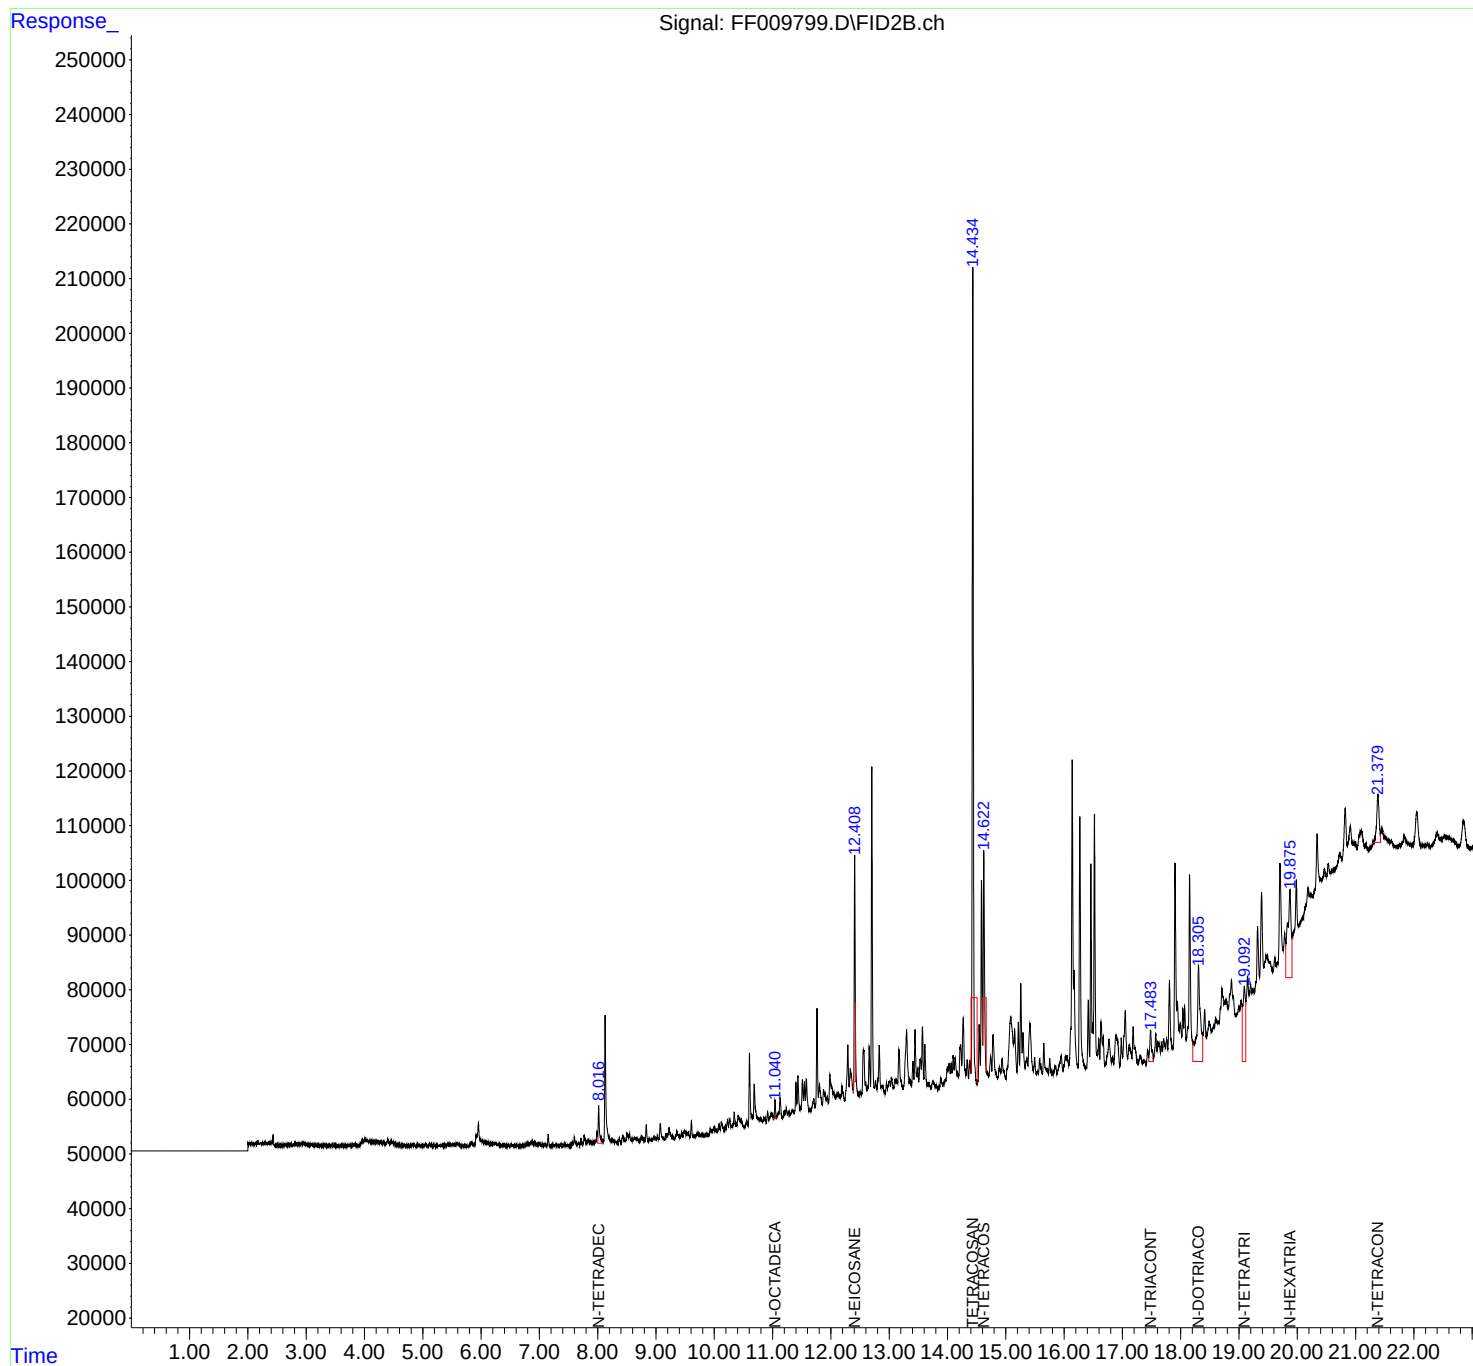


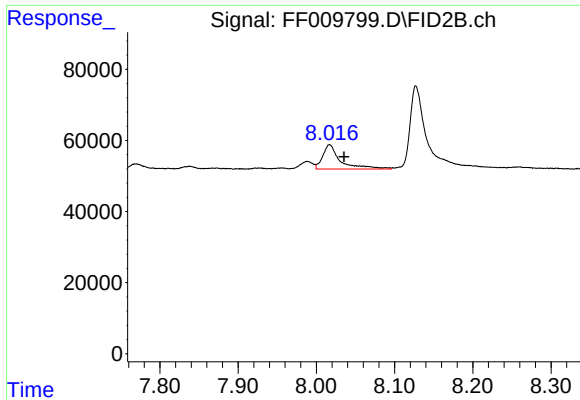

#4 N-TETRADECANE


R.T.: 8.017 min
Delta R.T.: -0.019 min
Response: 108652
Conc: 0.74 ug/ml

Instrument :
FID_F
ClientSampleId :

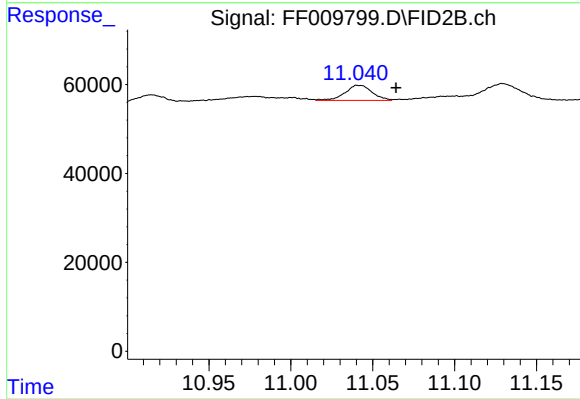


#6 N-OCTADECANE

R.T.: 11.040 min
Delta R.T.: -0.024 min
Response: 39122
Conc: 0.25 ug/ml

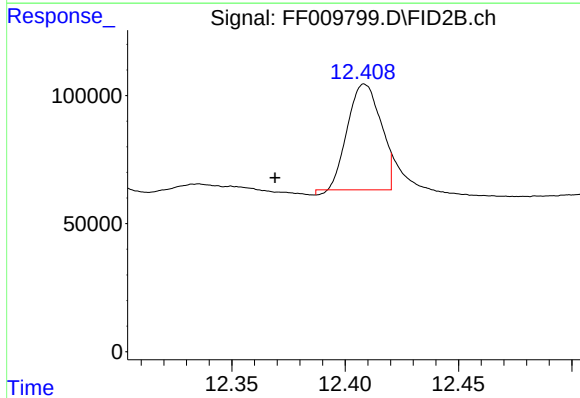


#7 N-EICOSANE

R.T.: 12.408 min
Delta R.T.: 0.039 min
Response: 417070
Conc: 2.76 ug/ml

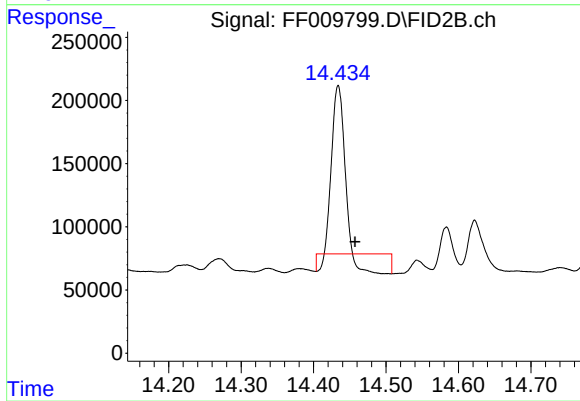

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.434 min
Delta R.T.: -0.023 min
Response: 1117640
Conc: 8.55 ug/ml

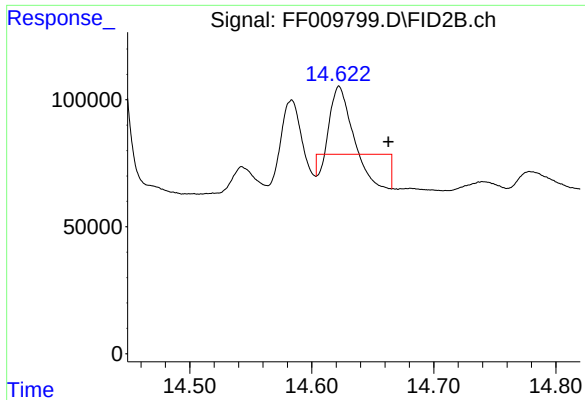

#10 N-TETRACOSANE


R.T.: 14.622 min
Delta R.T.: -0.040 min
Response: 76933
Conc: 0.52 ug/ml

Instrument :
FID_F
ClientSampleId :

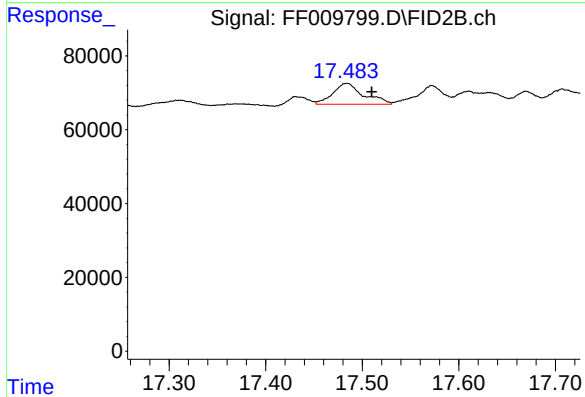


#13 N-TRIACONTANE

R.T.: 17.484 min
Delta R.T.: -0.026 min
Response: 125218
Conc: 0.88 ug/ml

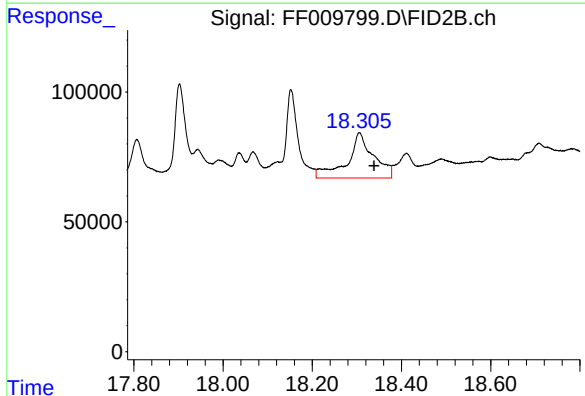


#14 N-DOTRIACONTANE

R.T.: 18.306 min
Delta R.T.: -0.033 min
Response: 712429
Conc: 5.24 ug/ml

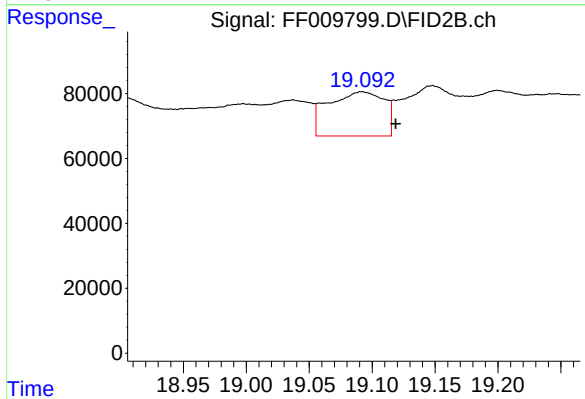

#15 N-TETRATRIACONTANE


R.T.: 19.093 min
Delta R.T.: -0.026 min
Response: 421219
Conc: 3.55 ug/ml

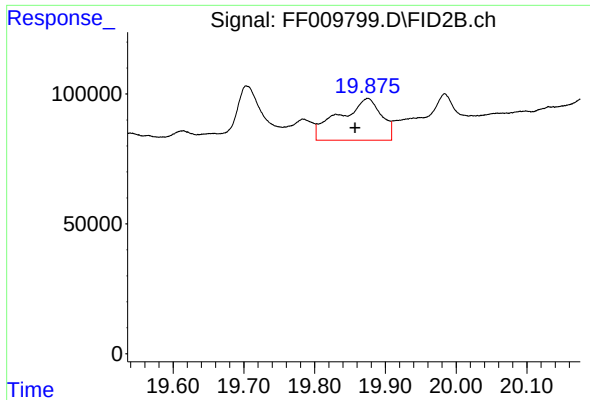

#16 N-HEXATRIACONTANE

R.T.: 19.875 min
Delta R.T.: 0.018 min
Response: 667171
Conc: 6.47 ug/ml

Instrument :
FID_F
ClientSampleId :

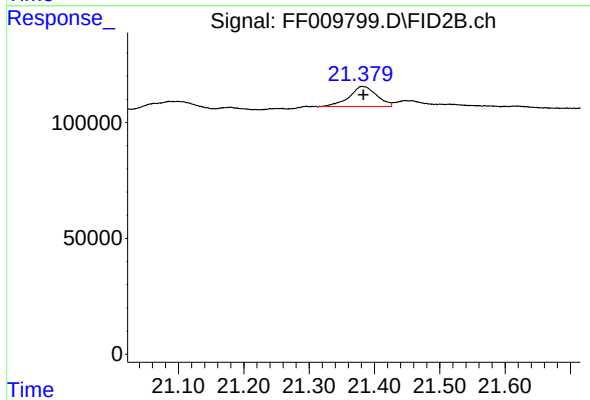

#18 N-TETRACONTANE

R.T.: 21.381 min
Delta R.T.: -0.002 min
Response: 252086
Conc: 2.78 ug/ml