

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012720\
 Data File : FF006310.D
 Signal(s) : FID2B.ch
 Acq On : 27 Jan 2020 16:40
 Operator : DD\AJ
 Sample : L1269-05
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 28 03:06:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.636	2315337	21.367 ug/ml
Target Compounds			
4) N-TETRADECANE	8.258f	1473947	11.677 ug/ml
5) N-HEXADECANE	9.820	139397	1.091 ug/ml
8) N-DOCOSANE	13.737	99279	0.787 ug/ml
11) N-HEXACOSANE	15.856	134949	1.098 ug/ml
12) N-OCTACOSANE	16.804	584912	4.812 ug/ml
13) N-TRIACONTANE	17.688	484656	4.042 ug/ml
14) N-DOTRIACONTANE	18.517	870600	7.533 ug/ml
15) N-TETRATRIACONTANE	19.261	236630	2.100 ug/ml
16) N-HEXATRIACONTANE	20.028	891022	8.333 ug/ml
17) N-OCTATRIACONTANE	20.734	1680217	18.161 ug/ml
18) N-TETRACONTANE	21.645	462989	4.598 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012720\
Data File : FF006310.D
Signal(s) : FID2B.ch
Acq On : 27 Jan 2020 16:40
Operator : DD\AJ
Sample : L1269-05
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 28 03:06:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

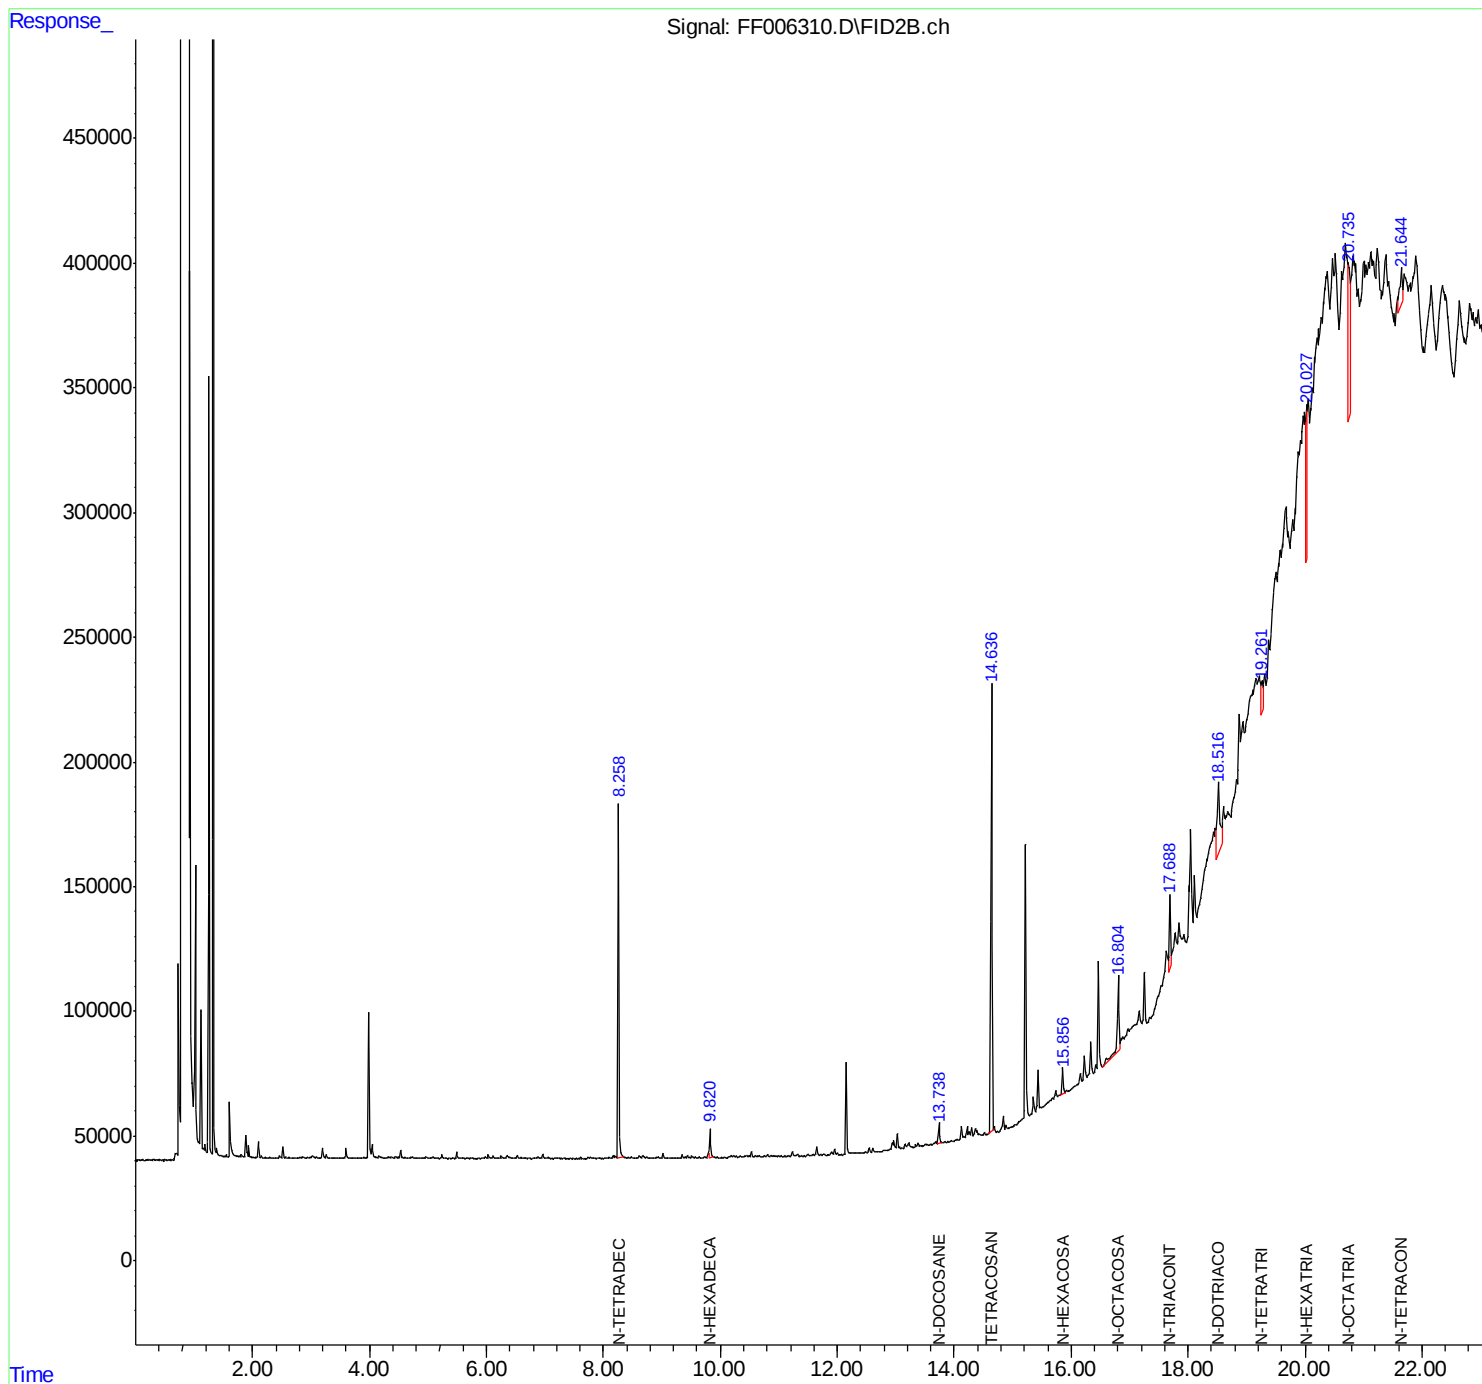

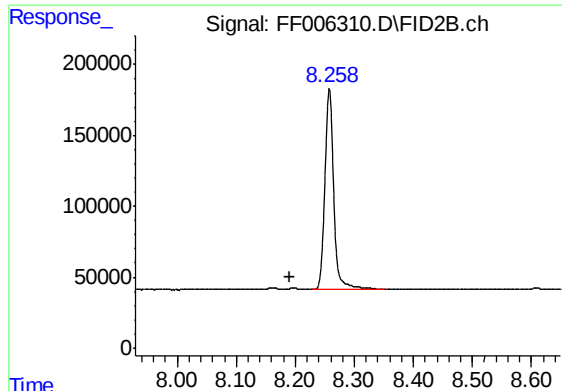


#4 N-TETRADECANE

R.T.: 8.258 min
Delta R.T.: 0.068 min
Response: 1473947
Conc: 11.68 ug/ml

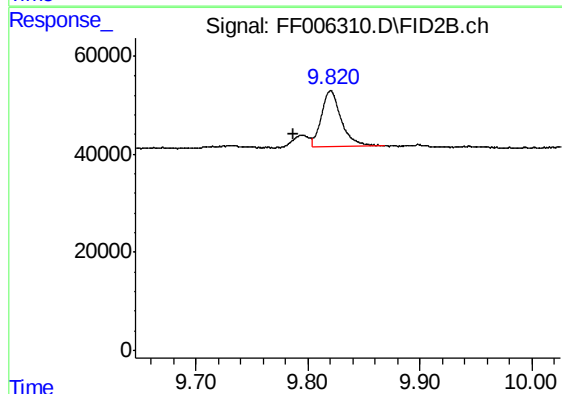


#5 N-HEXADECANE

R.T.: 9.820 min
Delta R.T.: 0.034 min
Response: 139397
Conc: 1.09 ug/ml

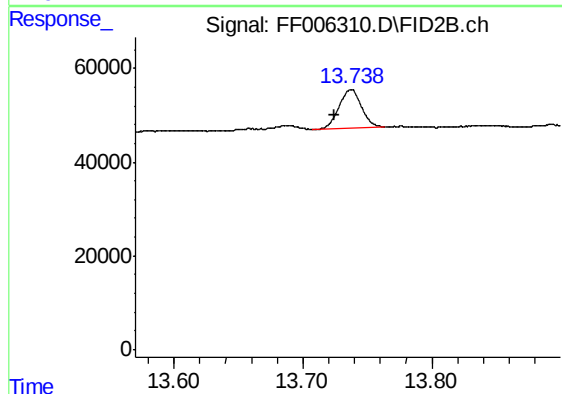


#8 N-DOCOSANE

R.T.: 13.737 min
Delta R.T.: 0.013 min
Response: 99279
Conc: 0.79 ug/ml

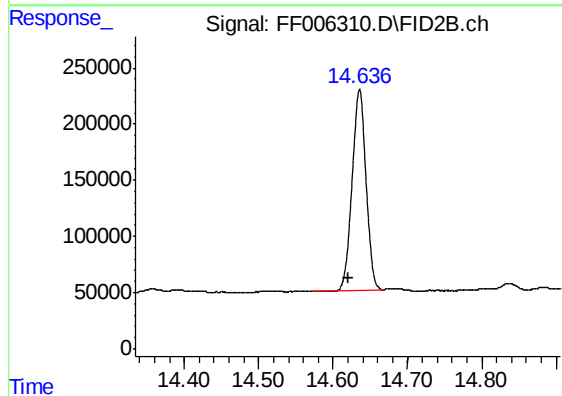


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.636 min
Delta R.T.: 0.016 min
Response: 2315337
Conc: 21.37 ug/ml

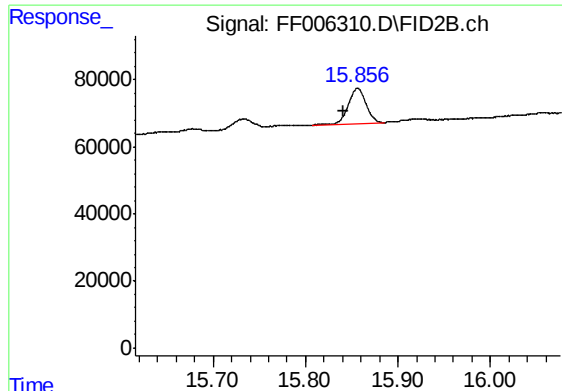


#11 N-HEXACOSANE

R.T.: 15.856 min
Delta R.T.: 0.015 min
Response: 134949
Conc: 1.10 ug/ml

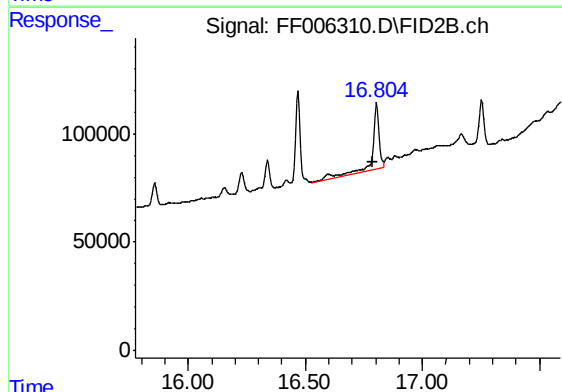


#12 N-OCTACOSANE

R.T.: 16.804 min
Delta R.T.: 0.017 min
Response: 584912
Conc: 4.81 ug/ml

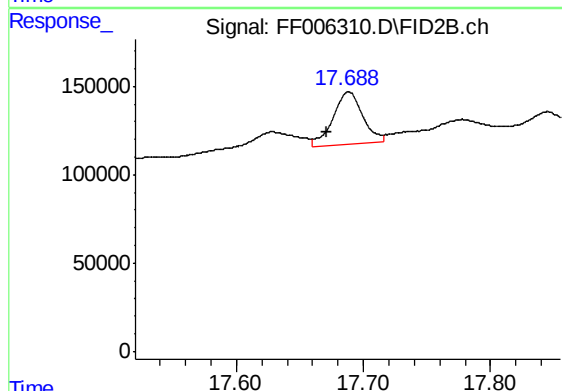


#13 N-TRIACONTANE

R.T.: 17.688 min
Delta R.T.: 0.017 min
Response: 484656
Conc: 4.04 ug/ml

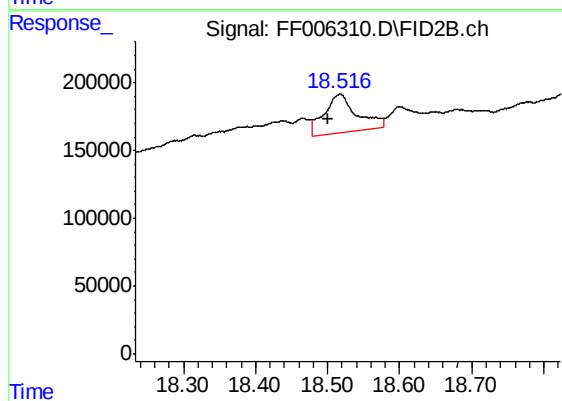


#14 N-DOTRIACONTANE

R.T.: 18.517 min
Delta R.T.: 0.016 min
Response: 870600
Conc: 7.53 ug/ml

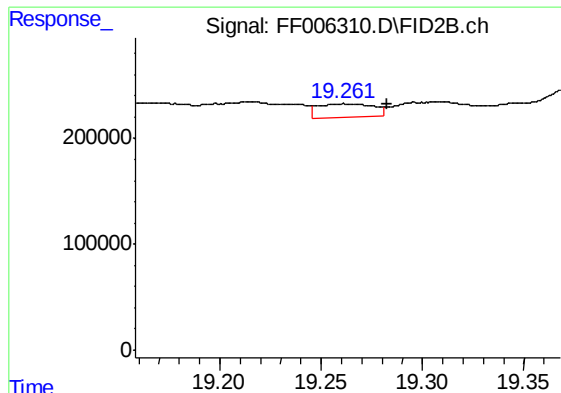


#15 N-TETRATRIACONTANE

R.T.: 19.261 min
Delta R.T.: -0.022 min
Response: 236630
Conc: 2.10 ug/ml

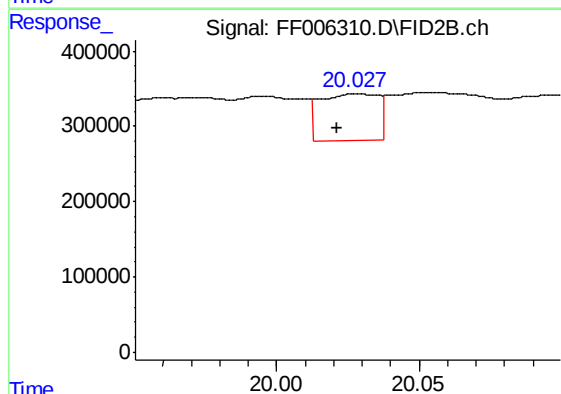


#16 N-HEXATRIACONTANE

R.T.: 20.028 min
Delta R.T.: 0.007 min
Response: 891022
Conc: 8.33 ug/ml

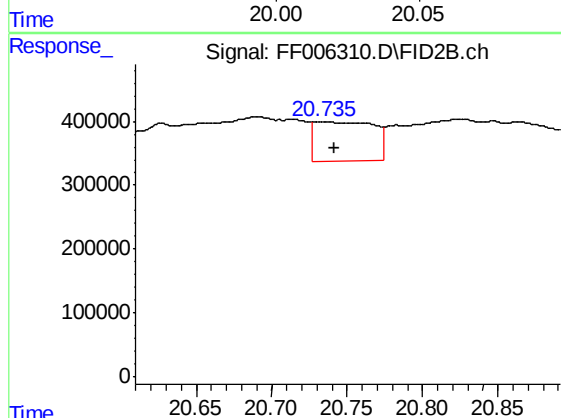

#17 N-OCTATRIACONTANE

R.T.: 20.734 min
Delta R.T.: -0.007 min
Response: 1680217
Conc: 18.16 ug/ml

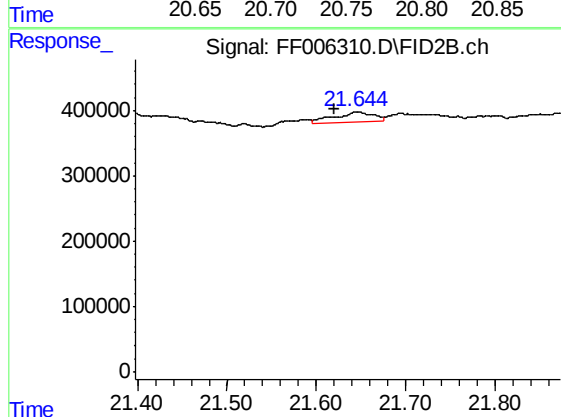

#18 N-TETRACONTANE

R.T.: 21.645 min
Delta R.T.: 0.025 min
Response: 462989
Conc: 4.60 ug/ml