

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012723\
 Data File : FF011936.D
 Signal(s) : FID2B.ch
 Acq On : 27 Jan 2023 11:02
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 27 15:44:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
 Quant Title :
 QLast Update : Fri Jan 27 14:21:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
12) N-OCTACOSANE	17.220	54709	0.421 ug/ml
13) N-TRIACONTANE	18.107	110200	0.854 ug/ml
14) N-DOTRIACONTANE	18.939	76718	0.589 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012723\
 Data File : FF011936.D
 Signal(s) : FID2B.ch
 Acq On : 27 Jan 2023 11:02
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 27 15:44:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
 Quant Title :
 QLast Update : Fri Jan 27 14:21:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

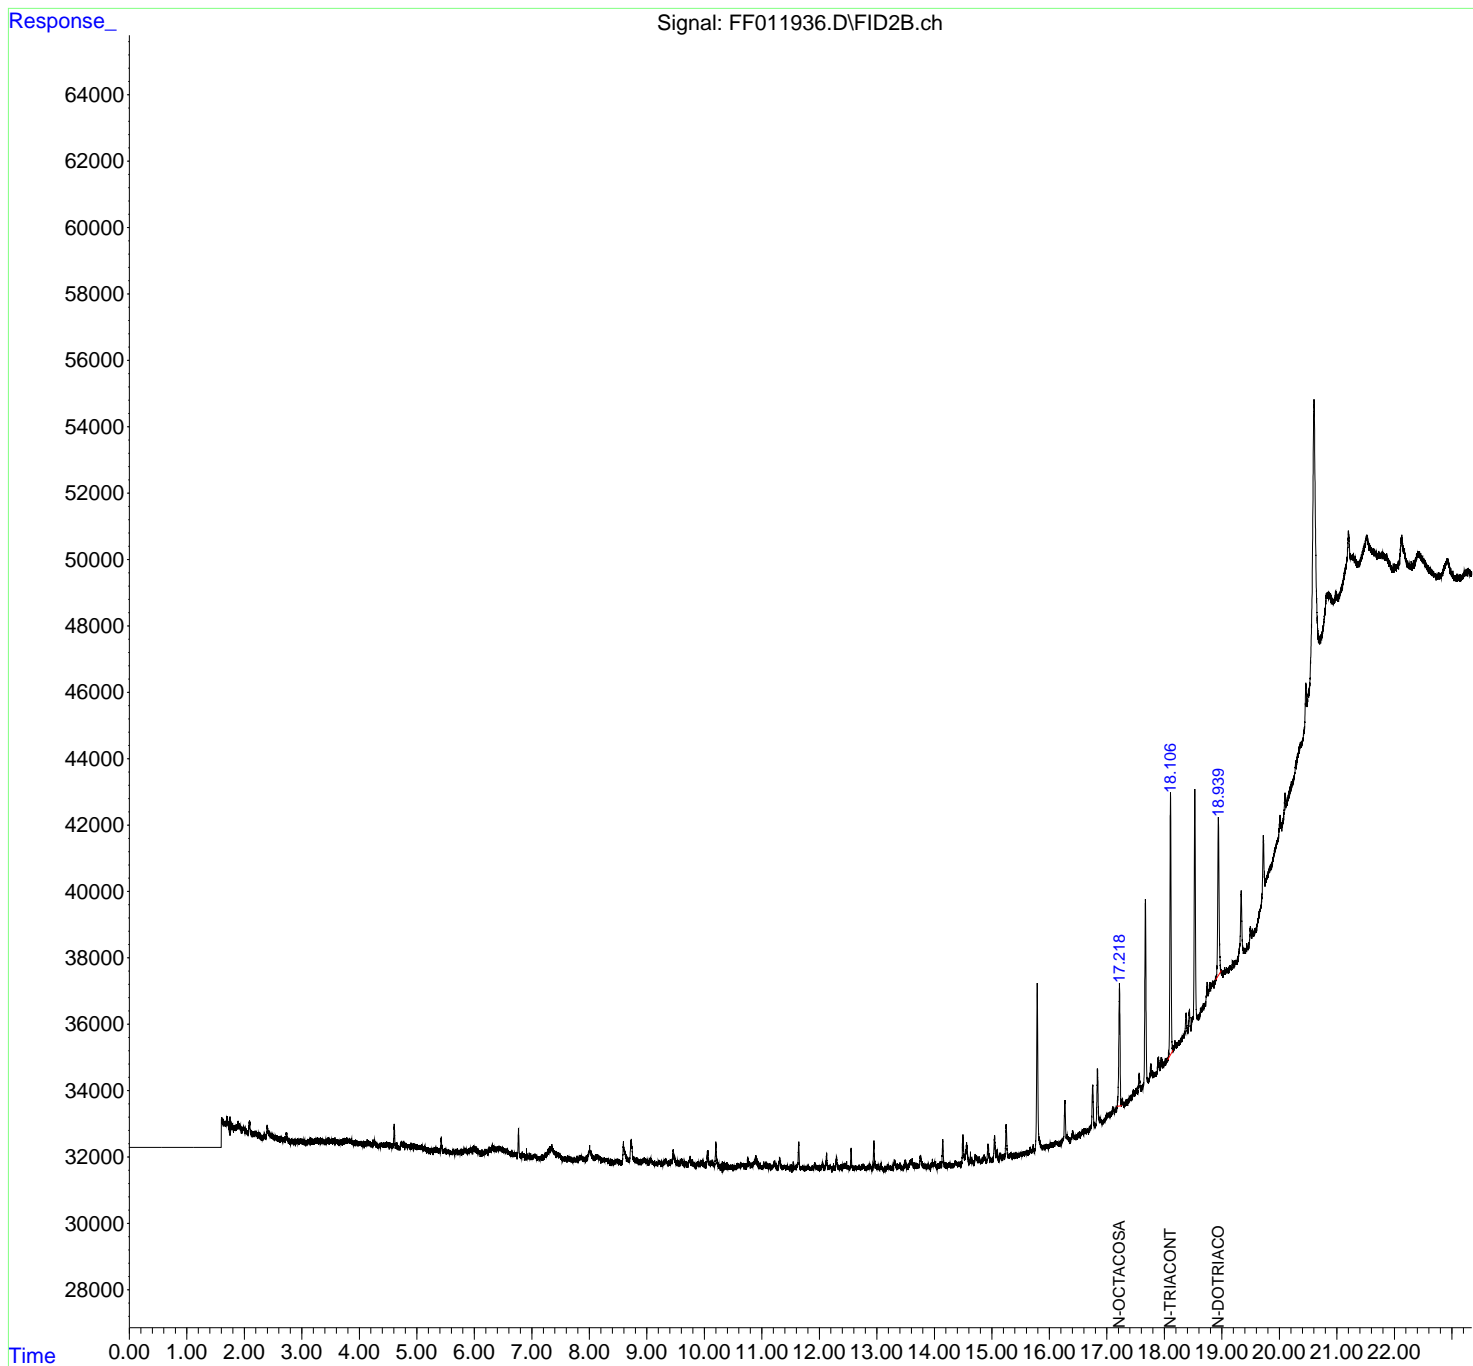


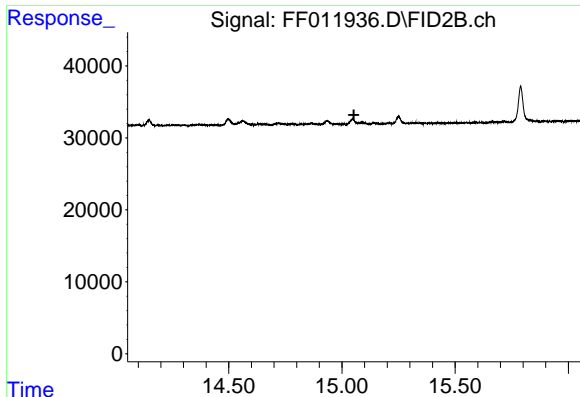

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
 Exp R.T.: 15.053 min
 Response: 0
 Conc: N.D.

Instrument :
 FID_F
 ClientSampleId :

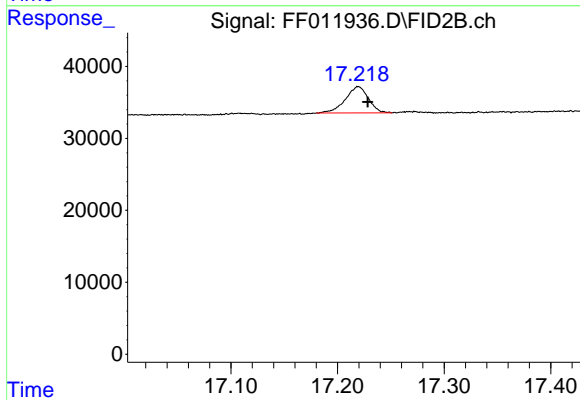


#12 N-OCTACOSANE

R.T.: 17.220 min
 Delta R.T.: -0.009 min
 Response: 54709
 Conc: 0.42 ug/ml

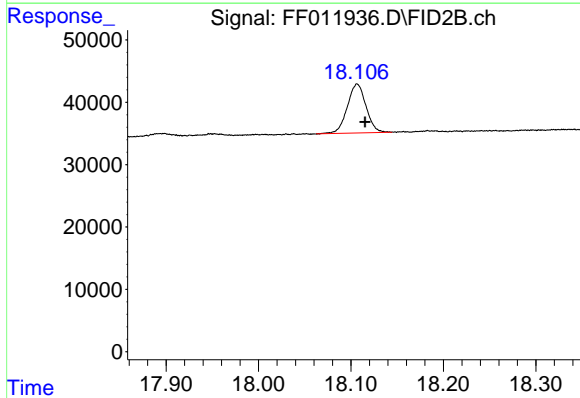

#13 N-TRIACONTANE

R.T.: 18.107 min
 Delta R.T.: -0.008 min
 Response: 110200
 Conc: 0.85 ug/ml

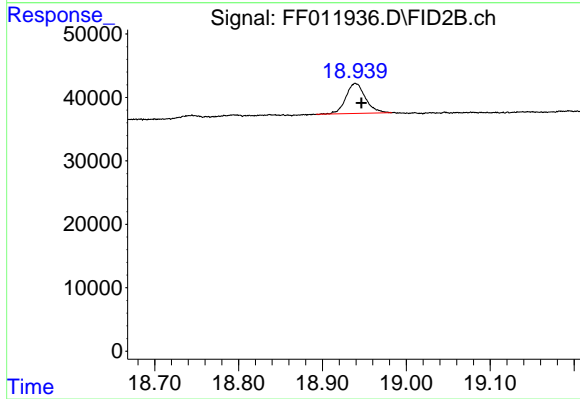

#14 N-DOTRIACONTANE

R.T.: 18.939 min
 Delta R.T.: -0.007 min
 Response: 76718
 Conc: 0.59 ug/ml