

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012723\
Data File : FF011937.D
Signal(s) : FID2B.ch
Acq On : 27 Jan 2023 11:31
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 27 15:44:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.047	2043996	17.738 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.106	85989	0.666 ug/ml
14) N-DOTRIACONTANE	18.941	78829	0.606 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012723\
Data File : FF011937.D
Signal(s) : FID2B.ch
Acq On : 27 Jan 2023 11:31
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 27 15:44:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

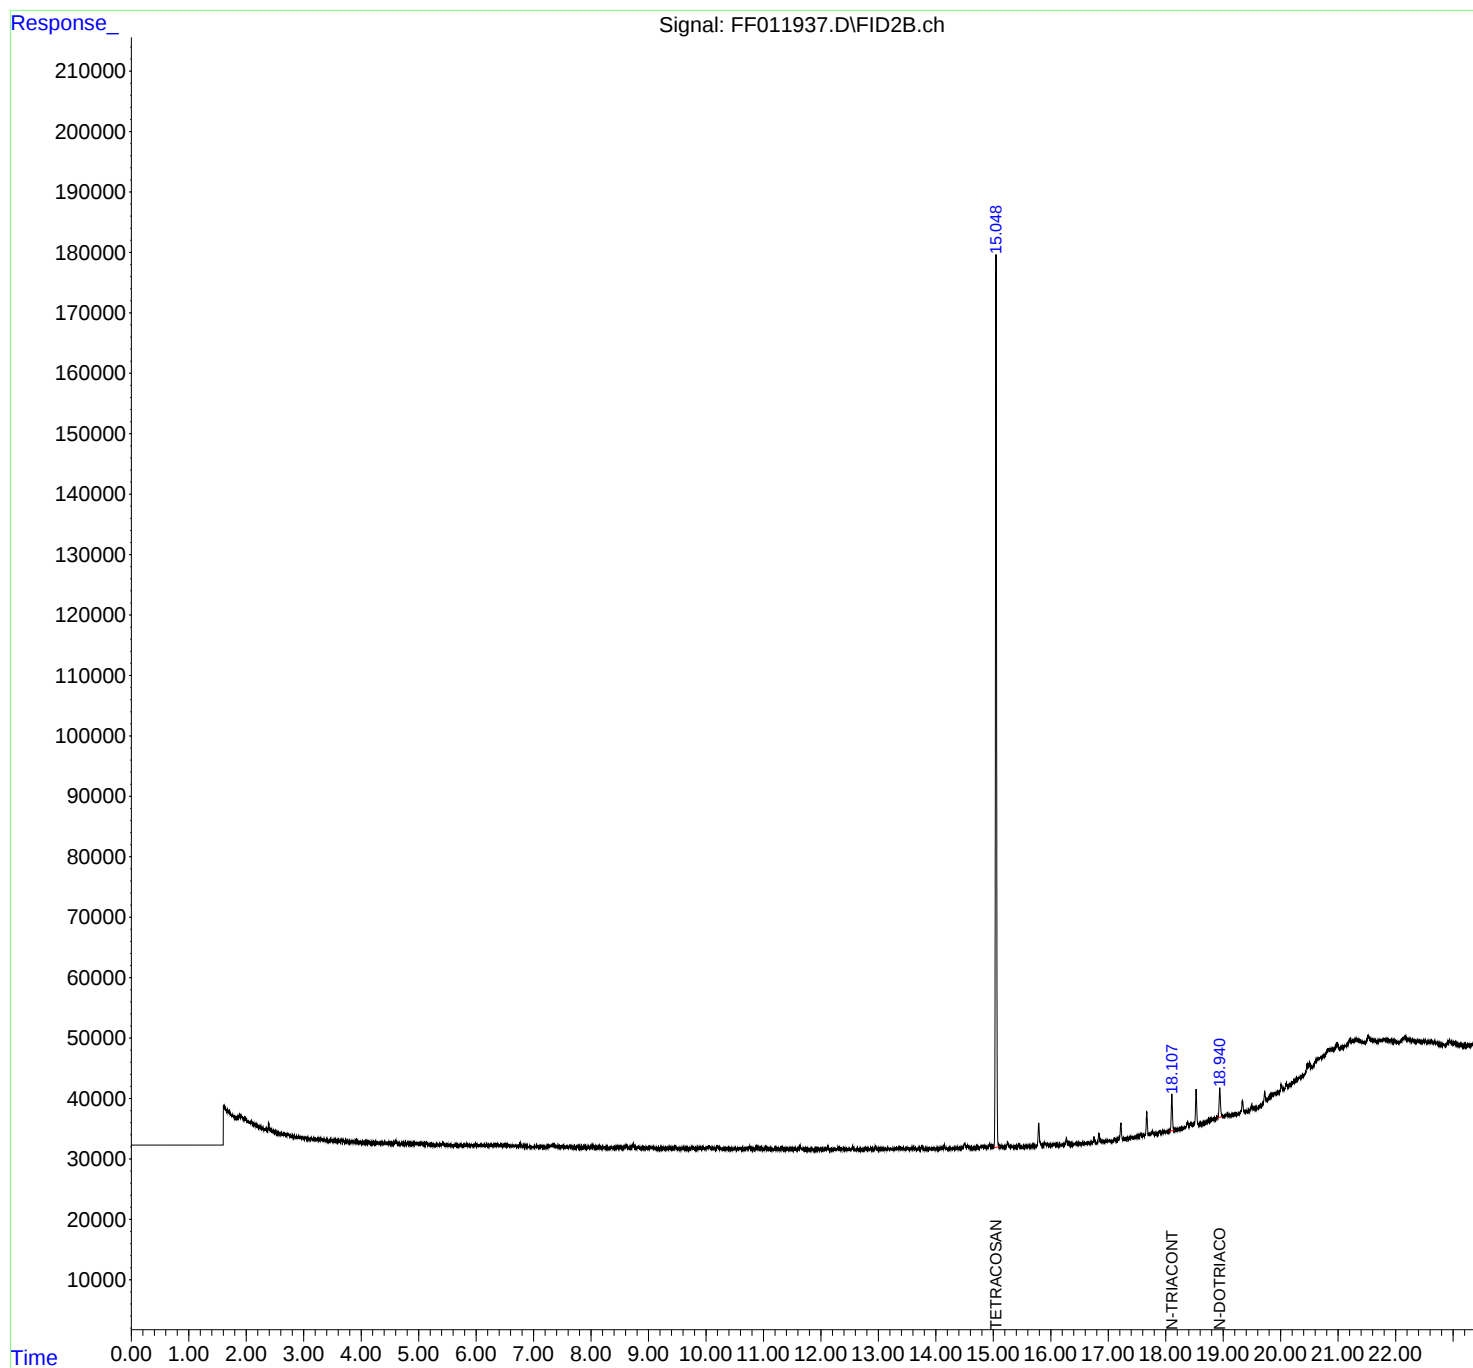


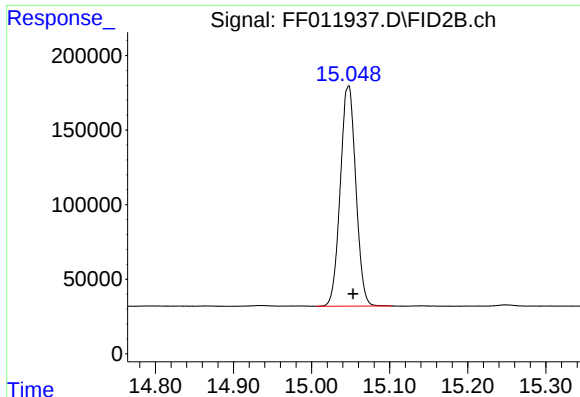

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.047 min
Delta R.T.: -0.006 min
Response: 2043996
Conc: 17.74 ug/ml

Instrument :
FID_F
ClientSampleId :

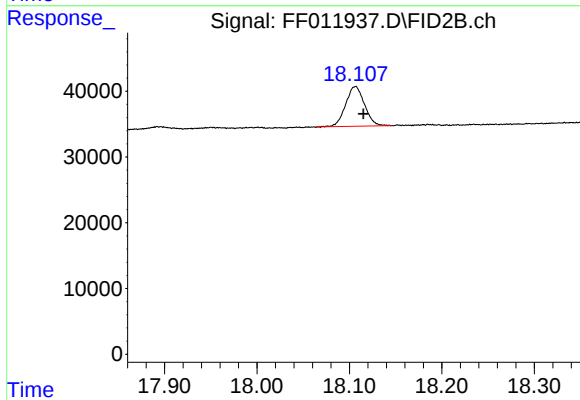

#13 N-TRIACONTANE

R.T.: 18.106 min
Delta R.T.: -0.009 min
Response: 85989
Conc: 0.67 ug/ml

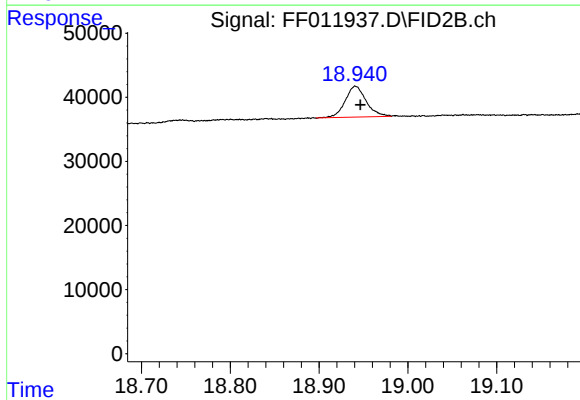

#14 N-DOTRIACONTANE

R.T.: 18.941 min
Delta R.T.: -0.005 min
Response: 78829
Conc: 0.61 ug/ml