

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012820\
Data File : FF006325.D
Signal(s) : FID2B.ch
Acq On : 28 Jan 2020 10:51
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 29 00:29:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.630	2046833	18.889 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.512	99971	0.865 ug/ml
15)	N-TETRATRIACONTANE	19.295	39742	0.353 ug/ml
16)	N-HEXATRIACONTANE	20.056	64446	0.603 ug/ml
17)	N-OCTATRIACONTANE	20.754	161478	1.745 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012820\
Data File : FF006325.D
Signal(s) : FID2B.ch
Acq On : 28 Jan 2020 10:51
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 29 00:29:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

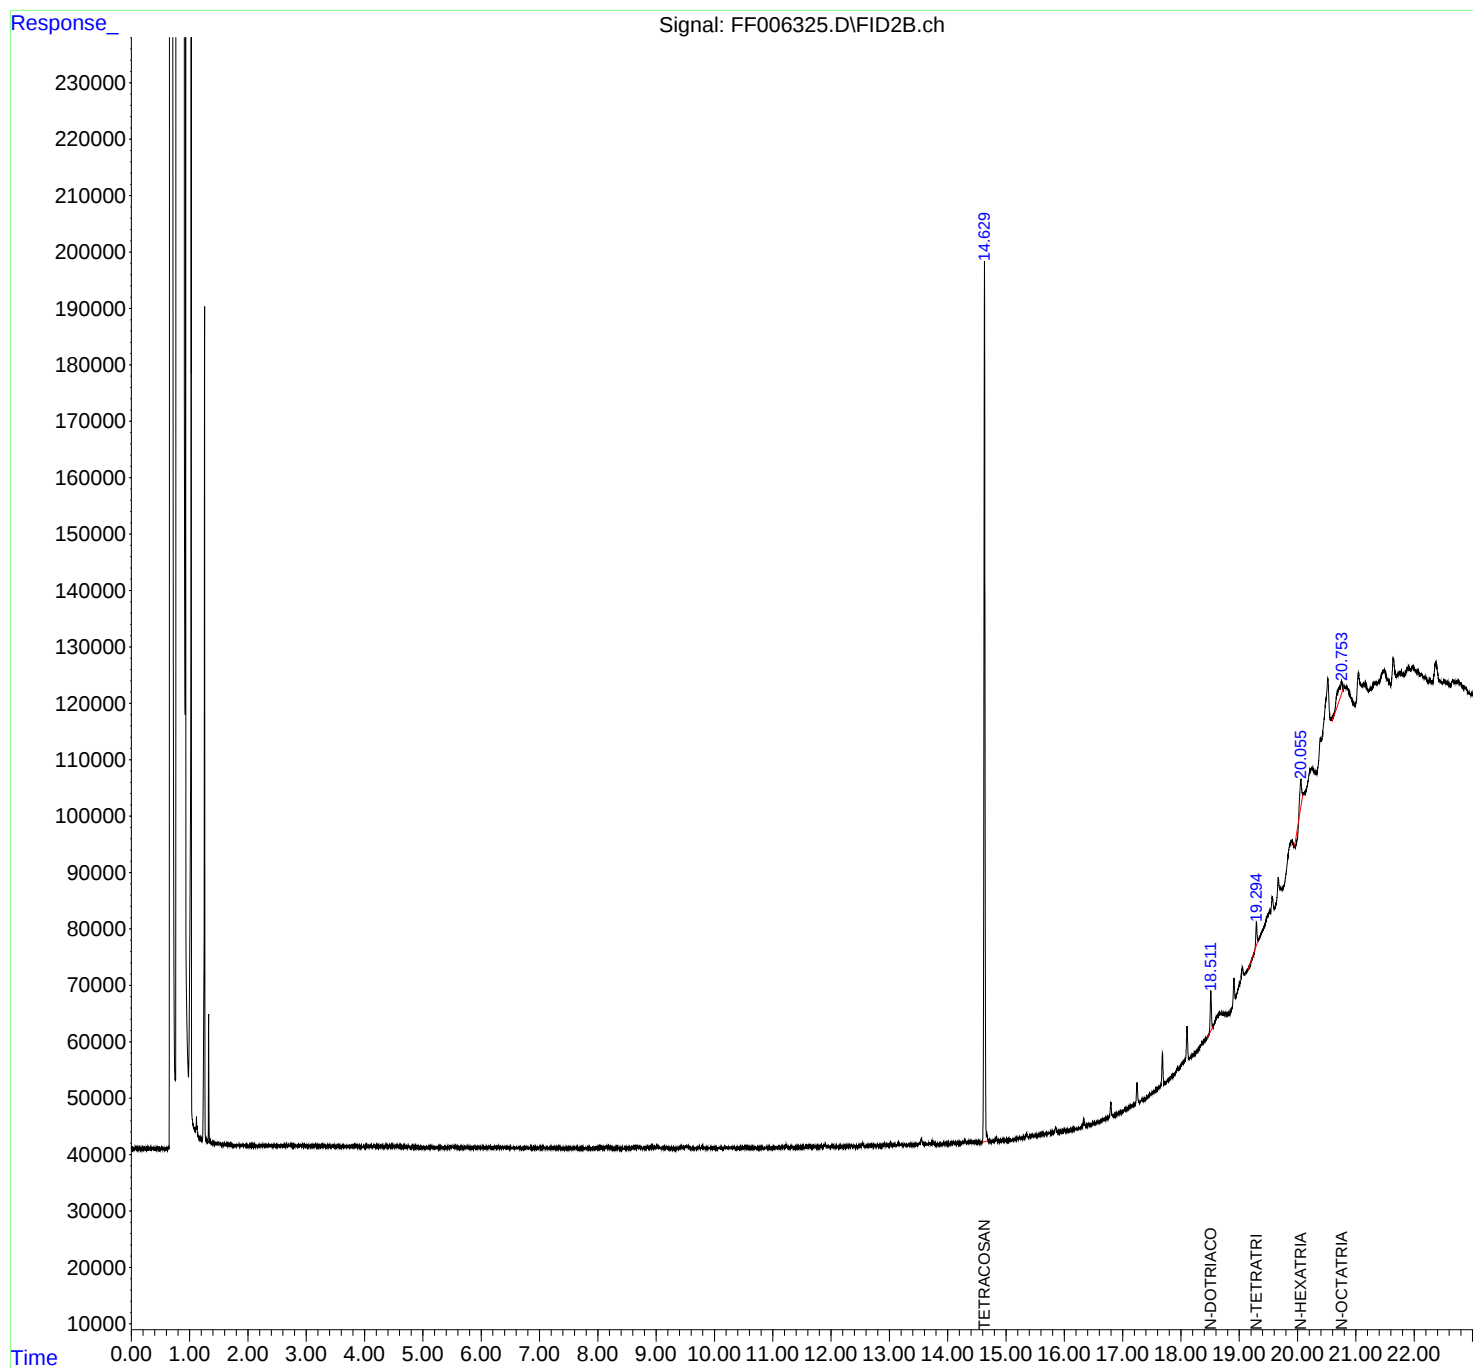


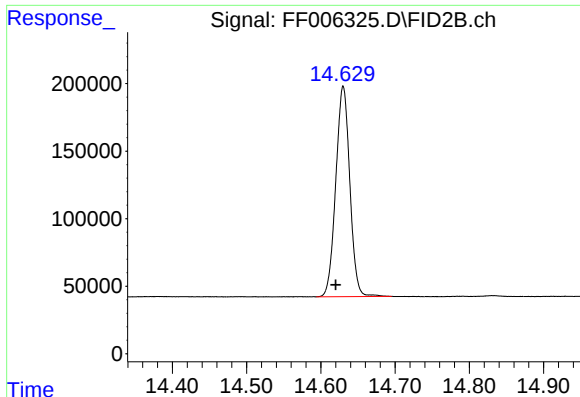

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.630 min
Delta R.T.: 0.010 min
Response: 2046833
Conc: 18.89 ug/ml

Instrument :
FID_F
ClientSampleId :

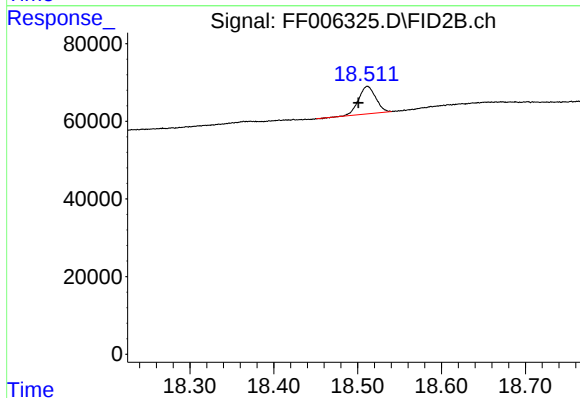


#14 N-DOTRIACONTANE

R.T.: 18.512 min
Delta R.T.: 0.011 min
Response: 99971
Conc: 0.87 ug/ml

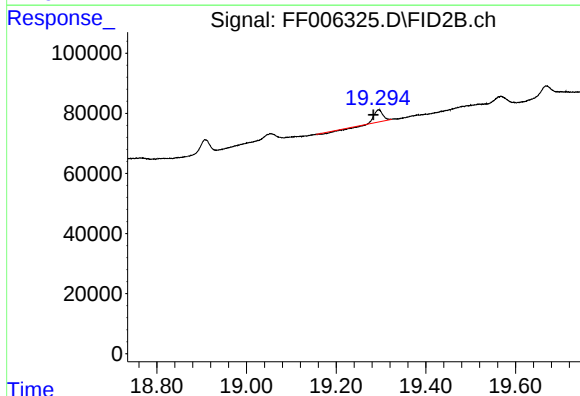


#15 N-TETRATRIACONTANE

R.T.: 19.295 min
Delta R.T.: 0.012 min
Response: 39742
Conc: 0.35 ug/ml

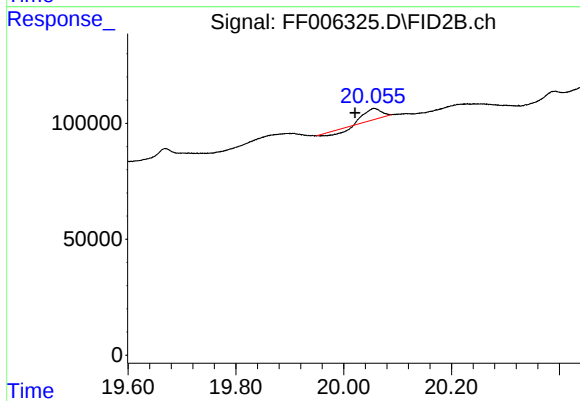

#16 N-HEXATRIACONTANE

R.T.: 20.056 min
Delta R.T.: 0.035 min
Response: 64446
Conc: 0.60 ug/ml

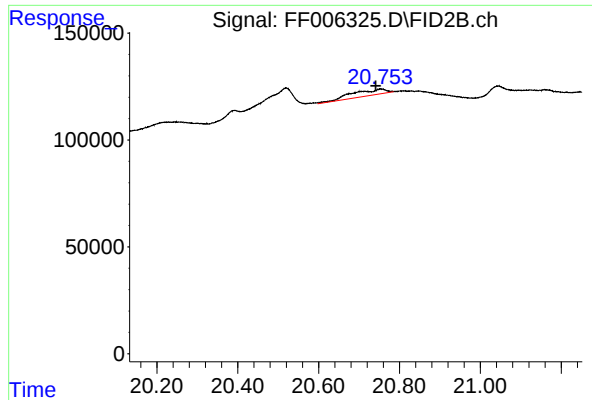

#17 N-OCTATRIACONTANE

R.T.: 20.754 min
Delta R.T.: 0.013 min
Response: 161478
Conc: 1.75 ug/ml

Instrument :
FID_F
ClientSampleId :