

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012820\
 Data File : FF006329.D
 Signal(s) : FID2B.ch
 Acq On : 28 Jan 2020 14:06
 Operator : DD\AJ
 Sample : L1265-02
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 29 00:30:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.630	1580746	14.588 ug/ml
Target Compounds			
3) N-DODECANE	6.355	116721	0.924 ug/ml
4) N-TETRADECANE	8.192	172425	1.366 ug/ml
5) N-HEXADECANE	9.789	157643	1.234 ug/ml
6) N-OCTADECANE	11.227	230108	1.814 ug/ml
7) N-EICOSANE	12.533	416384	3.258 ug/ml
8) N-DOCOSANE	13.734	295606	2.344 ug/ml
10) N-TETRACOSANE	14.822	1601629	12.857 ug/ml
11) N-HEXACOSANE	15.850	423544	3.445 ug/ml
12) N-OCTACOSANE	16.803	1624470	13.363 ug/ml
13) N-TRIACONTANE	17.693	5020464	41.872 ug/ml
14) N-DOTRIACONTANE	18.499	2832789	24.513 ug/ml
15) N-TETRATRIACONTANE	19.303	3484078	30.925 ug/ml
16) N-HEXATRIACONTANE	20.009	1302247	12.179 ug/ml
17) N-OCTATRIACONTANE	20.729	1383566	14.955 ug/ml
18) N-TETRACONTANE	21.610	110137	1.094 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012820\
Data File : FF006329.D
Signal(s) : FID2B.ch
Acq On : 28 Jan 2020 14:06
Operator : DD\AJ
Sample : L1265-02
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 29 00:30:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

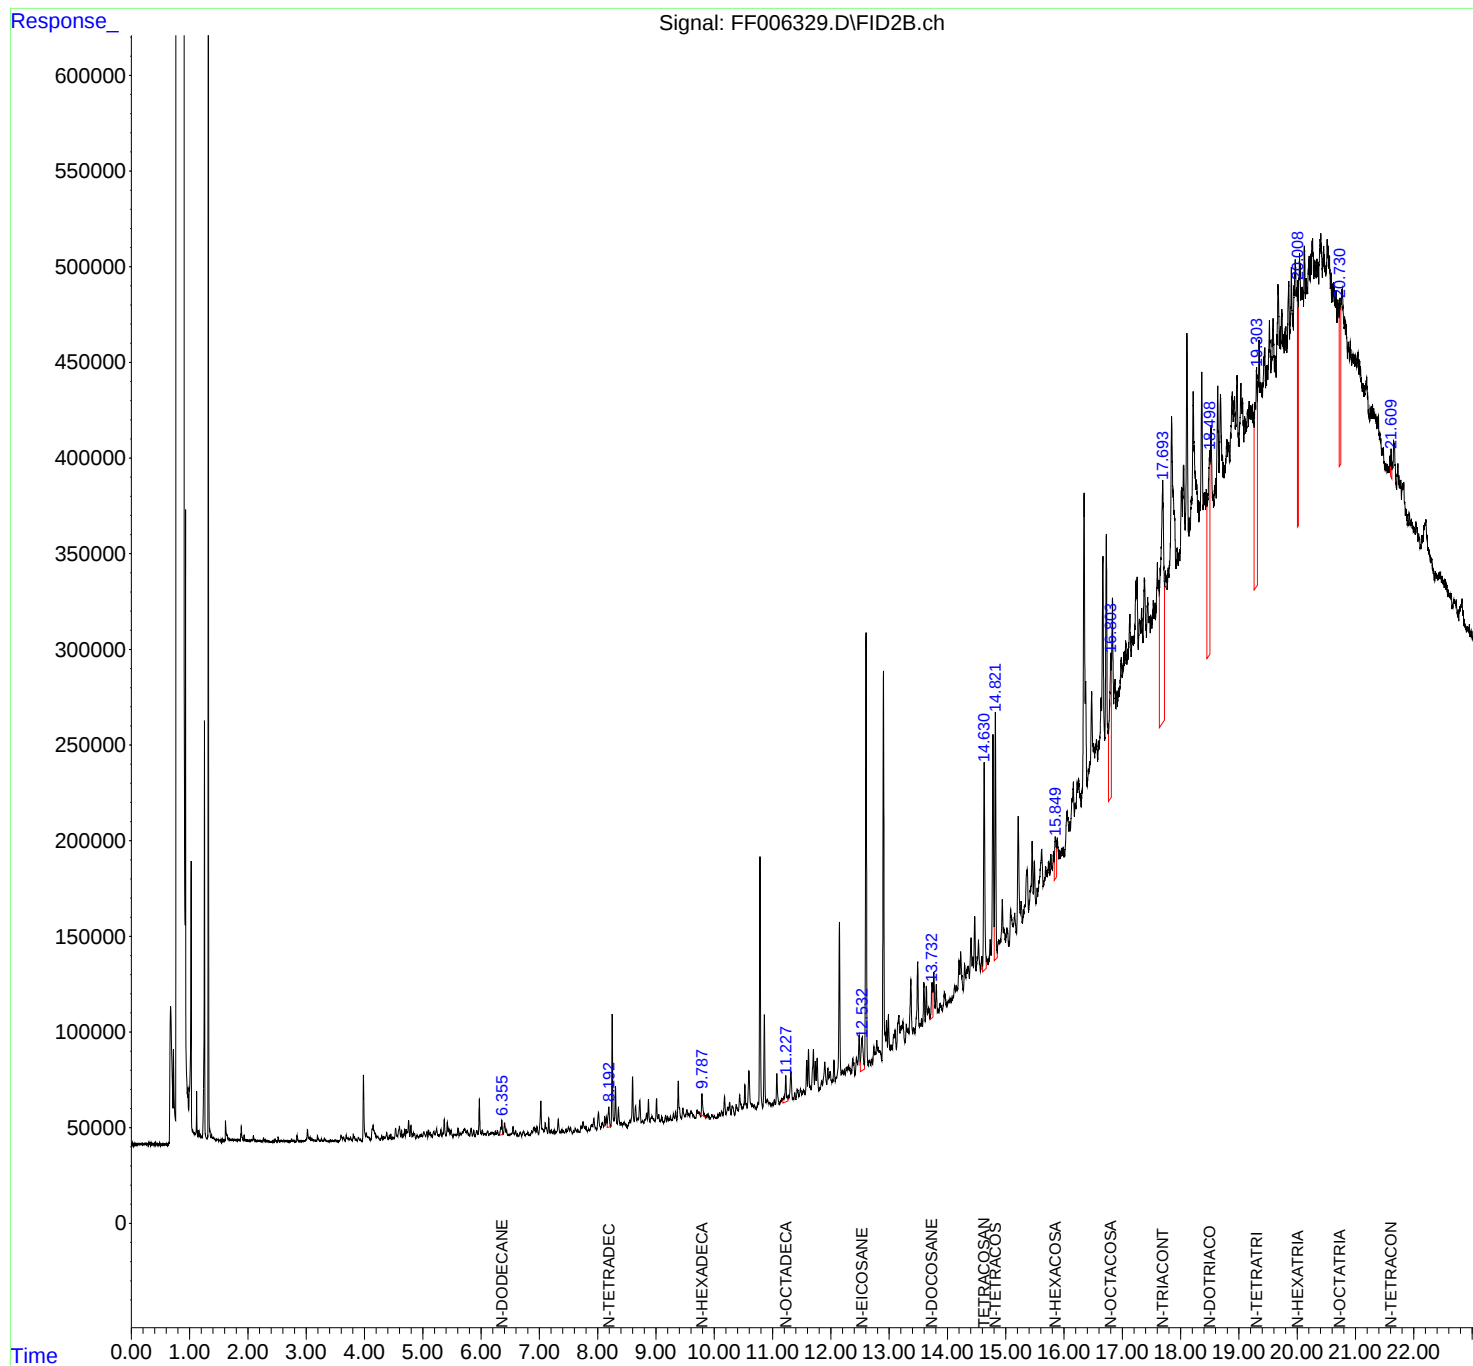


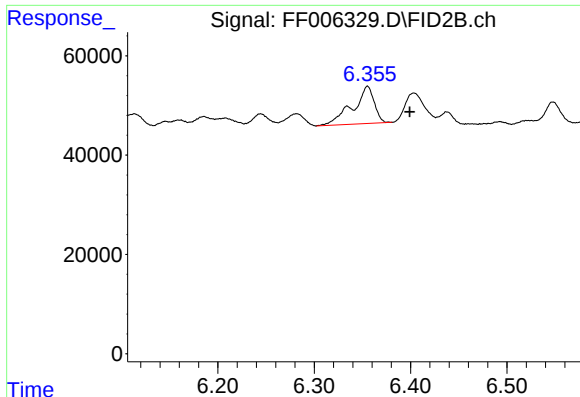

#3 N-DODECANE


R.T.: 6.355 min
Delta R.T.: -0.044 min
Response: 116721
Conc: 0.92 ug/ml

Instrument :
FID_F
ClientSampleId :

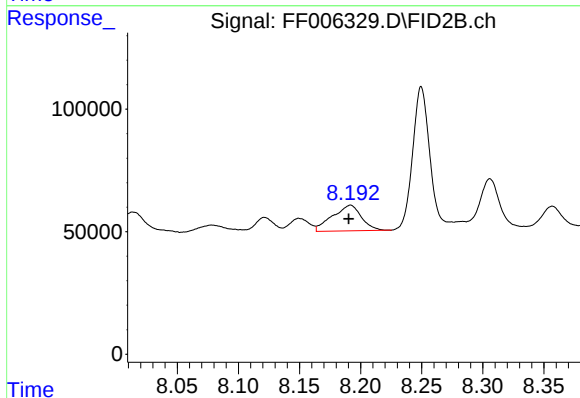


#4 N-TETRADECANE

R.T.: 8.192 min
Delta R.T.: 0.001 min
Response: 172425
Conc: 1.37 ug/ml

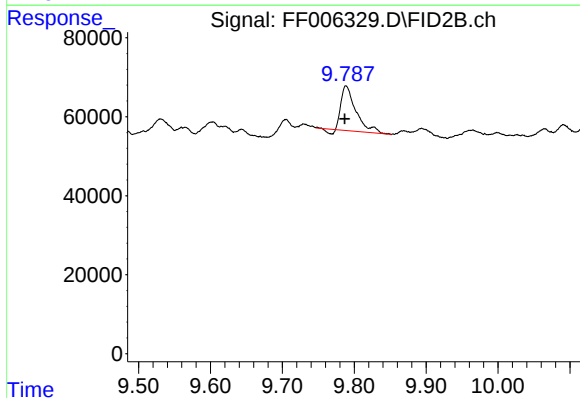


#5 N-HEXADECANE

R.T.: 9.789 min
Delta R.T.: 0.002 min
Response: 157643
Conc: 1.23 ug/ml

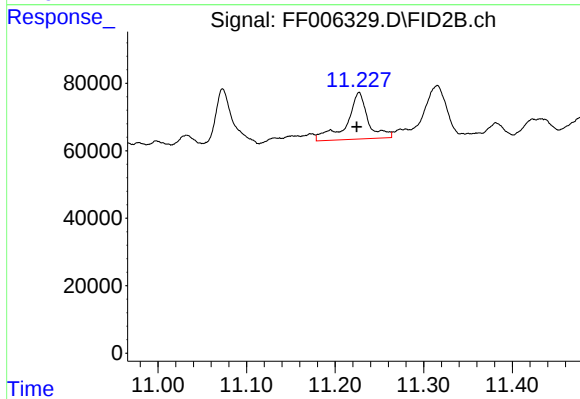

#6 N-OCTADECANE


R.T.: 11.227 min
Delta R.T.: 0.003 min
Response: 230108
Conc: 1.81 ug/ml

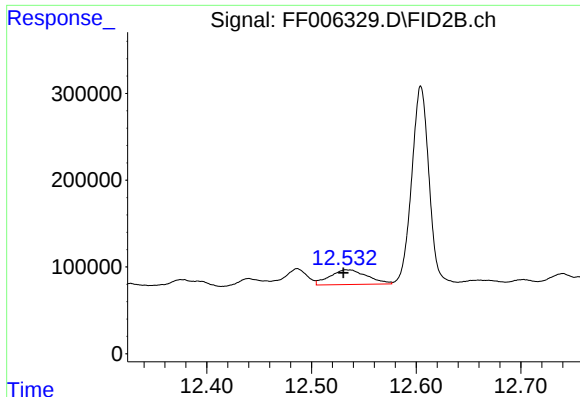

#7 N-EICOSANE


R.T.: 12.533 min
Delta R.T.: 0.003 min
Response: 416384
Conc: 3.26 ug/ml

Instrument :
FID_F
ClientSampleId :

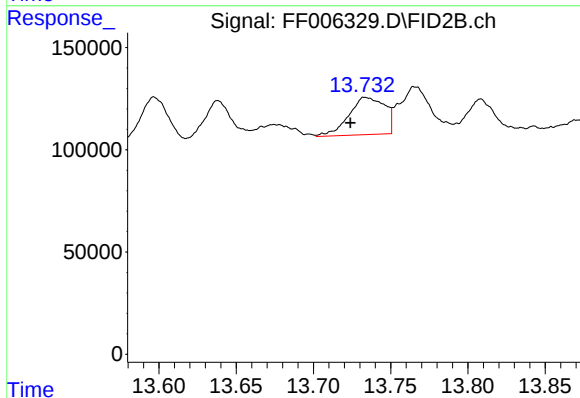


#8 N-DOCOSANE

R.T.: 13.734 min
Delta R.T.: 0.010 min
Response: 295606
Conc: 2.34 ug/ml

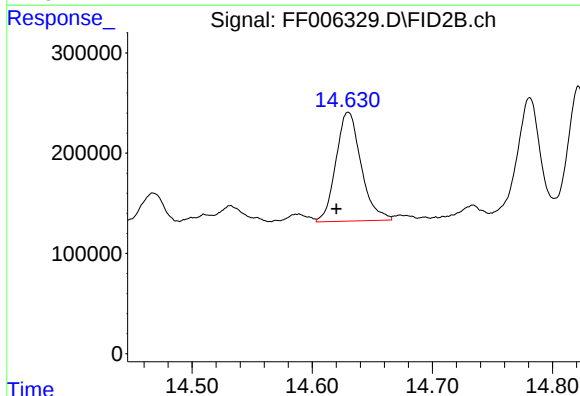


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.630 min
Delta R.T.: 0.010 min
Response: 1580746
Conc: 14.59 ug/ml

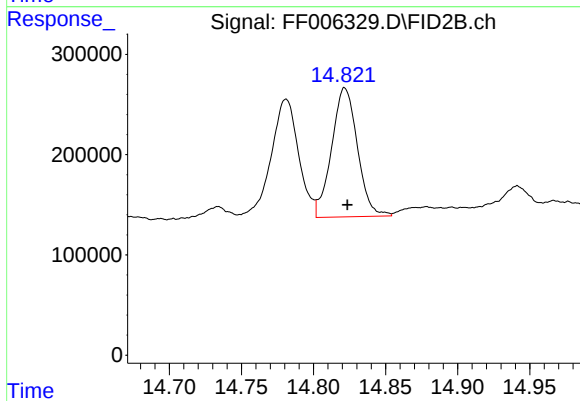

#10 N-TETRACOSANE


R.T.: 14.822 min
Delta R.T.: -0.002 min
Response: 1601629
Conc: 12.86 ug/ml

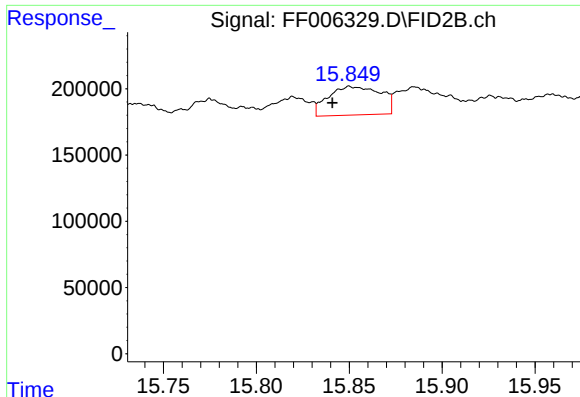

#11 N-HEXACOSANE


R.T.: 15.850 min
Delta R.T.: 0.010 min
Response: 423544
Conc: 3.45 ug/ml

Instrument :
FID_F
ClientSampleId :

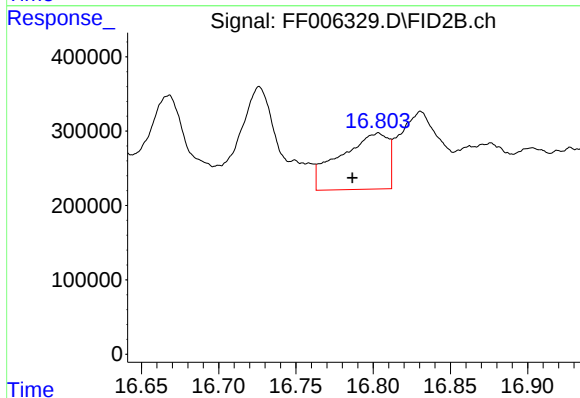


#12 N-OCTACOSANE

R.T.: 16.803 min
Delta R.T.: 0.017 min
Response: 1624470
Conc: 13.36 ug/ml

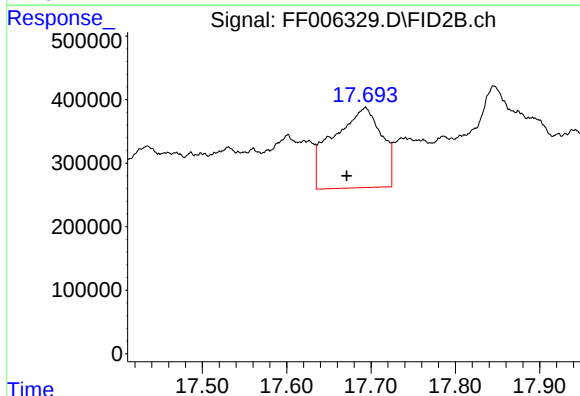


#13 N-TRIACONTANE

R.T.: 17.693 min
Delta R.T.: 0.022 min
Response: 5020464
Conc: 41.87 ug/ml

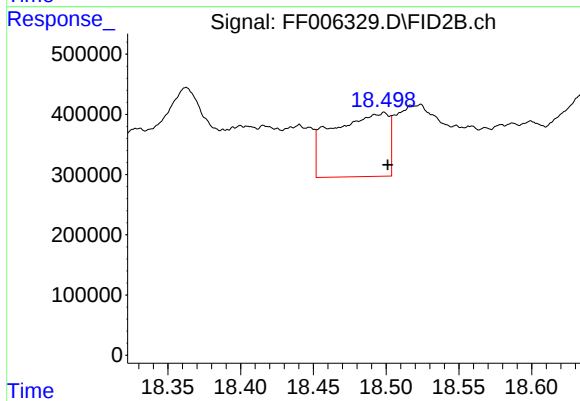

#14 N-DOTRIACONTANE


R.T.: 18.499 min
Delta R.T.: -0.002 min
Response: 2832789
Conc: 24.51 ug/ml

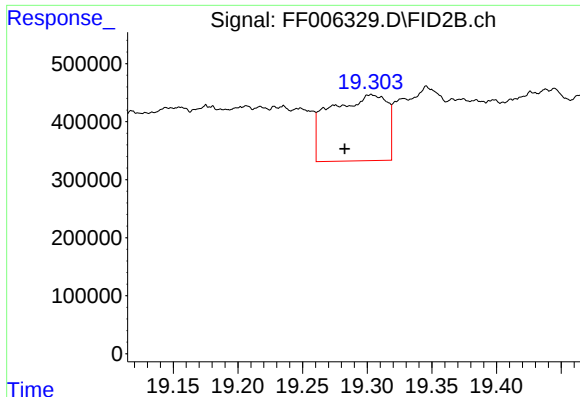

#15 N-TETRATRIACONTANE


R.T.: 19.303 min
Delta R.T.: 0.020 min
Response: 3484078
Conc: 30.93 ug/ml

Instrument :
FID_F
ClientSampleId :

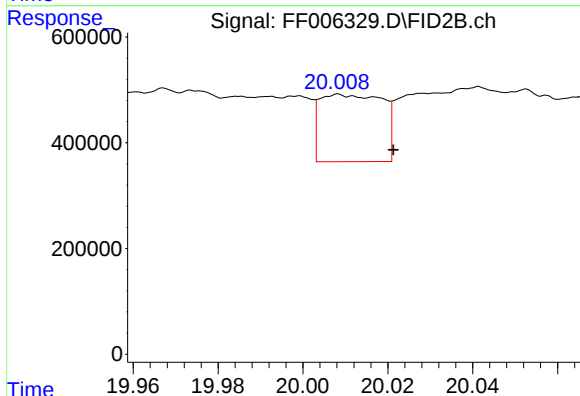


#16 N-HEXATRIACONTANE

R.T.: 20.009 min
Delta R.T.: -0.013 min
Response: 1302247
Conc: 12.18 ug/ml

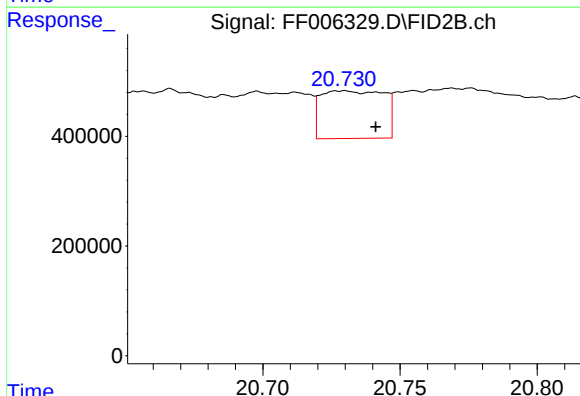

#17 N-OCTATRIACONTANE

R.T.: 20.729 min
Delta R.T.: -0.012 min
Response: 1383566
Conc: 14.95 ug/ml

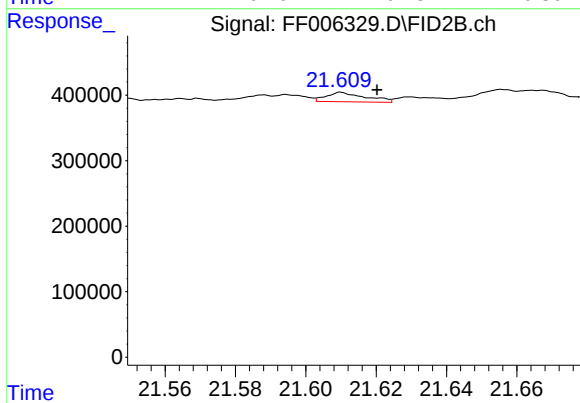

#18 N-TETRACONTANE

R.T.: 21.610 min
Delta R.T.: -0.010 min
Response: 110137
Conc: 1.09 ug/ml