

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012820\
 Data File : FF006332.D
 Signal(s) : FID2B.ch
 Acq On : 28 Jan 2020 15:37
 Operator : DD\AJ
 Sample : L1263-04 10X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 29 00:31:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.629	137359	1.268 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.823	182410	1.464 ug/ml
12) N-OCTACOSANE	16.803	113109	0.930 ug/ml
13) N-TRIACONTANE	17.687	421299	3.514 ug/ml
14) N-DOTRIACONTANE	18.504	439267	3.801 ug/ml
15) N-TETRATRIACONTANE	19.302	189803	1.685 ug/ml
16) N-HEXATRIACONTANE	20.030	1630067	15.245 ug/ml
17) N-OCTATRIACONTANE	20.734	975328	10.542 ug/ml
18) N-TETRACONTANE	21.595	152488	1.514 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012820\
Data File : FF006332.D
Signal(s) : FID2B.ch
Acq On : 28 Jan 2020 15:37
Operator : DD\AJ
Sample : L1263-04 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 29 00:31:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

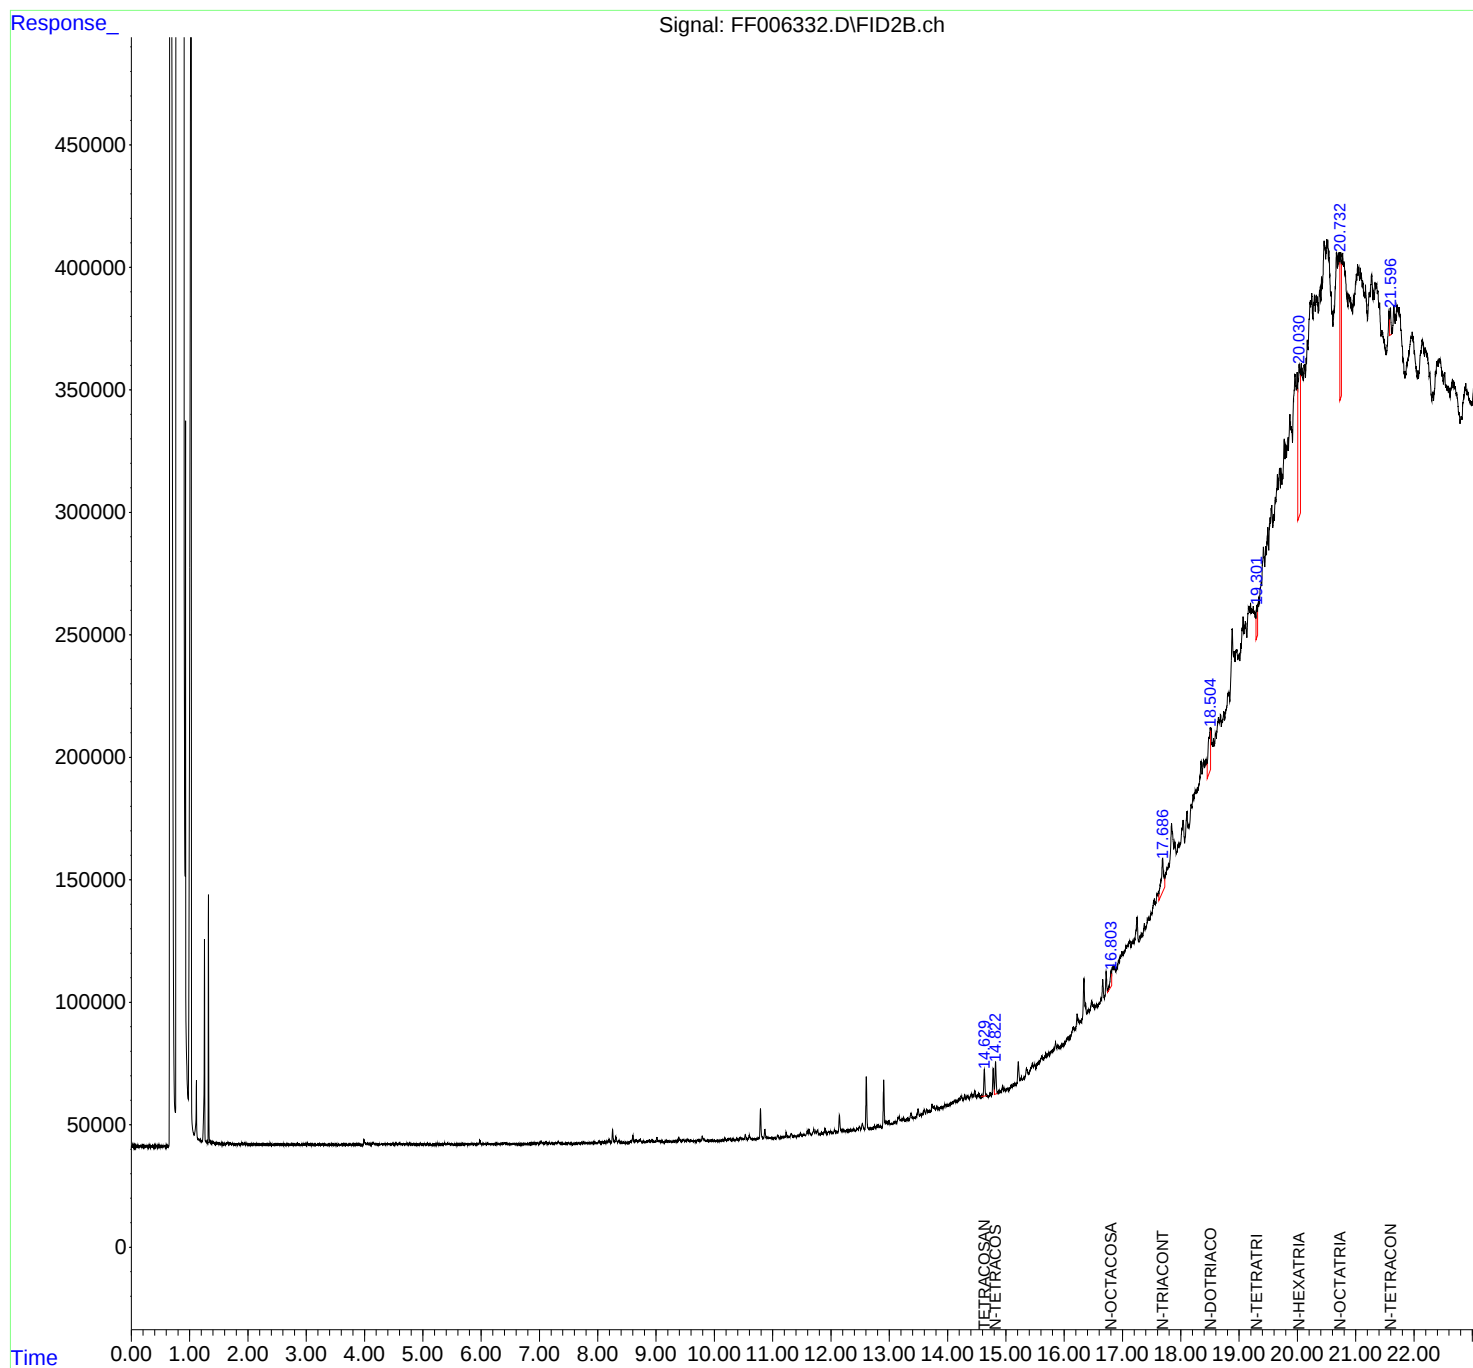


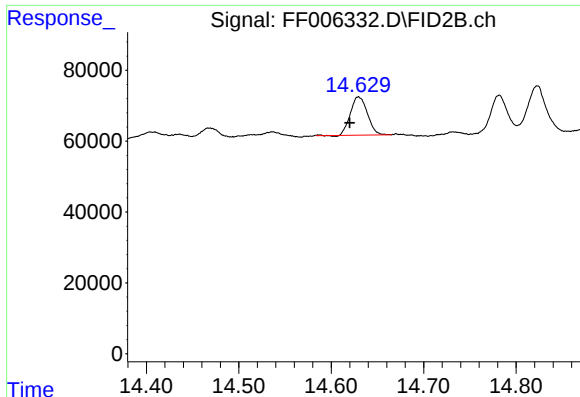

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.629 min
Delta R.T.: 0.009 min
Response: 137359
Conc: 1.27 ug/ml

Instrument :
FID_F
ClientSampleId :

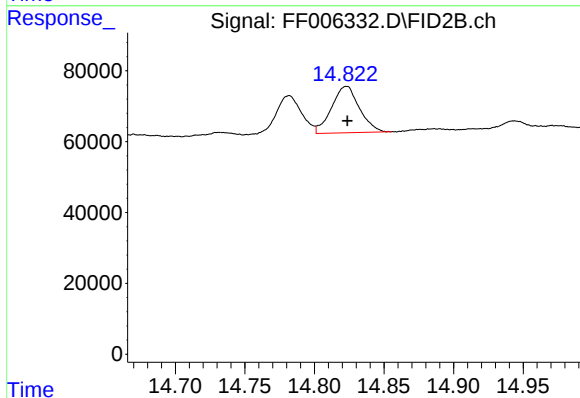


#10 N-TETRACOSANE

R.T.: 14.823 min
Delta R.T.: 0.000 min
Response: 182410
Conc: 1.46 ug/ml

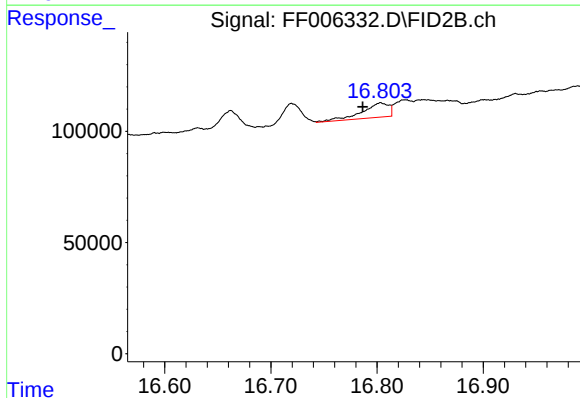


#12 N-OCTACOSANE

R.T.: 16.803 min
Delta R.T.: 0.017 min
Response: 113109
Conc: 0.93 ug/ml

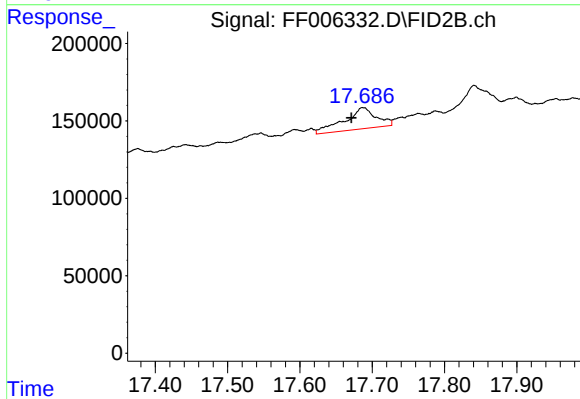

#13 N-TRIACONTANE


R.T.: 17.687 min
Delta R.T.: 0.016 min
Response: 421299
Conc: 3.51 ug/ml

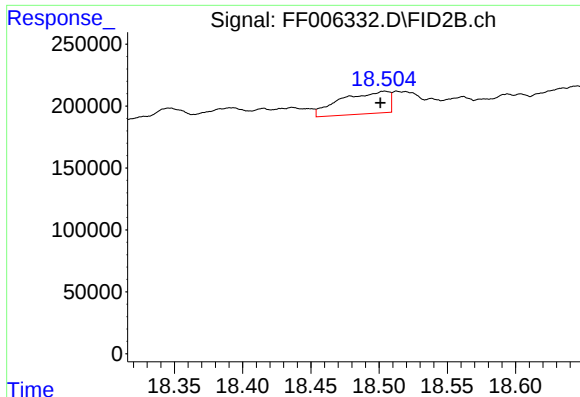

#14 N-DOTRIACONTANE


R.T.: 18.504 min
Delta R.T.: 0.003 min
Response: 439267
Conc: 3.80 ug/ml

Instrument :
FID_F
ClientSampleId :

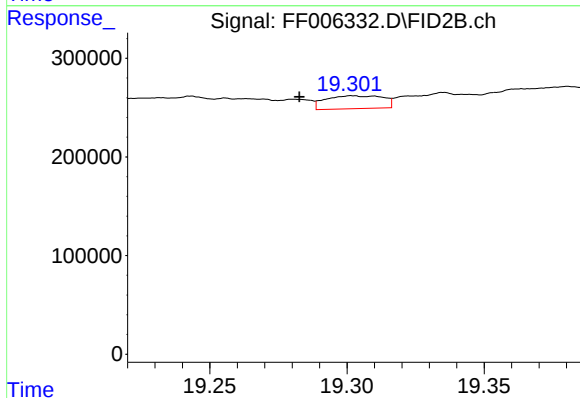


#15 N-TETRATRIACONTANE

R.T.: 19.302 min
Delta R.T.: 0.019 min
Response: 189803
Conc: 1.68 ug/ml

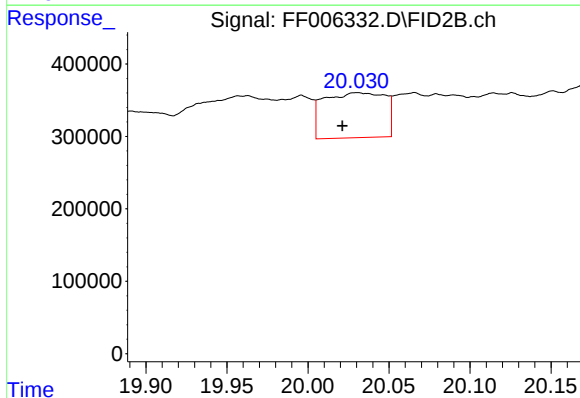


#16 N-HEXATRIACONTANE

R.T.: 20.030 min
Delta R.T.: 0.009 min
Response: 1630067
Conc: 15.25 ug/ml

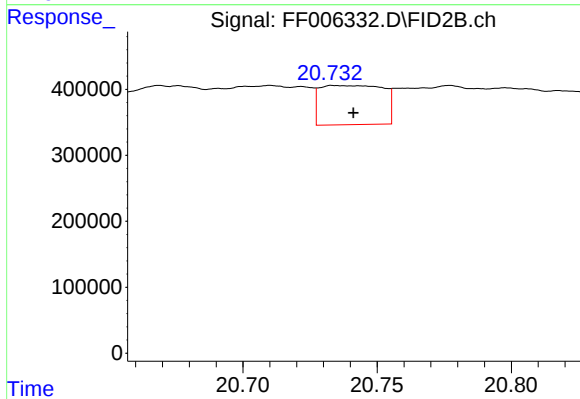

#17 N-OCTATRIACONTANE

R.T.: 20.734 min
Delta R.T.: -0.007 min
Response: 975328
Conc: 10.54 ug/ml

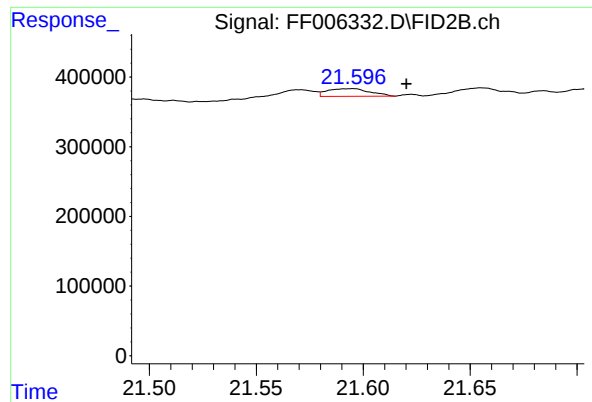

#18 N-TETRACONTANE

R.T.: 21.595 min
Delta R.T.: -0.025 min
Response: 152488
Conc: 1.51 ug/ml

Instrument :
FID_F
ClientSampleId :