

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012820\
 Data File : FF006335.D
 Signal(s) : FID2B.ch
 Acq On : 28 Jan 2020 17:08
 Operator : DD\AJ
 Sample : PB126392BS
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 29 00:32:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.630	1683226	15.534 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.683	217456	1.814 ug/ml
14) N-DOTRIACONTANE	18.513	537925	4.655 ug/ml
15) N-TETRATRIACONTANE	19.298	76363	0.678 ug/ml
16) N-HEXATRIACONTANE	20.036	457398	4.278 ug/ml
17) N-OCTATRIACONTANE	20.729	183429	1.983 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012820\
Data File : FF006335.D
Signal(s) : FID2B.ch
Acq On : 28 Jan 2020 17:08
Operator : DD\AJ
Sample : PB126392BS
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 29 00:32:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

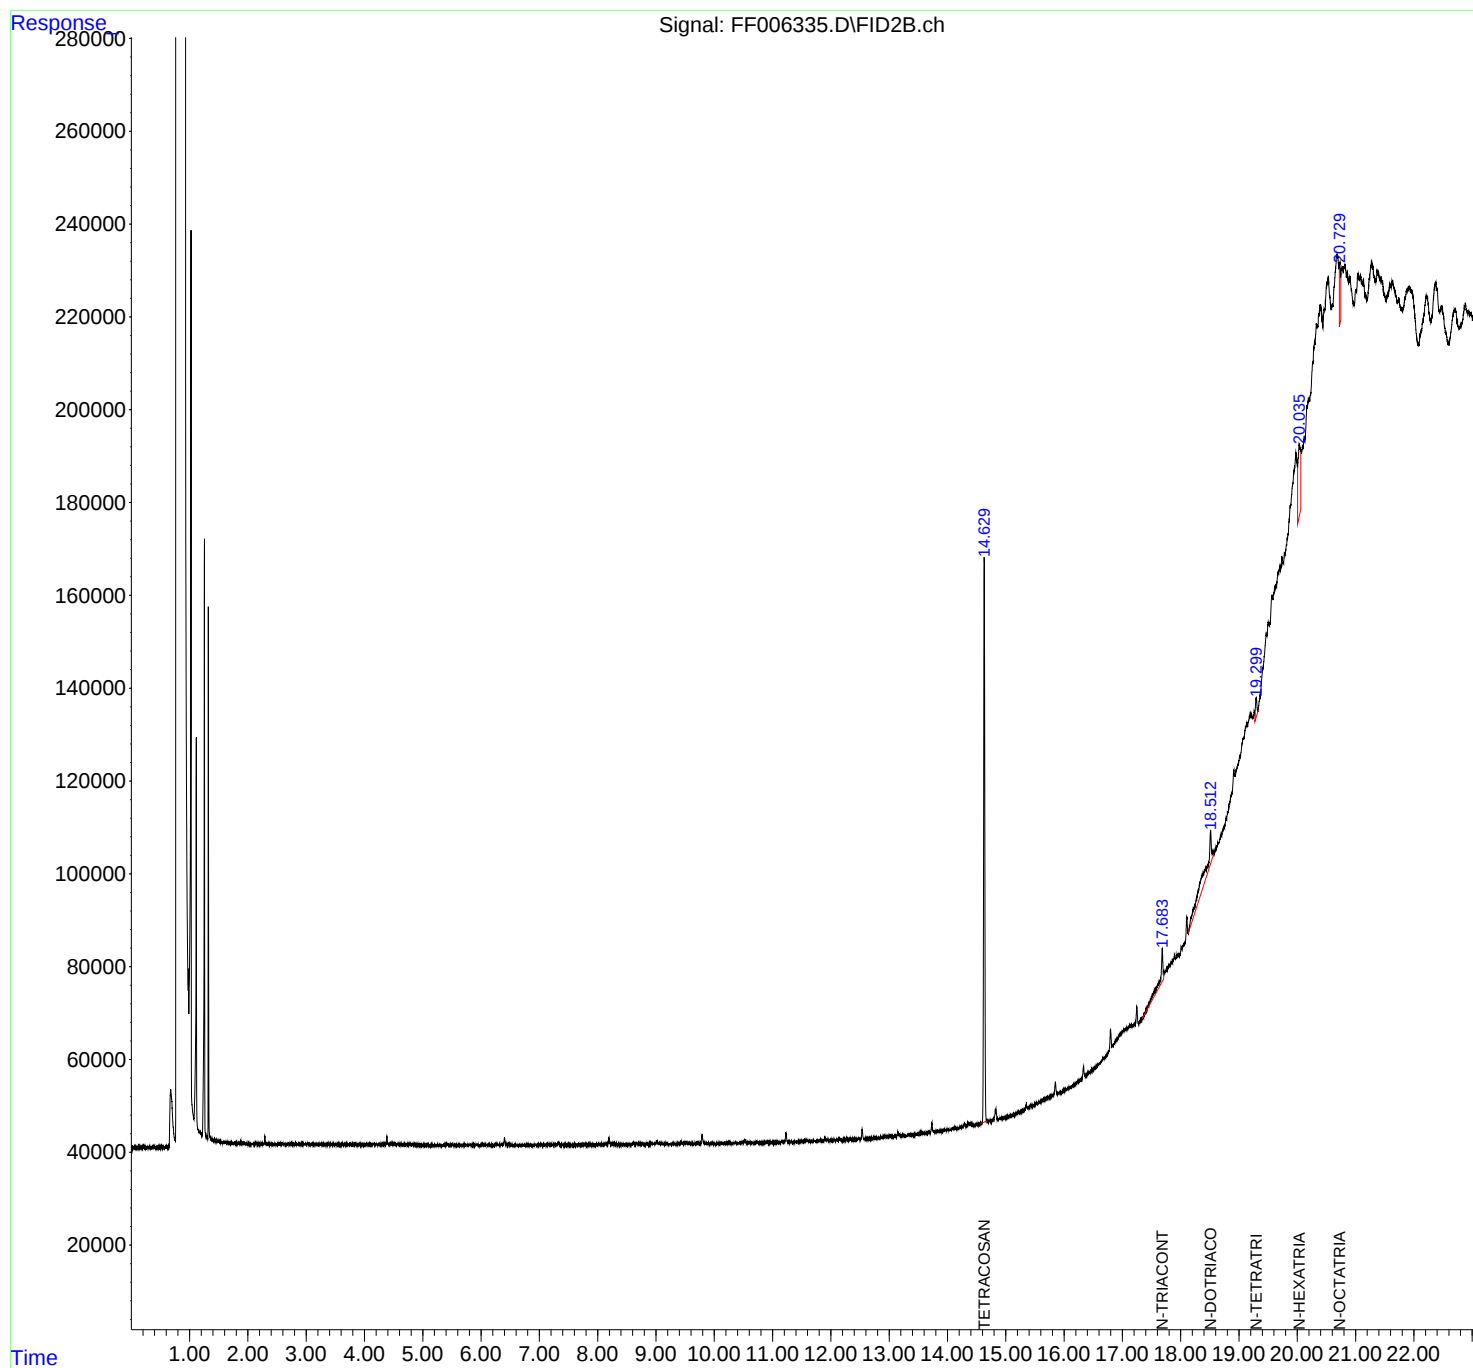


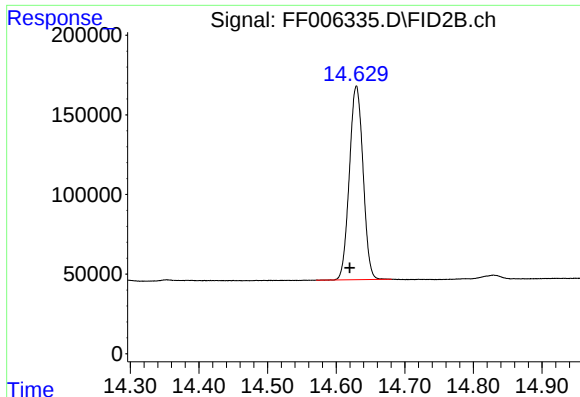

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.630 min
Delta R.T.: 0.009 min
Response: 1683226
Conc: 15.53 ug/ml

Instrument :
FID_F
ClientSampleId :

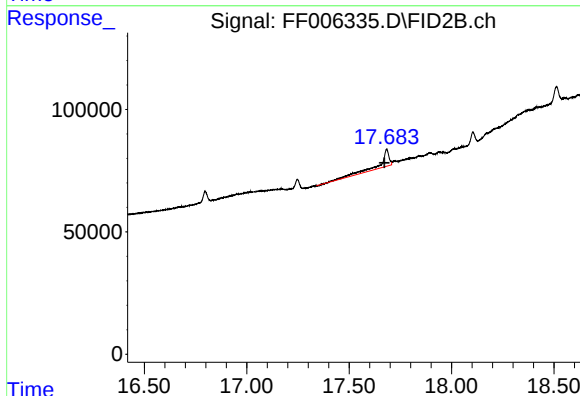


#13 N-TRIACONTANE

R.T.: 17.683 min
Delta R.T.: 0.012 min
Response: 217456
Conc: 1.81 ug/ml

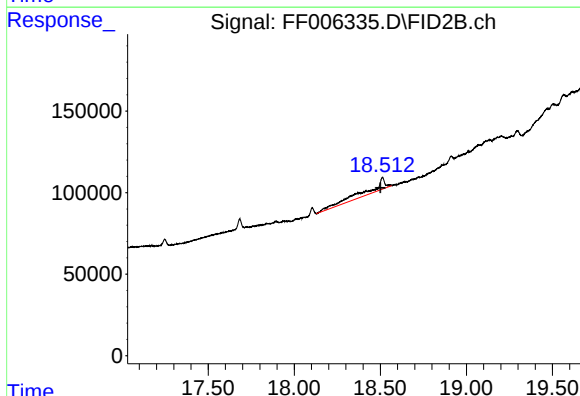


#14 N-DOTRIACONTANE

R.T.: 18.513 min
Delta R.T.: 0.012 min
Response: 537925
Conc: 4.65 ug/ml

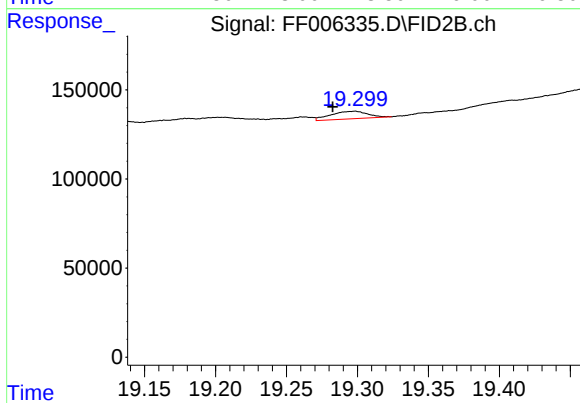

#15 N-TETRATRIACONTANE


R.T.: 19.298 min
Delta R.T.: 0.015 min
Response: 76363
Conc: 0.68 ug/ml

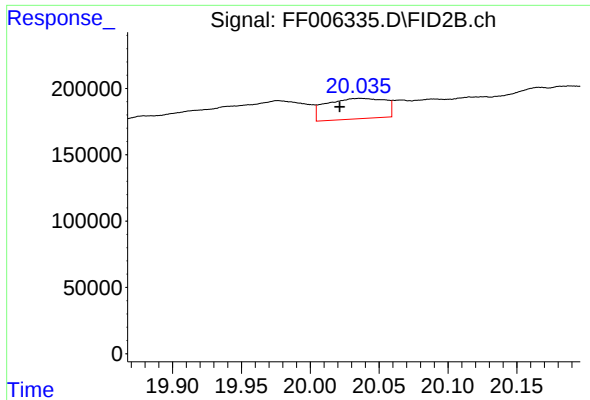

#16 N-HEXATRIACONTANE

R.T.: 20.036 min
Delta R.T.: 0.015 min
Response: 457398
Conc: 4.28 ug/ml

Instrument :
FID_F
ClientSampleId :

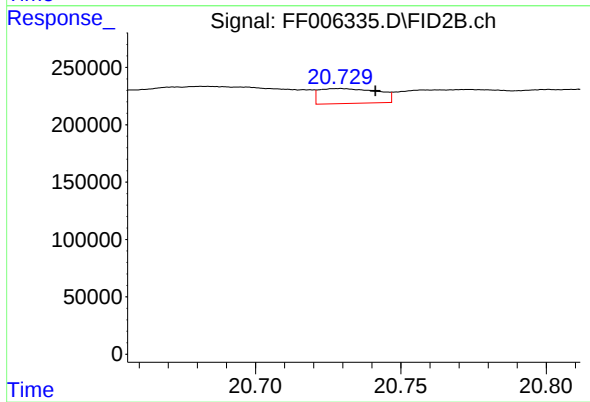

#17 N-OCTATRIACONTANE

R.T.: 20.729 min
Delta R.T.: -0.012 min
Response: 183429
Conc: 1.98 ug/ml