

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012820\
 Data File : FF006336.D
 Signal(s) : FID2B.ch
 Acq On : 28 Jan 2020 17:38
 Operator : DD\AJ
 Sample : L1264-01
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 29 00:32:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.630	1818025	16.778 ug/ml
Target Compounds			
4) N-TETRADECANE	8.253f	91144	0.722 ug/ml
11) N-HEXACOSANE	15.850	169148	1.376 ug/ml
12) N-OCTACOSANE	16.796	446752	3.675 ug/ml
13) N-TRIACONTANE	17.683	611942	5.104 ug/ml
14) N-DOTRIACONTANE	18.513	666770	5.770 ug/ml
15) N-TETRATRIACONTANE	19.294	158027	1.403 ug/ml
16) N-HEXATRIACONTANE	20.046	114023	1.066 ug/ml
17) N-OCTATRIACONTANE	20.756	74663	0.807 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012820\
Data File : FF006336.D
Signal(s) : FID2B.ch
Acq On : 28 Jan 2020 17:38
Operator : DD\AJ
Sample : L1264-01
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Jan 29 00:32:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

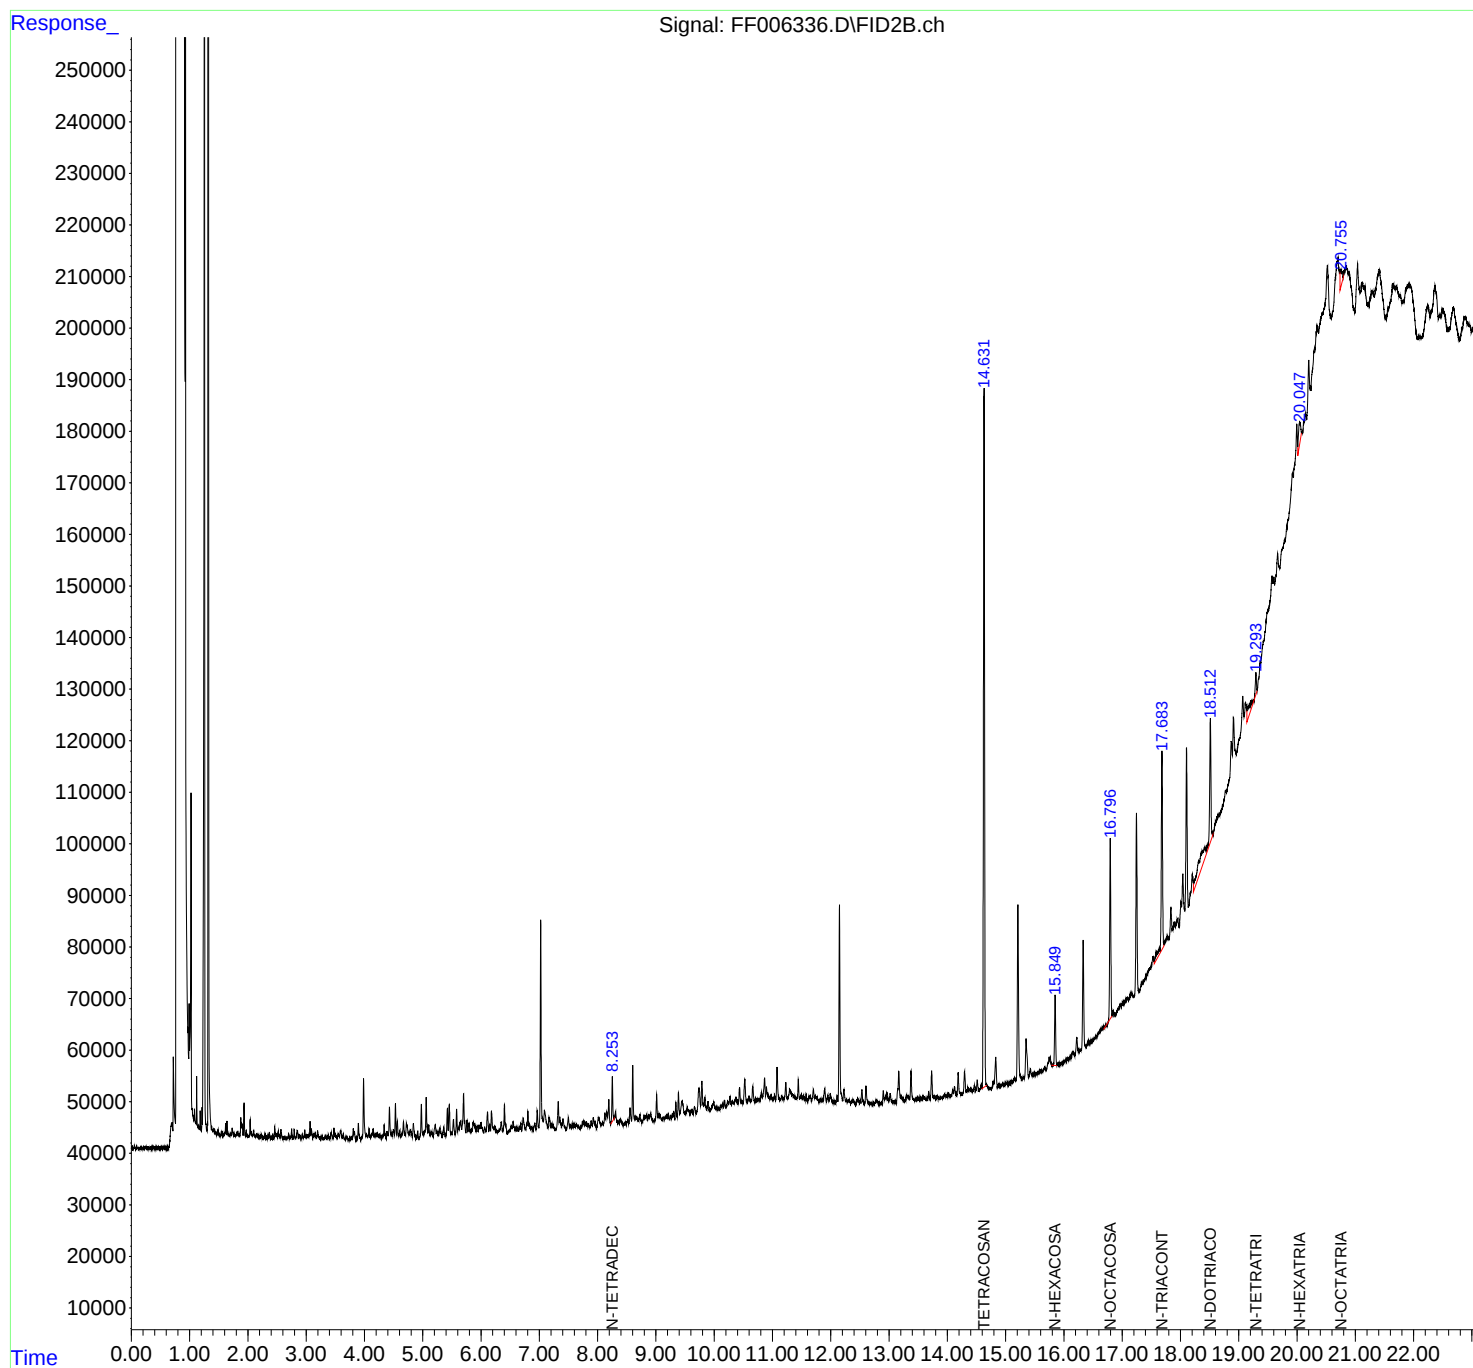


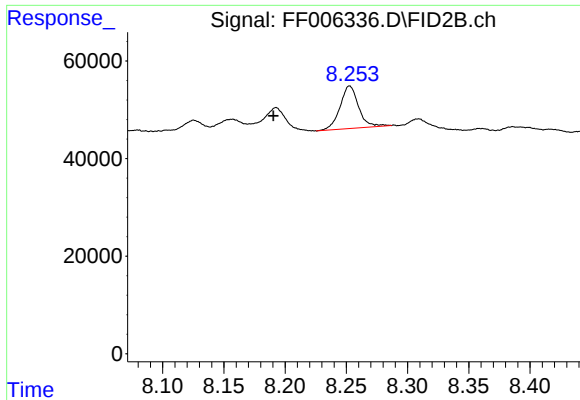

#4 N-TETRADECANE


R.T.: 8.253 min
Delta R.T.: 0.062 min
Response: 91144
Conc: 0.72 ug/ml

Instrument :
FID_F
ClientSampleId :

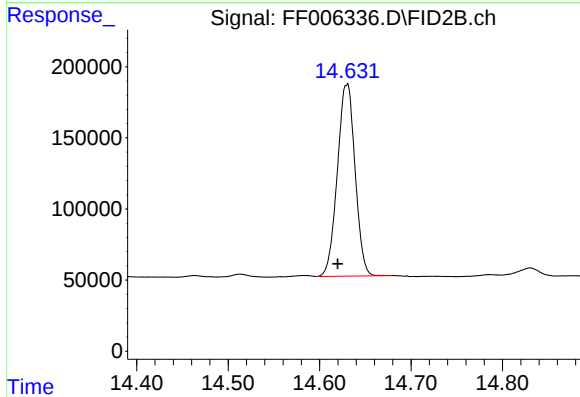


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.630 min
Delta R.T.: 0.010 min
Response: 1818025
Conc: 16.78 ug/ml

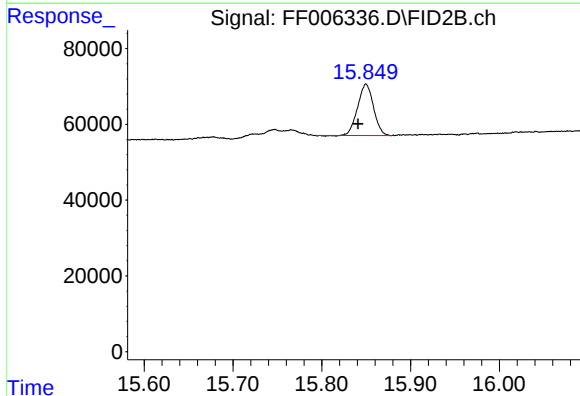


#11 N-HEXACOSANE

R.T.: 15.850 min
Delta R.T.: 0.009 min
Response: 169148
Conc: 1.38 ug/ml

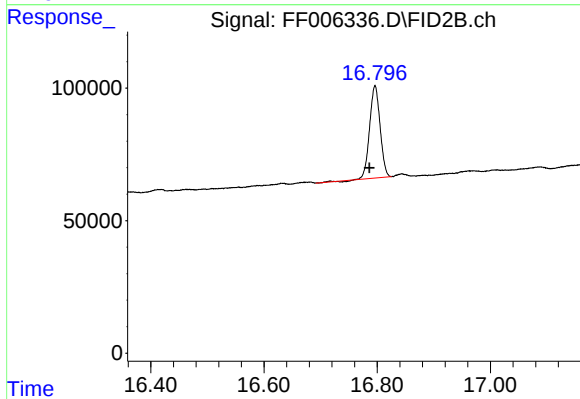

#12 N-OCTACOSANE


R.T.: 16.796 min
Delta R.T.: 0.010 min
Response: 446752
Conc: 3.68 ug/ml

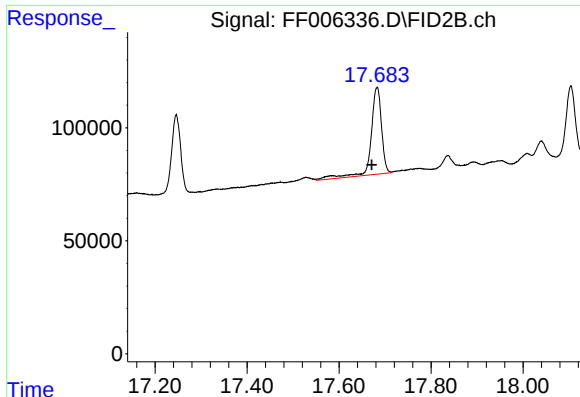

#13 N-TRIACONTANE


R.T.: 17.683 min
Delta R.T.: 0.012 min
Response: 611942
Conc: 5.10 ug/ml

Instrument :
FID_F
ClientSampleId :

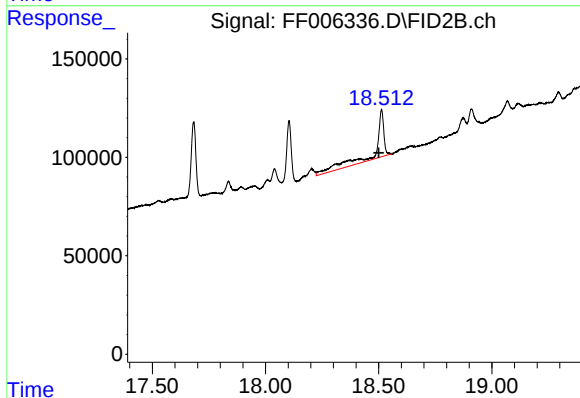


#14 N-DOTRIACONTANE

R.T.: 18.513 min
Delta R.T.: 0.012 min
Response: 666770
Conc: 5.77 ug/ml

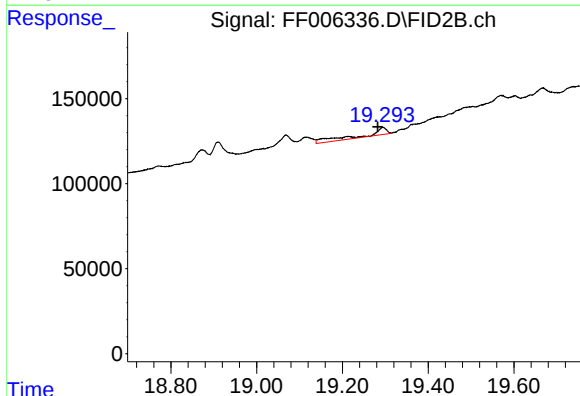


#15 N-TETRATRIACONTANE

R.T.: 19.294 min
Delta R.T.: 0.012 min
Response: 158027
Conc: 1.40 ug/ml

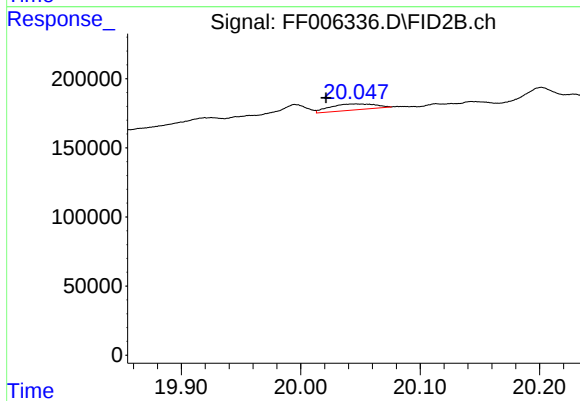

#16 N-HEXATRIACONTANE

R.T.: 20.046 min
Delta R.T.: 0.025 min
Response: 114023
Conc: 1.07 ug/ml

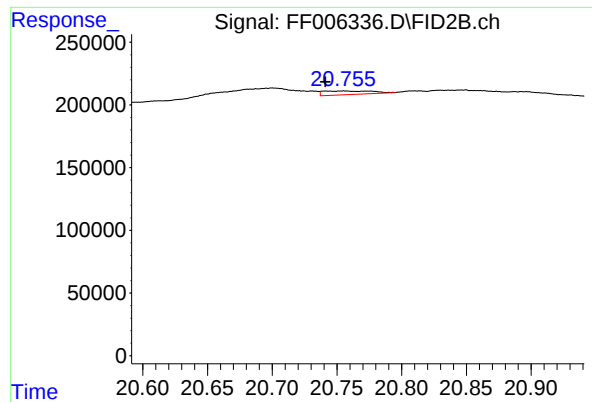

#17 N-OCTATRIACONTANE

R.T.: 20.756 min
Delta R.T.: 0.015 min
Response: 74663
Conc: 0.81 ug/ml

Instrument :
FID_F
ClientSampleId :