

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012820\
 Data File : FF006337.D
 Signal(s) : FID2B.ch
 Acq On : 28 Jan 2020 18:08
 Operator : DD\AJ
 Sample : L1265-01
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 29 00:32:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.628	1931820	17.828 ug/ml
Target Compounds			
3) N-DODECANE	6.401	95393	0.755 ug/ml
4) N-TETRADECANE	8.192	91405	0.724 ug/ml
5) N-HEXADECANE	9.790	86805	0.679 ug/ml
11) N-HEXACOSANE	15.848	94684	0.770 ug/ml
12) N-OCTACOSANE	16.796	288846	2.376 ug/ml
13) N-TRIACONTANE	17.682	376873	3.143 ug/ml
14) N-DOTRIACONTANE	18.511	515916	4.464 ug/ml
15) N-TETRATRIACONTANE	19.294	46744	0.415 ug/ml
16) N-HEXATRIACONTANE	19.998	576545	5.392 ug/ml
17) N-OCTATRIACONTANE	20.682f	280886	3.036 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012820\
Data File : FF006337.D
Signal(s) : FID2B.ch
Acq On : 28 Jan 2020 18:08
Operator : DD\AJ
Sample : L1265-01
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 29 00:32:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

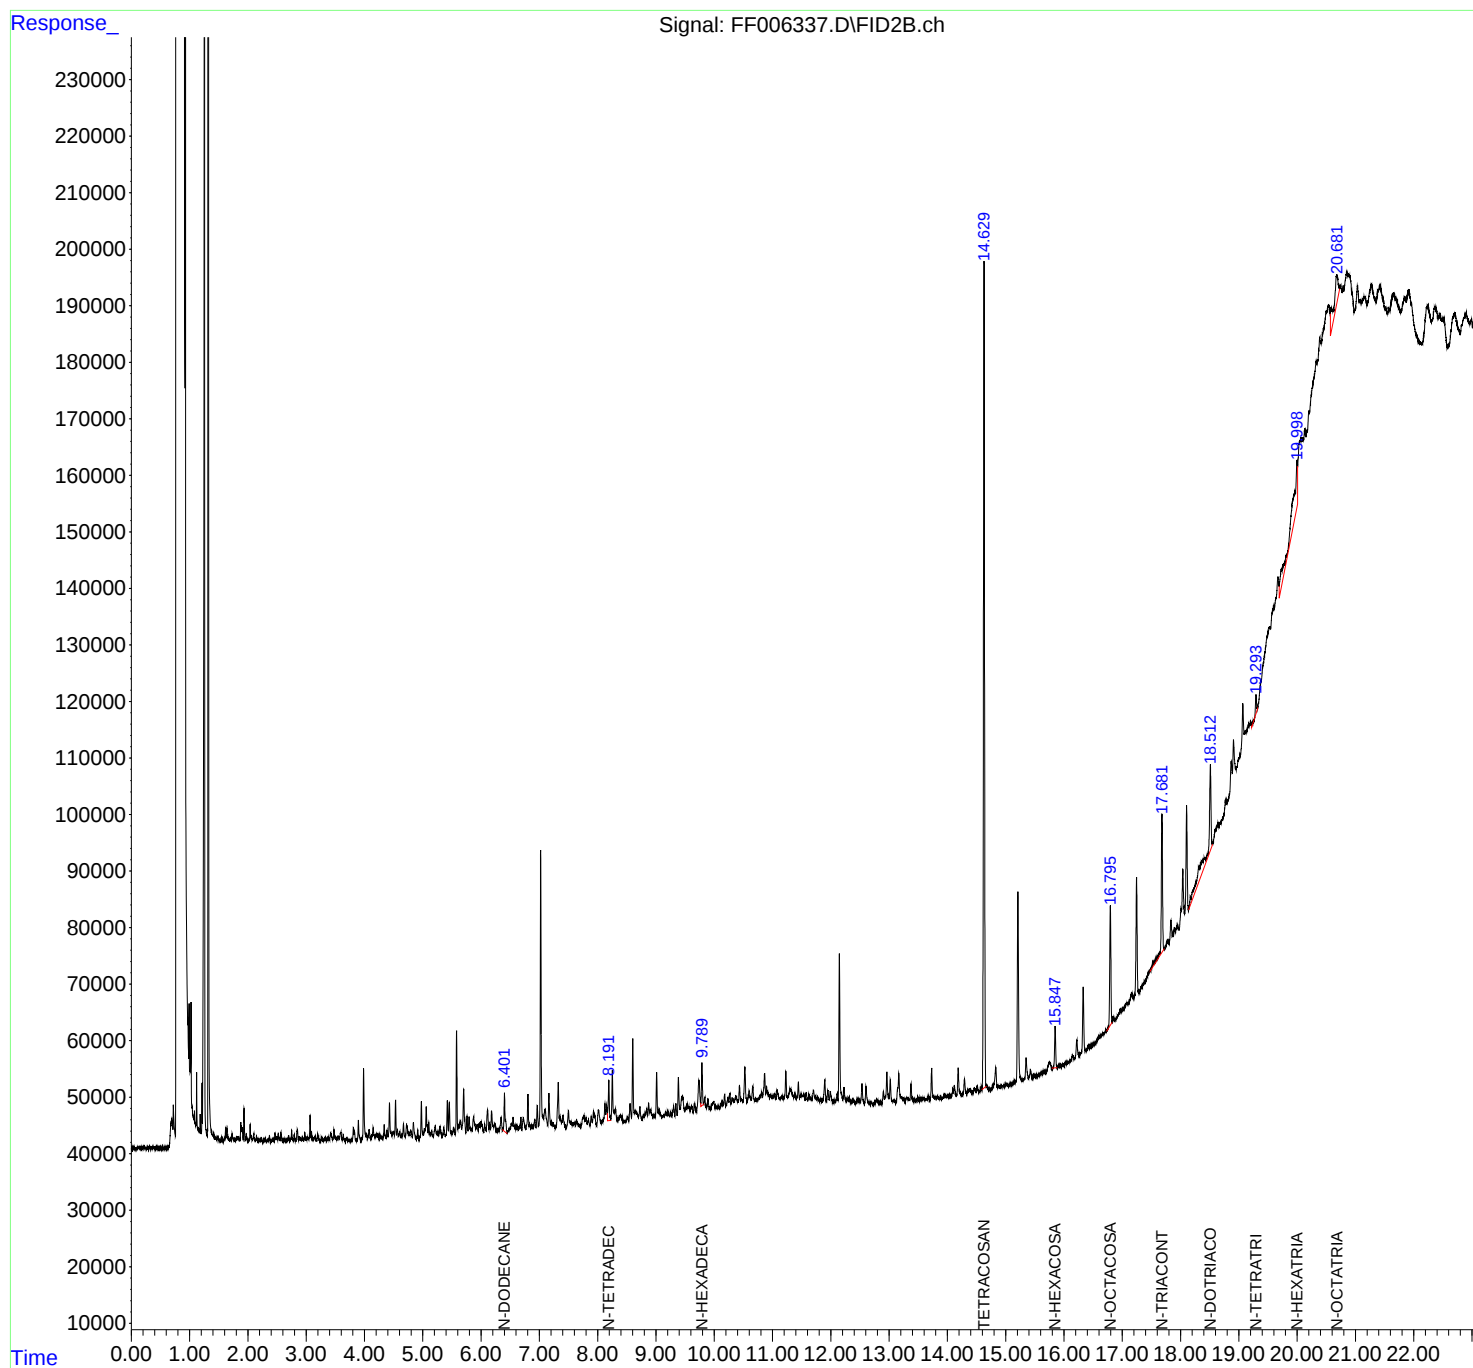


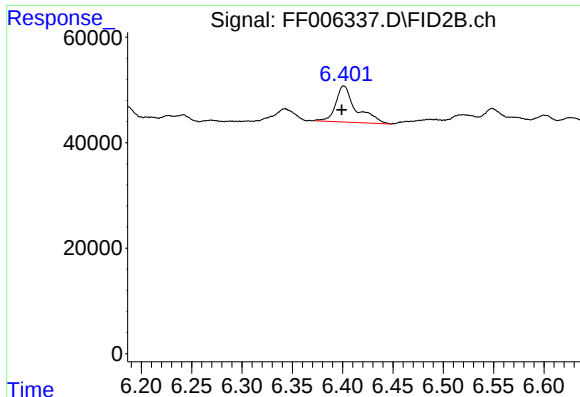

#3 N-DODECANE


R.T.: 6.401 min
Delta R.T.: 0.002 min
Response: 95393
Conc: 0.76 ug/ml

Instrument :
FID_F
ClientSampleId :

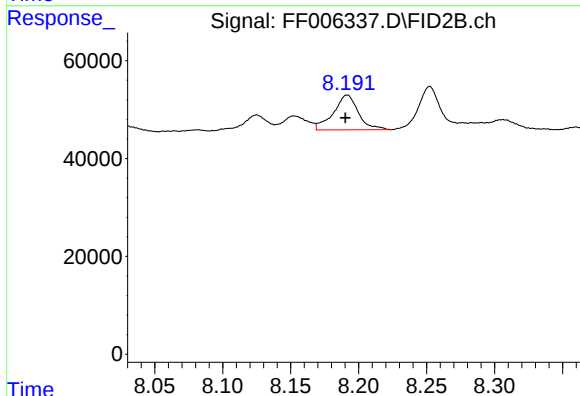


#4 N-TETRADECANE

R.T.: 8.192 min
Delta R.T.: 0.001 min
Response: 91405
Conc: 0.72 ug/ml

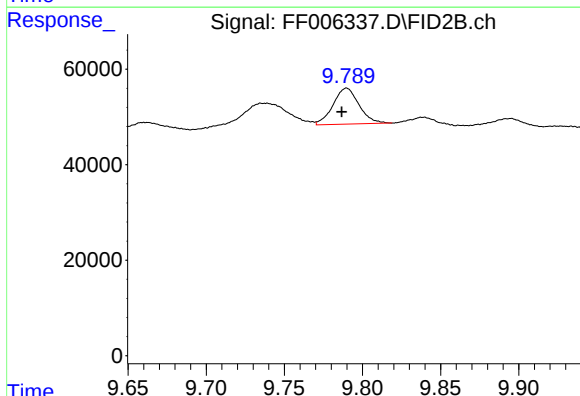


#5 N-HEXADECANE

R.T.: 9.790 min
Delta R.T.: 0.003 min
Response: 86805
Conc: 0.68 ug/ml

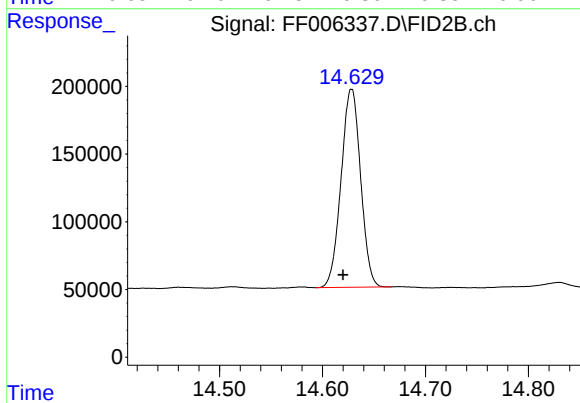

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.628 min
Delta R.T.: 0.008 min
Response: 1931820
Conc: 17.83 ug/ml

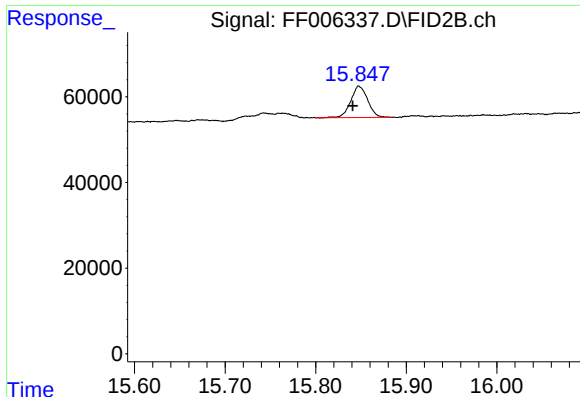

#11 N-HEXACOSANE


R.T.: 15.848 min
Delta R.T.: 0.007 min
Response: 94684
Conc: 0.77 ug/ml

Instrument :
FID_F
ClientSampleId :

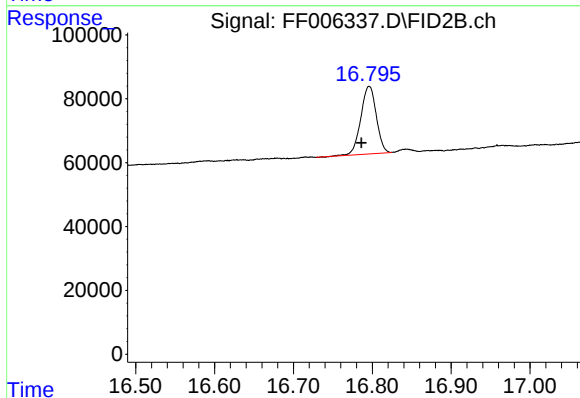


#12 N-OCTACOSANE

R.T.: 16.796 min
Delta R.T.: 0.010 min
Response: 288846
Conc: 2.38 ug/ml

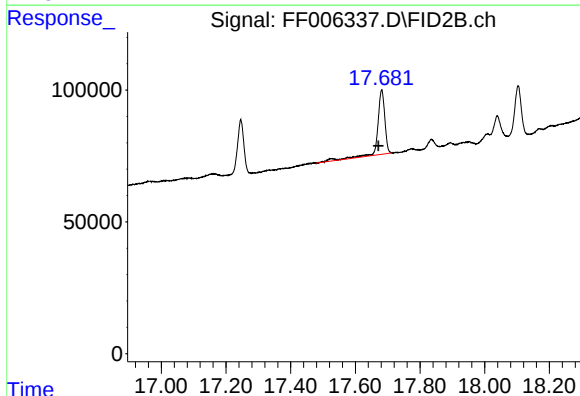


#13 N-TRIACONTANE

R.T.: 17.682 min
Delta R.T.: 0.010 min
Response: 376873
Conc: 3.14 ug/ml

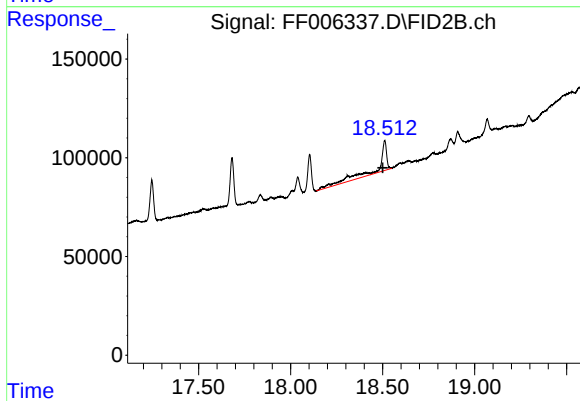

#14 N-DOTRIACONTANE


R.T.: 18.511 min
Delta R.T.: 0.010 min
Response: 515916
Conc: 4.46 ug/ml

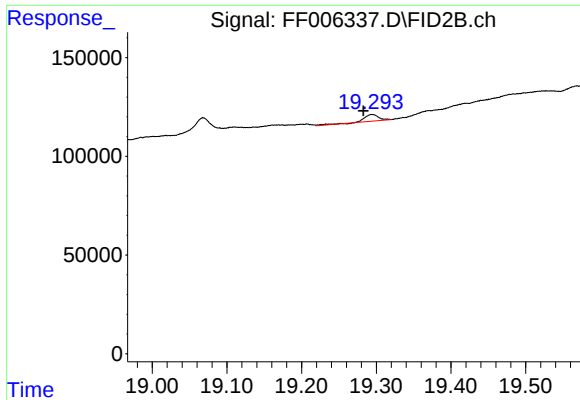

#15 N-TETRATRIACONTANE


R.T.: 19.294 min
Delta R.T.: 0.012 min
Response: 46744
Conc: 0.41 ug/ml

Instrument :
FID_F
ClientSampleId :

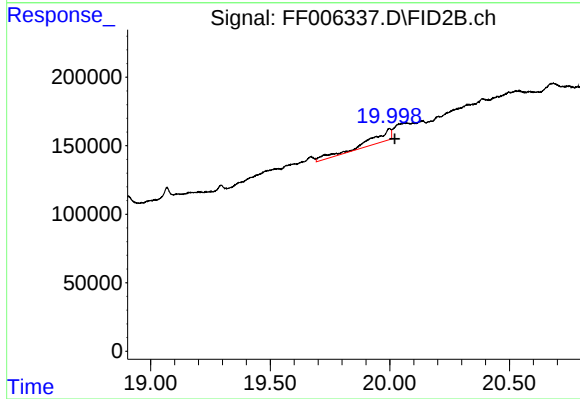

#16 N-HEXATRIACONTANE

R.T.: 19.998 min
Delta R.T.: -0.023 min
Response: 576545
Conc: 5.39 ug/ml

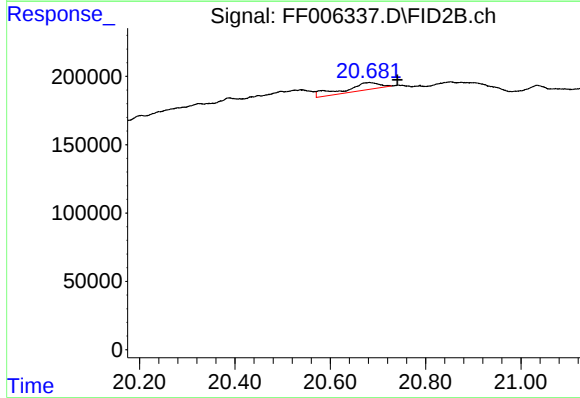

#17 N-OCTATRIACONTANE

R.T.: 20.682 min
Delta R.T.: -0.059 min
Response: 280886
Conc: 3.04 ug/ml