

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF012820\  
 Data File : FF006342.D  
 Signal(s) : FID2B.ch  
 Acq On : 28 Jan 2020 20:39  
 Operator : DD\AJ  
 Sample : L1265-02 50X  
 Misc :  
 ALS Vial : 69 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Jan 29 00:33:51 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF011020.M  
 Quant Title :  
 QLast Update : Fri Jan 10 12:35:13 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.    | Response | Conc Units  |
|-------------------------------|---------|----------|-------------|
| -----                         |         |          |             |
| System Monitoring Compounds   |         |          |             |
| 9) S TETRACOSANE-d50 (SURR... | 14.625  | 120873   | 1.115 ug/ml |
| Target Compounds              |         |          |             |
| 7) N-EICOSANE                 | 12.600f | 217742   | 1.704 ug/ml |
| 10) N-TETRACOSANE             | 14.816  | 161937   | 1.300 ug/ml |
| 12) N-OCTACOSANE              | 16.794  | 144473   | 1.188 ug/ml |
| 13) N-TRIACONTANE             | 17.680  | 193458   | 1.613 ug/ml |
| 14) N-DOTRIACONTANE           | 18.507  | 142268   | 1.231 ug/ml |
| 15) N-TETRATRIACONTANE        | 19.293  | 95583    | 0.848 ug/ml |
| 16) N-HEXATRIACONTANE         | 20.034  | 117659   | 1.100 ug/ml |
| -----                         |         |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF012820\  
Data File : FF006342.D  
Signal(s) : FID2B.ch  
Acq On : 28 Jan 2020 20:39  
Operator : DD\AJ  
Sample : L1265-02 50X  
Misc :  
ALS Vial : 69 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jan 29 00:33:51 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF011020.M  
Quant Title :  
QLast Update : Fri Jan 10 12:35:13 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

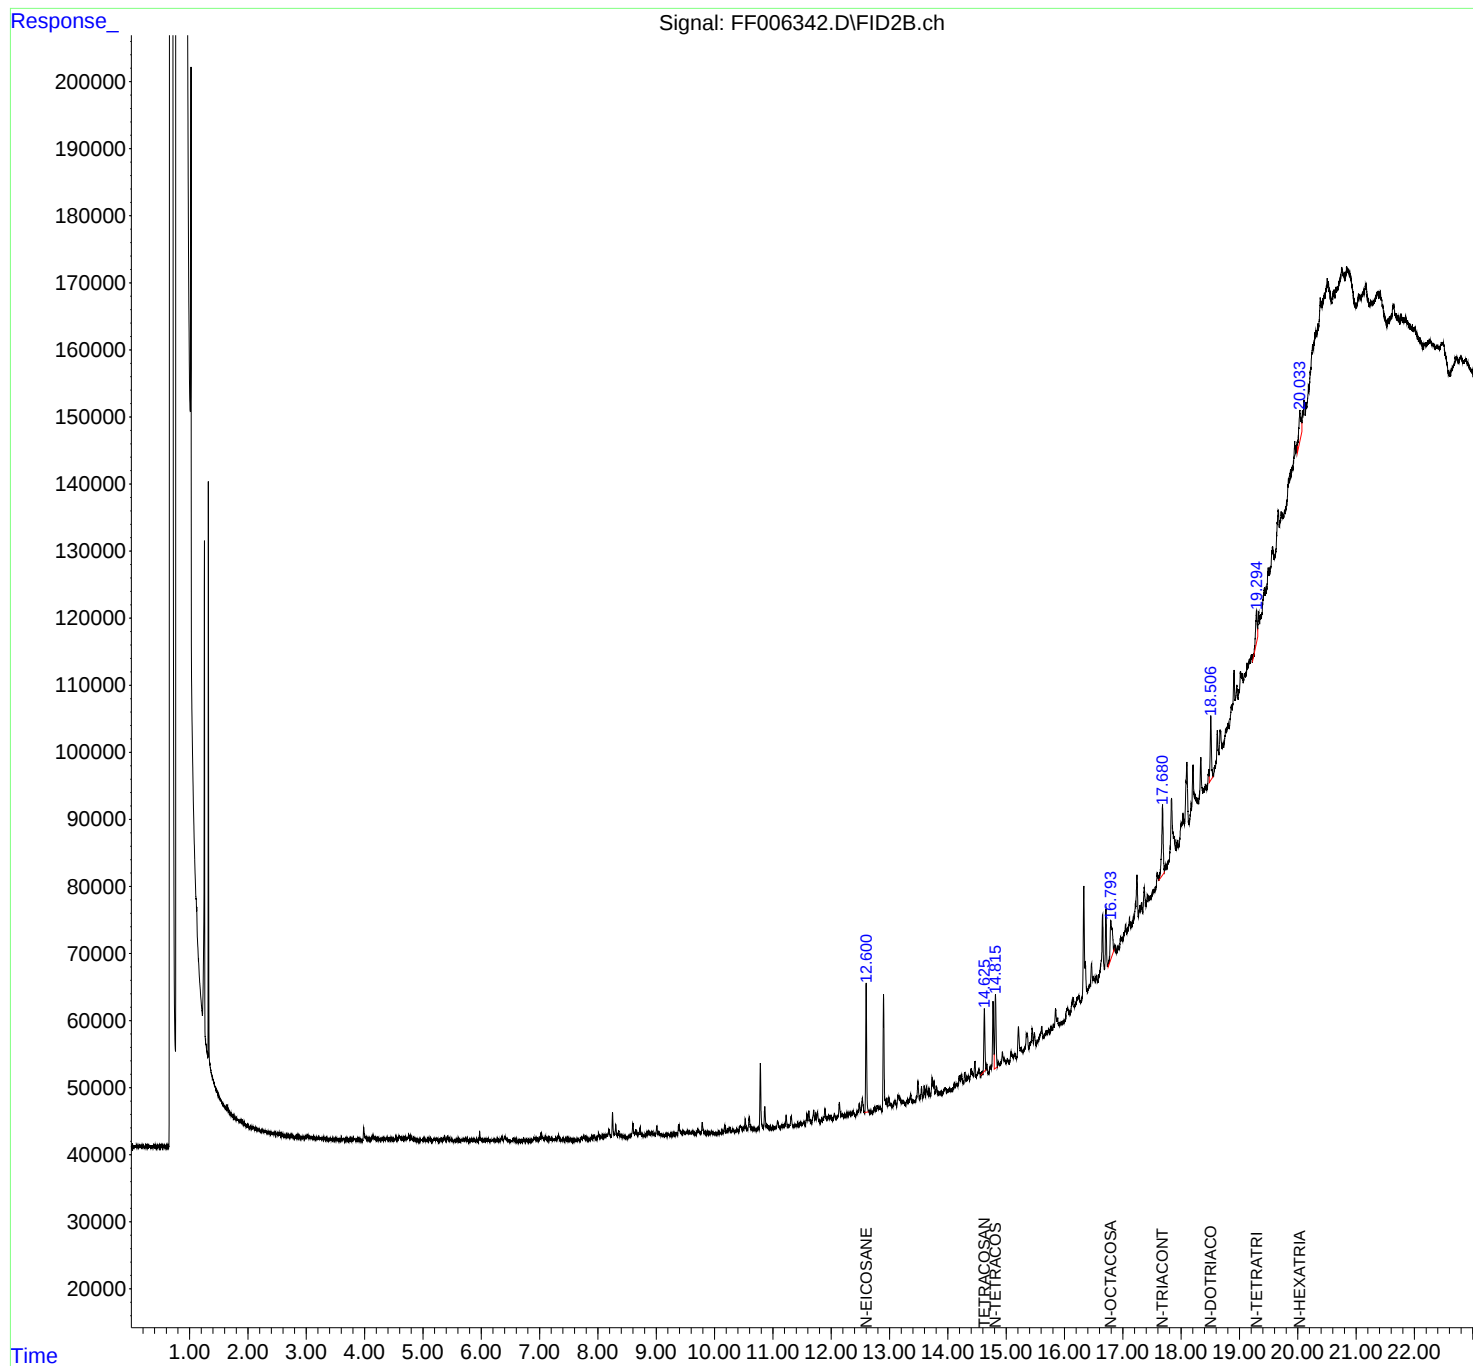


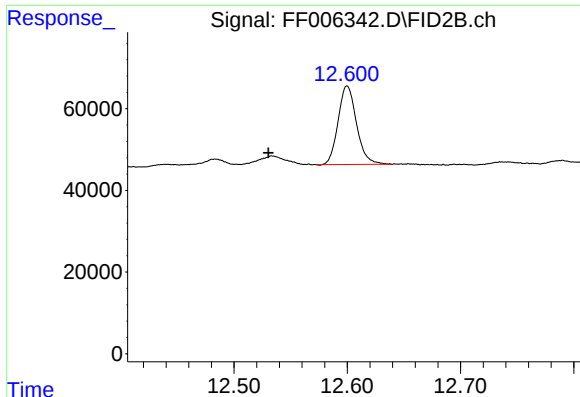

#7 N-EICOSANE


R.T.: 12.600 min  
Delta R.T.: 0.070 min  
Response: 217742  
Conc: 1.70 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

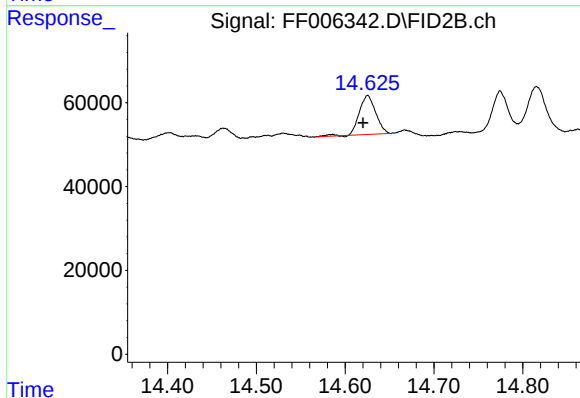


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.625 min  
Delta R.T.: 0.005 min  
Response: 120873  
Conc: 1.12 ug/ml

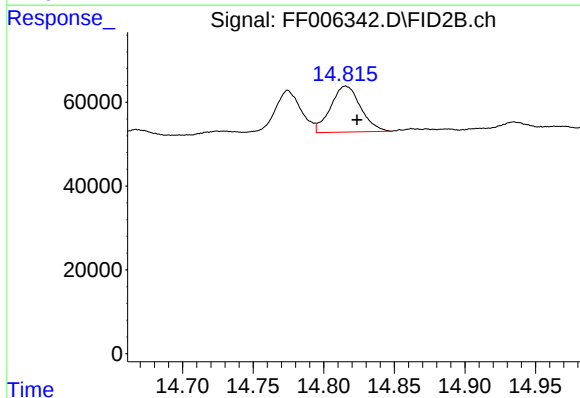


#10 N-TETRACOSANE

R.T.: 14.816 min  
Delta R.T.: -0.008 min  
Response: 161937  
Conc: 1.30 ug/ml

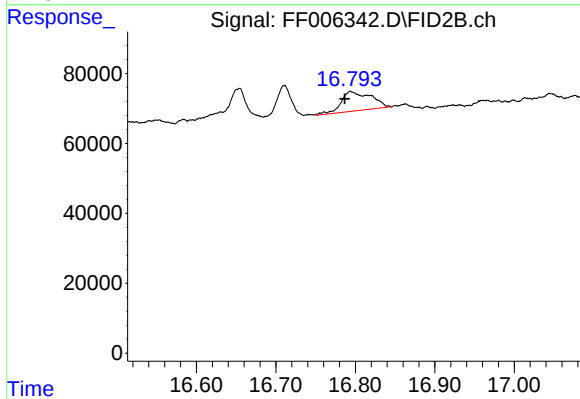

#12 N-OCTACOSANE


R.T.: 16.794 min  
Delta R.T.: 0.008 min  
Response: 144473  
Conc: 1.19 ug/ml

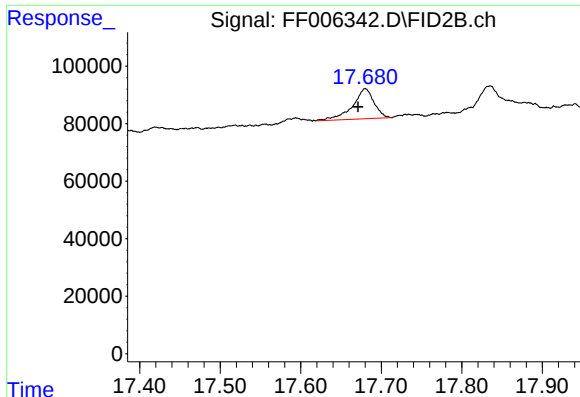

#13 N-TRIACONTANE


R.T.: 17.680 min  
Delta R.T.: 0.009 min  
Response: 193458  
Conc: 1.61 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

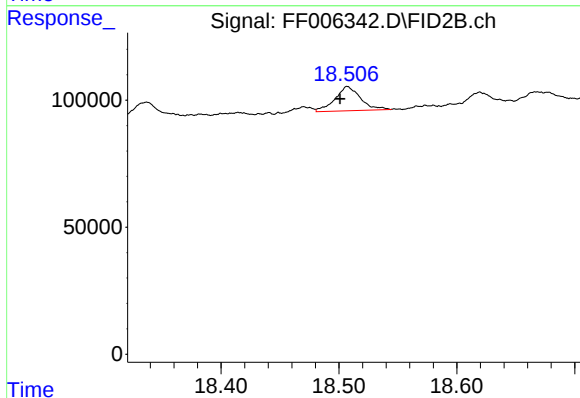


#14 N-DOTRIACONTANE

R.T.: 18.507 min  
Delta R.T.: 0.006 min  
Response: 142268  
Conc: 1.23 ug/ml

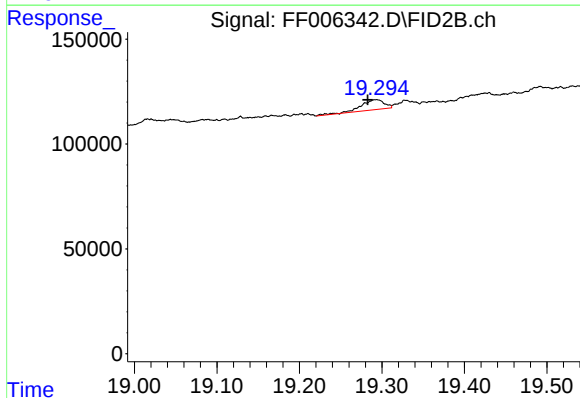

#15 N-TETRATRIACONTANE

R.T.: 19.293 min  
Delta R.T.: 0.010 min  
Response: 95583  
Conc: 0.85 ug/ml

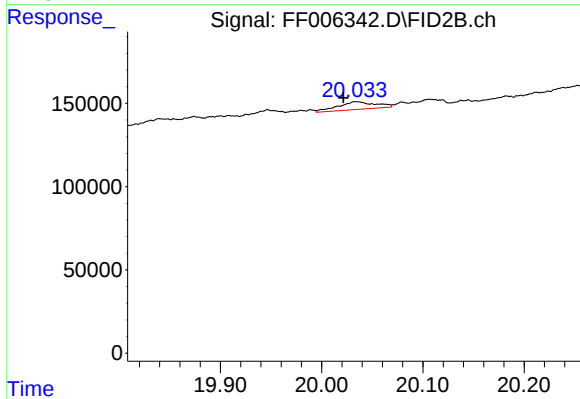

#16 N-HEXATRIACONTANE

R.T.: 20.034 min  
Delta R.T.: 0.013 min  
Response: 117659  
Conc: 1.10 ug/ml