

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012820\
 Data File : FF006343.D
 Signal(s) : FID2B.ch
 Acq On : 28 Jan 2020 21:10
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 29 00:34:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
 Quant Title :
 QLast Update : Fri Jan 10 12:35:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.626	2174377	20.066 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.507	93293	0.807 ug/ml
15) N-TETRATRIACONTANE	19.291	79751	0.708 ug/ml
17) N-OCTATRIACONTANE	20.749	481253	5.202 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012820\
Data File : FF006343.D
Signal(s) : FID2B.ch
Acq On : 28 Jan 2020 21:10
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 29 00:34:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

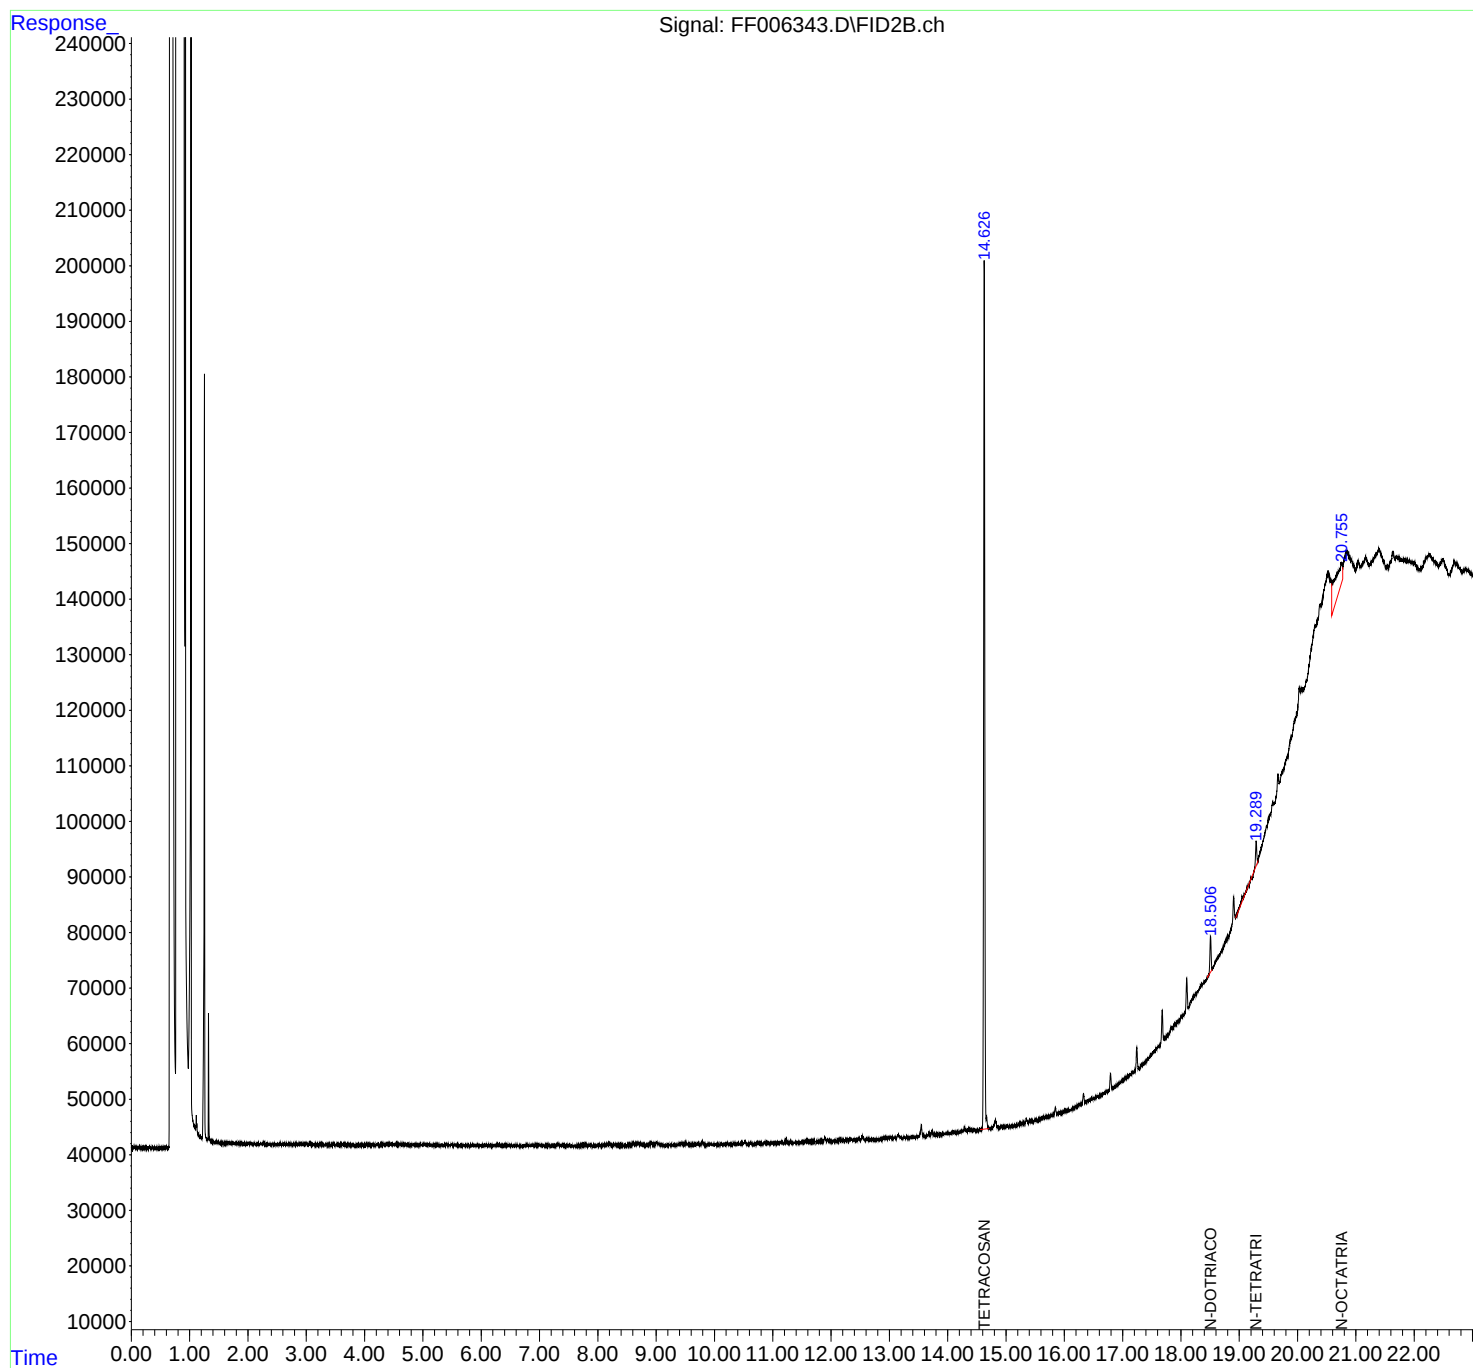


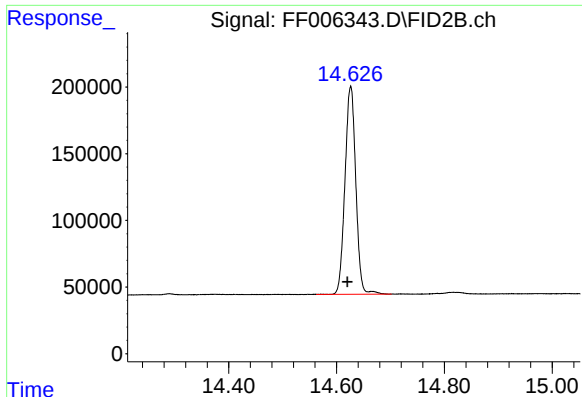

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.626 min
Delta R.T.: 0.006 min
Response: 2174377
Conc: 20.07 ug/ml

Instrument :
FID_F
ClientSampleId :

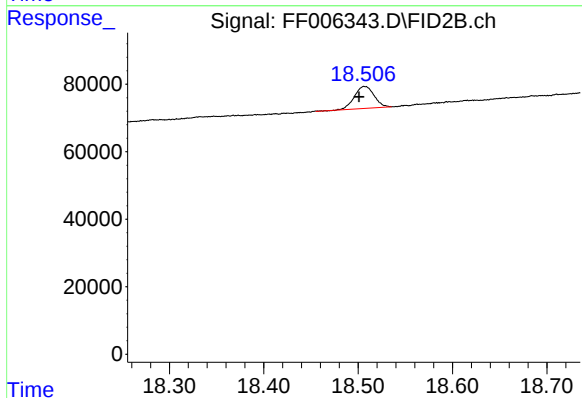


#14 N-DOTRIACONTANE

R.T.: 18.507 min
Delta R.T.: 0.006 min
Response: 93293
Conc: 0.81 ug/ml

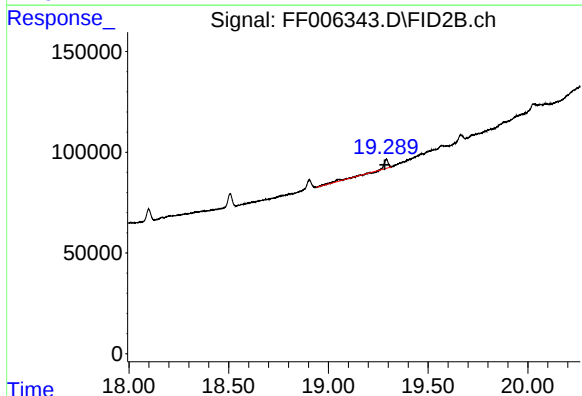

#15 N-TETRATRIACONTANE

R.T.: 19.291 min
Delta R.T.: 0.008 min
Response: 79751
Conc: 0.71 ug/ml

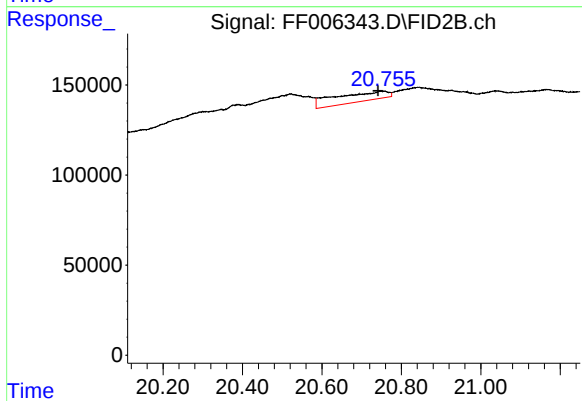

#17 N-OCTATRIACONTANE

R.T.: 20.749 min
Delta R.T.: 0.007 min
Response: 481253
Conc: 5.20 ug/ml