

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012820\
Data File : FF006328.D
Signal(s) : FID2B.ch
Acq On : 28 Jan 2020 13:36
Operator : DD\AJ
Sample : L1263-04
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CTY-SB-0203-0-11

Integration File: autoint1.e
Quant Time: Jan 29 00:30:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.627	1746283	16.116 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012820\
Data File : FF006328.D
Signal(s) : FID2B.ch
Acq On : 28 Jan 2020 13:36
Operator : DD\AJ
Sample : L1263-04
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CTY-SB-0203-0-11

Integration File: autoint1.e
Quant Time: Jan 29 00:30:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011020.M
Quant Title :
QLast Update : Fri Jan 10 12:35:13 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

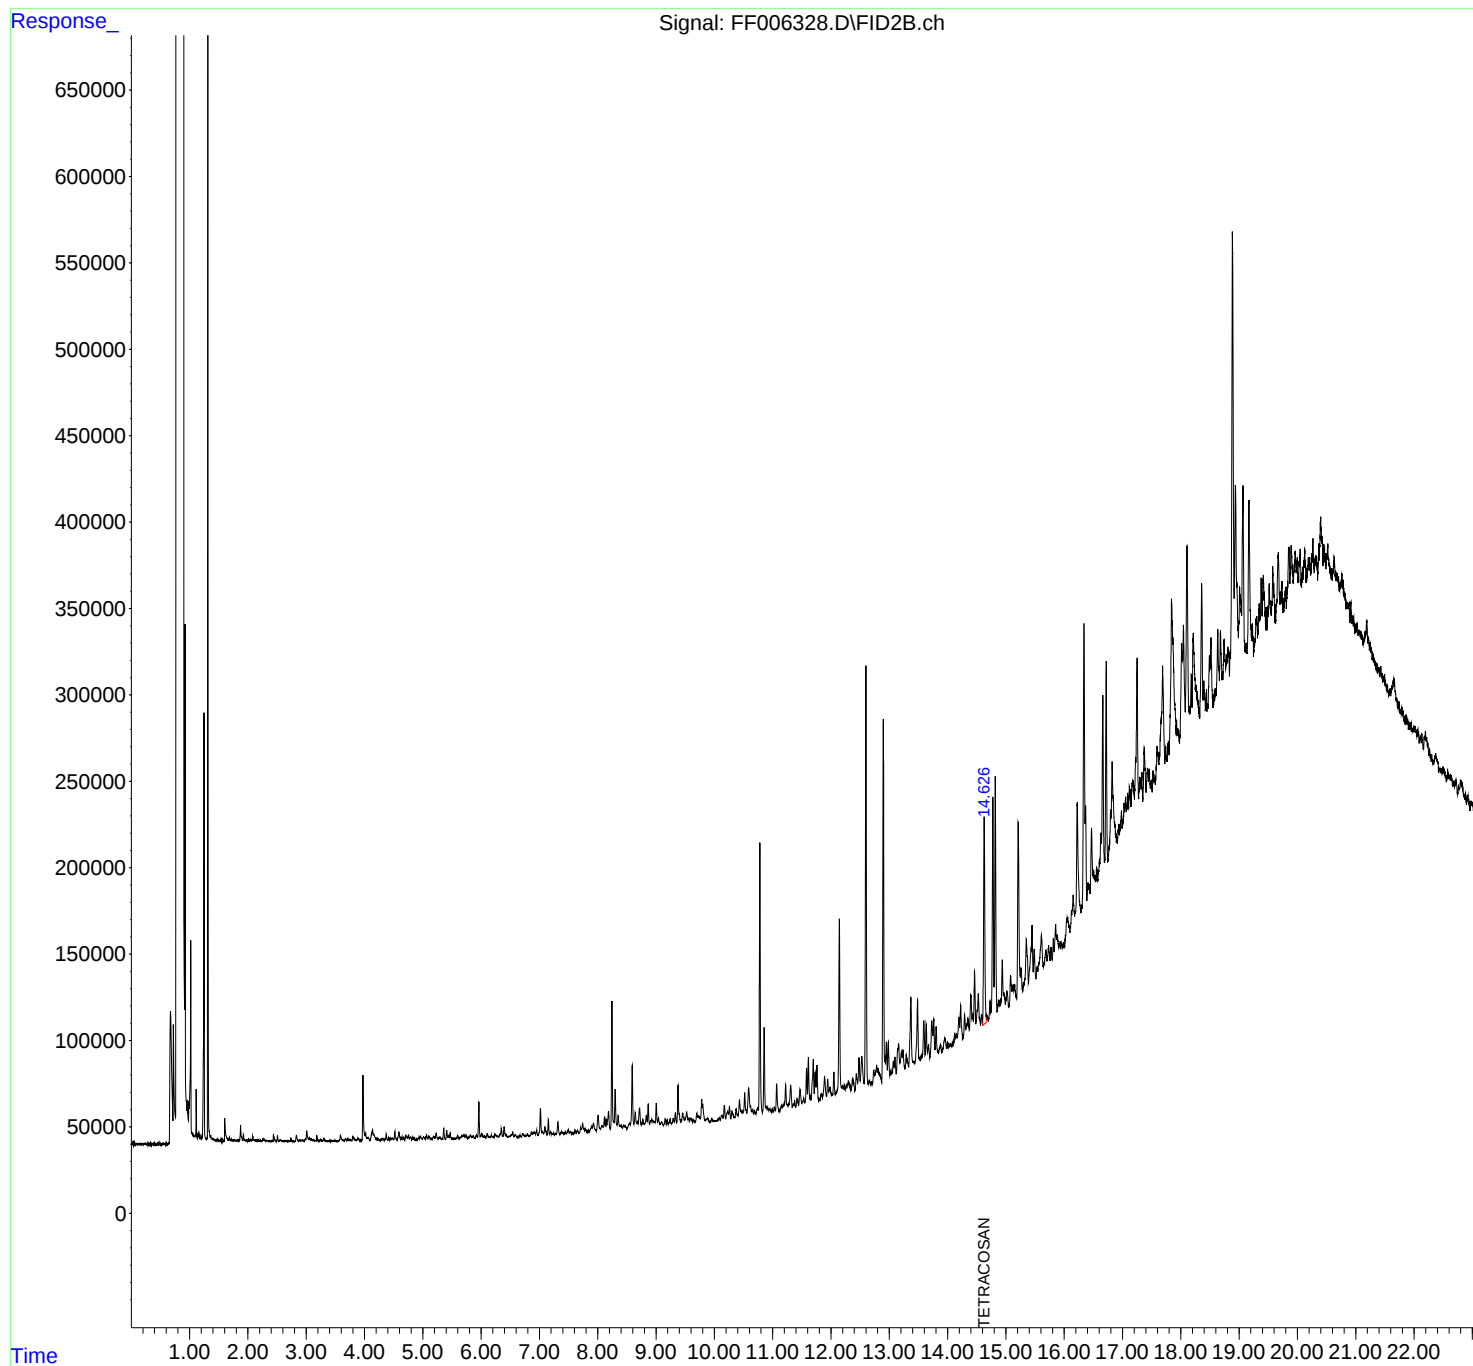

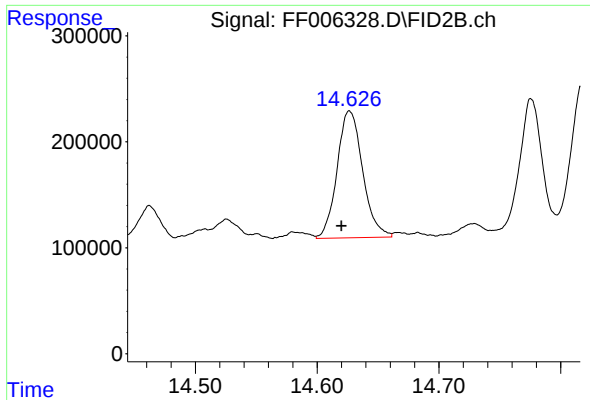

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.627 min
Delta R.T.: 0.006 min
Response: 1746283
Conc: 16.12 ug/ml

Instrument :
FID_F
ClientSampleId :
CTY-SB-0203-0-11