

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012825AR\
Data File : FF015323.D
Signal(s) : FID2B.ch
Acq On : 28 Jan 2025 10:57
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 29 00:45:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aromatic EPH 011425.M
Quant Title : GC Extractables
QLast Update : Wed Jan 15 07:05:42 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
19) T	Indeno[1,2,3-cd]pyren...	18.522	19982	0.159 ug/ml
20) T	Dibenz[a,h]anthracene...	18.522	19982	0.135 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF012825AR\
Data File : FF015323.D
Signal(s) : FID2B.ch
Acq On : 28 Jan 2025 10:57
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 29 00:45:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aromatic EPH 011425.M
Quant Title : GC Extractables
QLast Update : Wed Jan 15 07:05:42 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

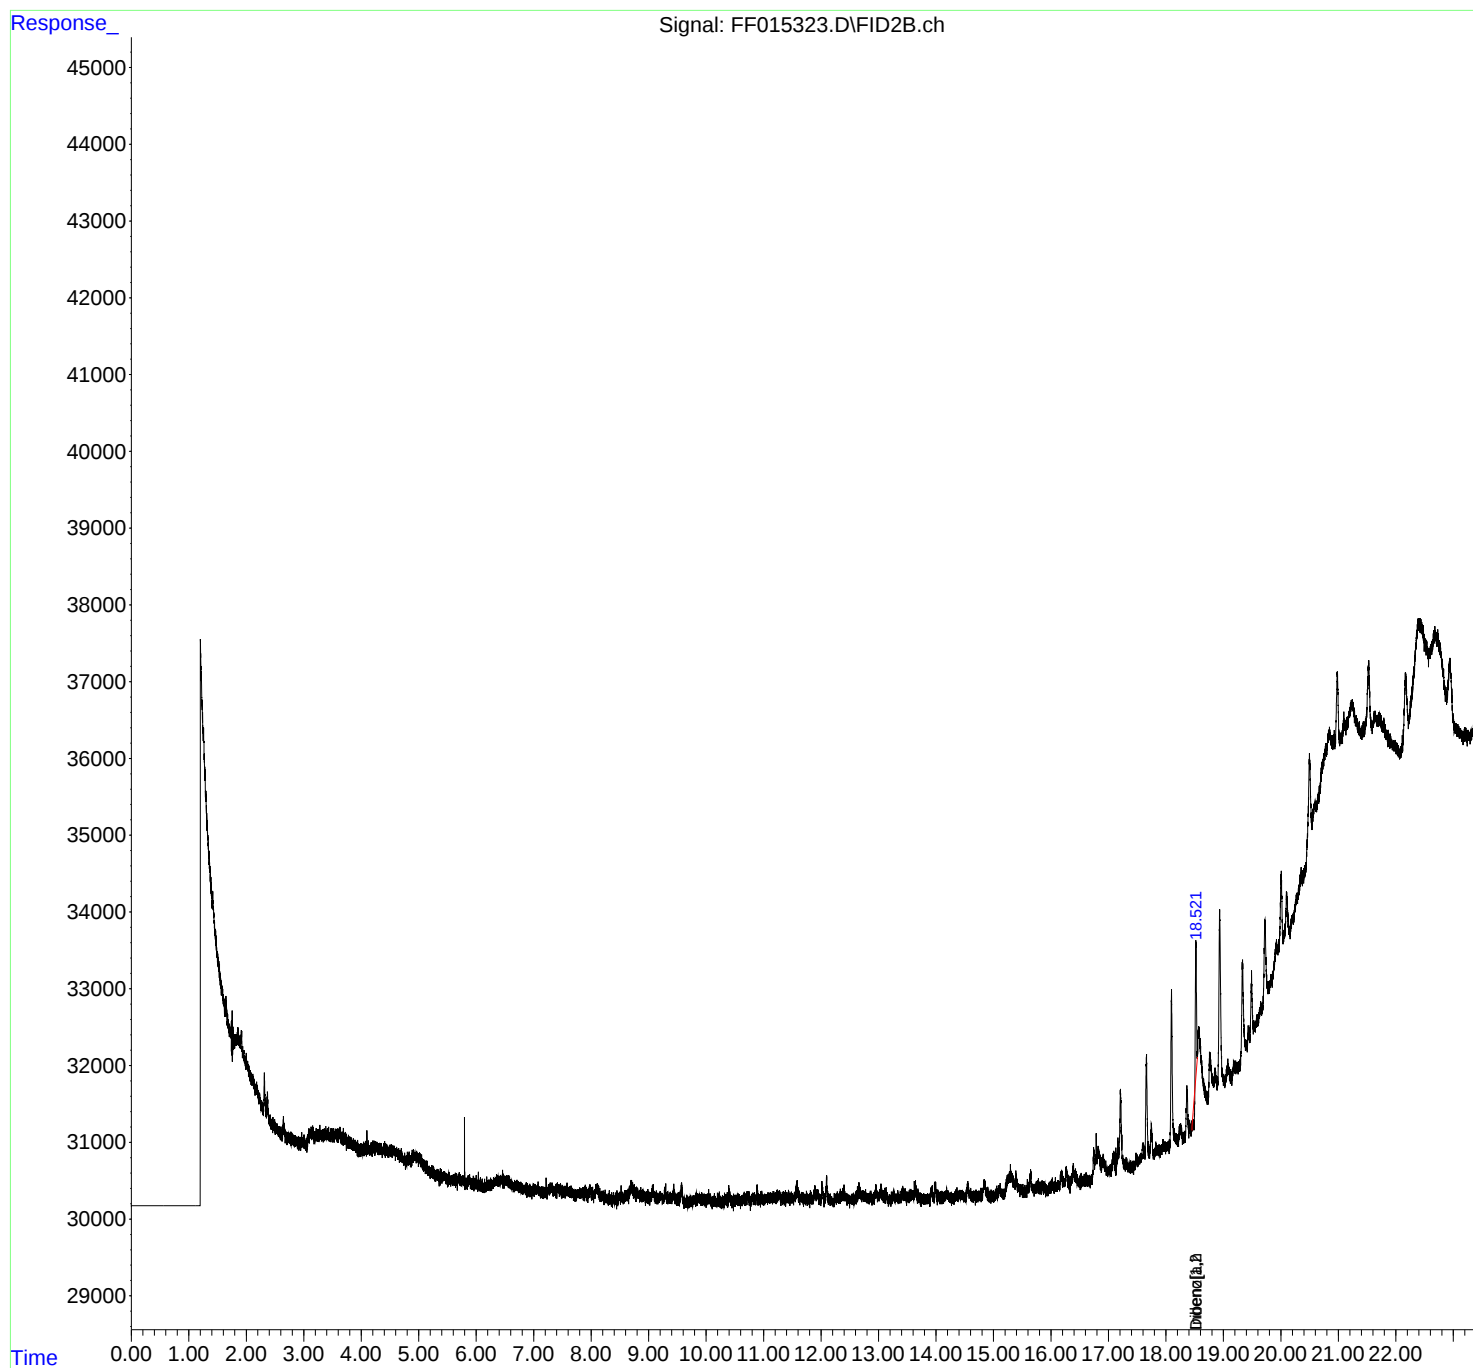


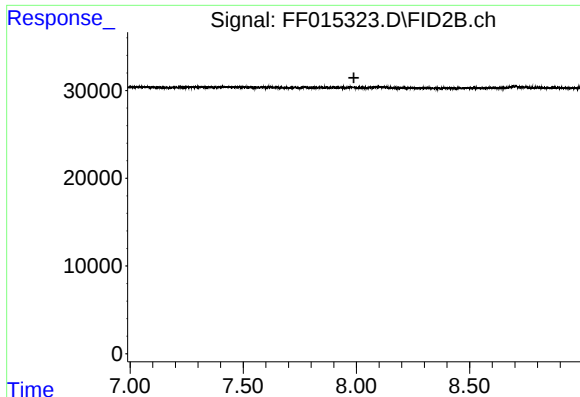

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T. : 7.989 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

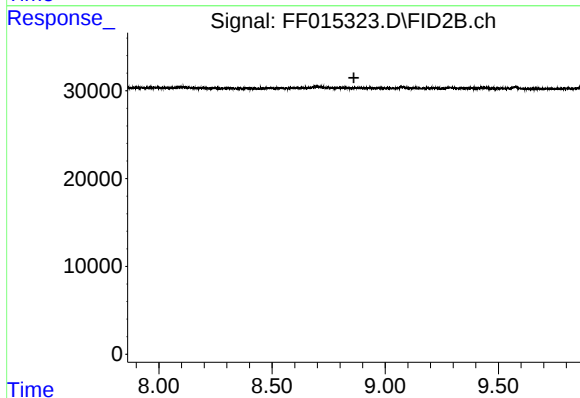


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 8.862 min
Response: 0
Conc: N.D.

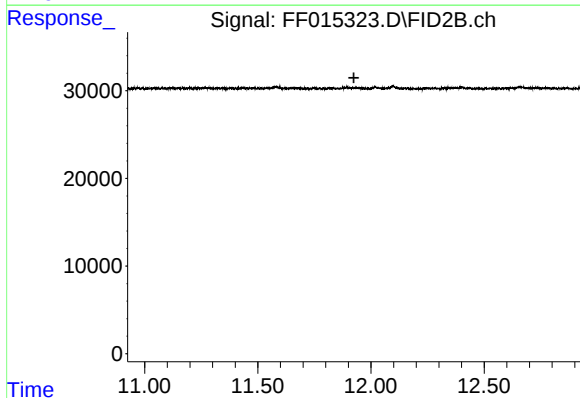


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.924 min
Response: 0
Conc: N.D.

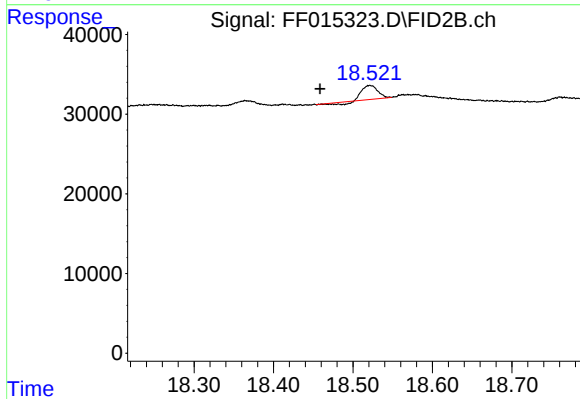

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 18.522 min
Delta R.T.: 0.063 min
Response: 19982
Conc: 0.16 ug/ml

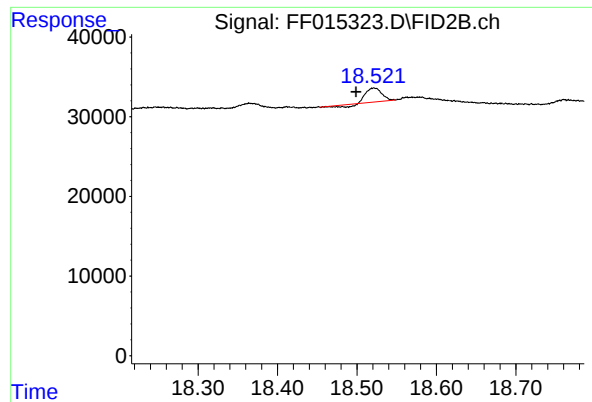

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 18.522 min
Delta R.T.: 0.023 min
Response: 19982
Conc: 0.14 ug/ml

Instrument :

FID_F

ClientSampleId :