

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020119\
 Data File : FF003350.D
 Signal(s) : FID2B.ch
 Acq On : 01 Feb 2019 16:31
 Operator : AJ\SJ
 Sample : 50 TRPH STD
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 01 22:52:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
 Quant Title :
 QLast Update : Fri Feb 01 22:50:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.613	5698059	50.000 ug/ml
Target Compounds			
1) N-OCTANE	2.246	6317203	50.000 ug/ml
2) N-DECANE	4.343	6388536	50.000 ug/ml
3) N-DODECANE	6.364	6446245	50.000 ug/ml
4) N-TETRADECANE	8.155	6481617	50.000 ug/ml
5) N-HEXADECANE	9.755	6535130	50.000 ug/ml
6) N-OCTADECANE	11.199	6568006	50.000 ug/ml
7) N-EICOSANE	12.510	6516471	50.000 ug/ml
8) N-DOCOSANE	13.711	6462596	50.000 ug/ml
10) N-TETRACOSANE	14.818	6405345	50.000 ug/ml
11) N-HEXACOSANE	15.842	6386111	50.000 ug/ml
12) N-OCTACOSANE	16.797	6396422	50.000 ug/ml
13) N-TRIACONTANE	17.687	6453946	50.000 ug/ml
14) N-DOTRIACONTANE	18.525	6222149	50.000 ug/ml
15) N-TETRATRIACONTANE	19.313	5932789	50.000 ug/ml
16) N-HEXATRIACONTANE	20.059	5645898	50.000 ug/ml
17) N-OCTATRIACONTANE	20.798	5067661	50.000 ug/ml
18) N-TETRACONTANE	21.694	5000023	50.000 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020119\
Data File : FF003350.D
Signal(s) : FID2B.ch
Acq On : 01 Feb 2019 16:31
Operator : AJ\SJ
Sample : 50 TRPH STD
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 01 22:52:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:50:23 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

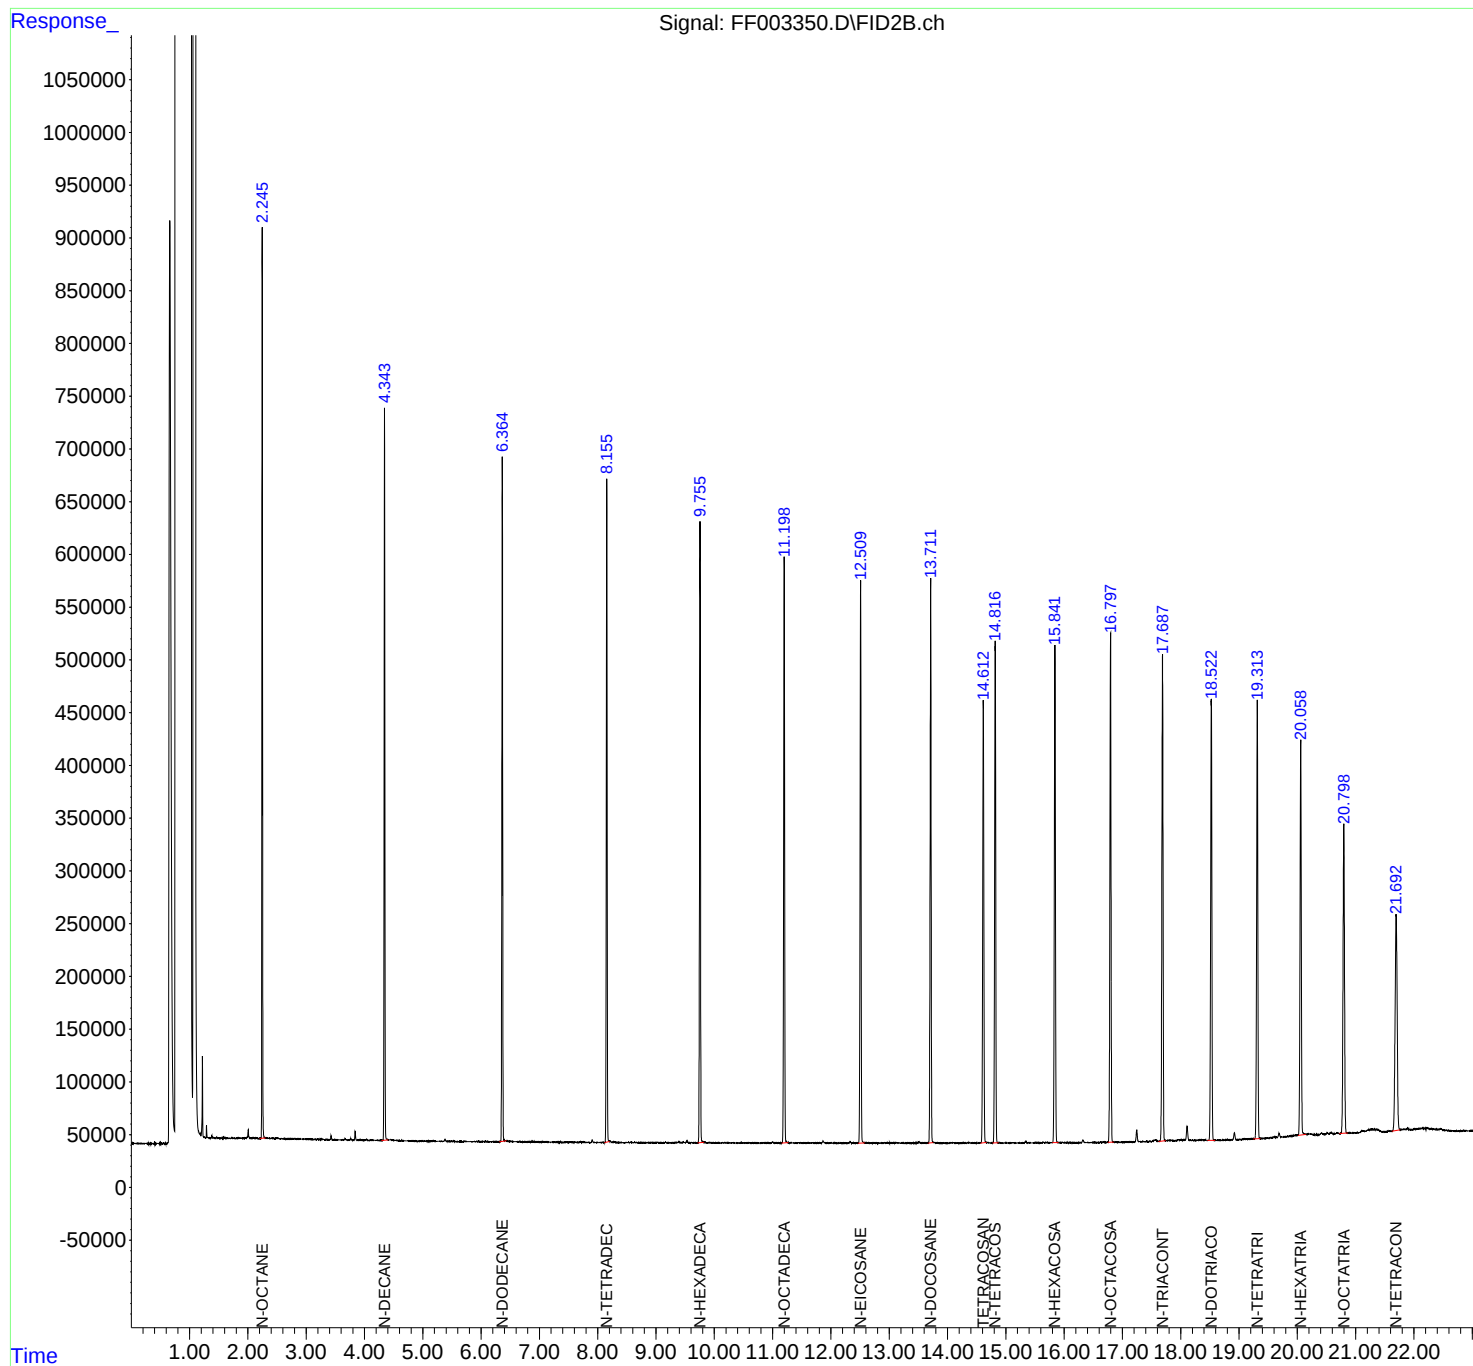

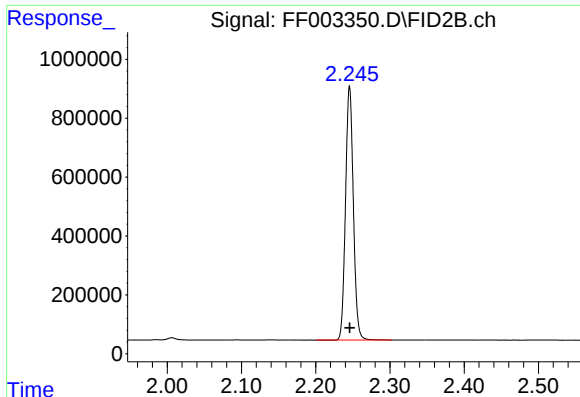


#1 N-OCTANE

R.T.: 2.246 min
Delta R.T.: 0.000 min
Response: 6317203
Conc: 50.00 ug/ml

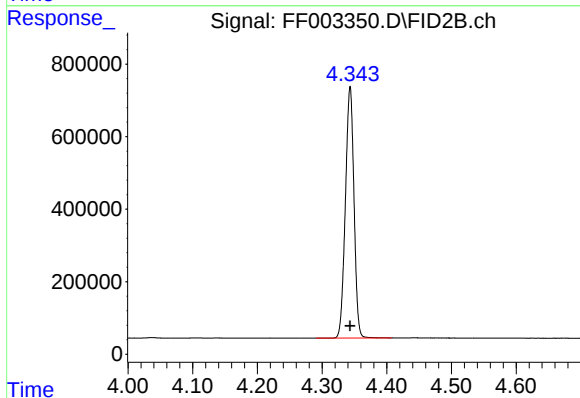


#2 N-DECANE

R.T.: 4.343 min
Delta R.T.: 0.000 min
Response: 6388536
Conc: 50.00 ug/ml

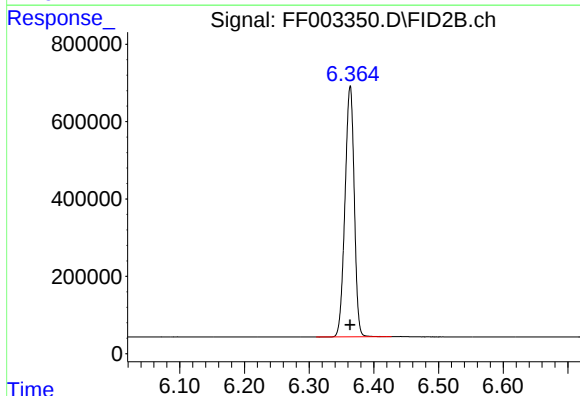


#3 N-DODECANE

R.T.: 6.364 min
Delta R.T.: 0.000 min
Response: 6446245
Conc: 50.00 ug/ml

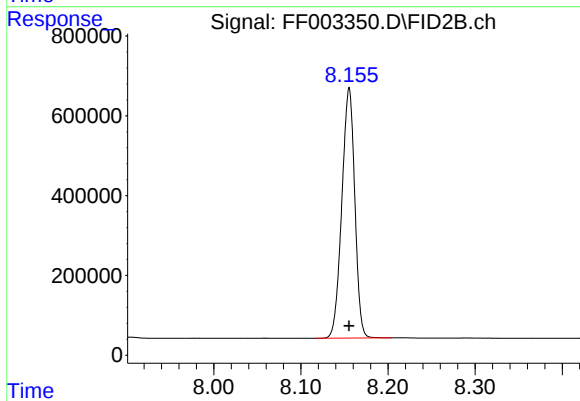


#4 N-TETRADECANE

R.T.: 8.155 min
Delta R.T.: 0.000 min
Response: 6481617
Conc: 50.00 ug/ml

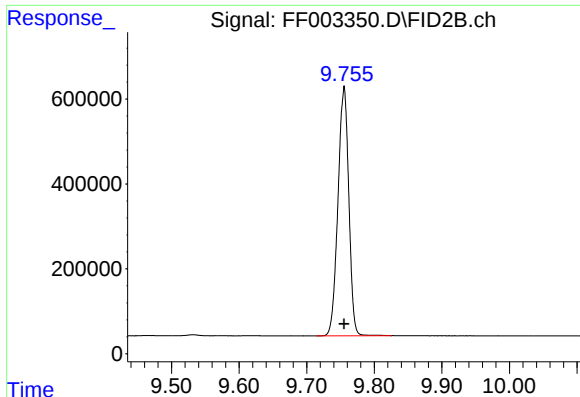


#5 N-HEXADECANE

R.T.: 9.755 min
Delta R.T.: 0.000 min
Response: 6535130
Conc: 50.00 ug/ml

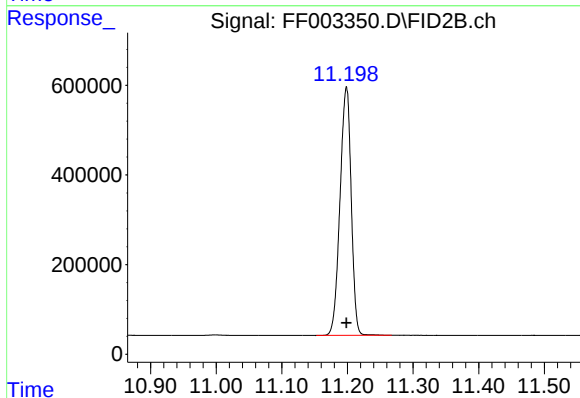


#6 N-OCTADECANE

R.T.: 11.199 min
Delta R.T.: 0.000 min
Response: 6568006
Conc: 50.00 ug/ml

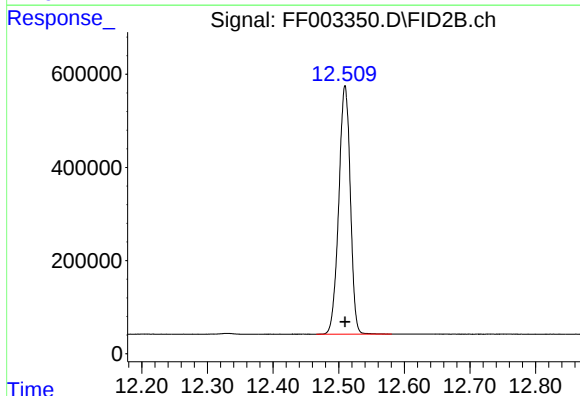


#7 N-EICOSANE

R.T.: 12.510 min
Delta R.T.: 0.000 min
Response: 6516471
Conc: 50.00 ug/ml

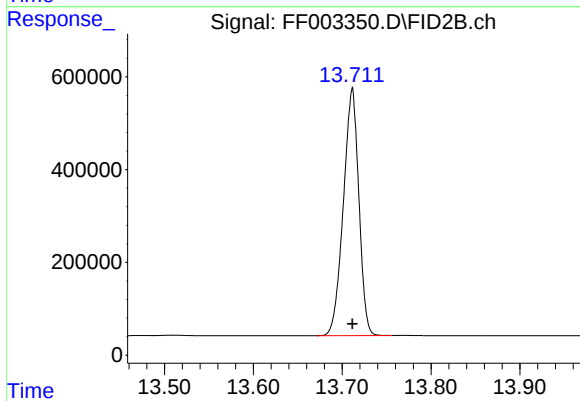


#8 N-DOCOSANE

R.T.: 13.711 min
Delta R.T.: 0.000 min
Response: 6462596
Conc: 50.00 ug/ml

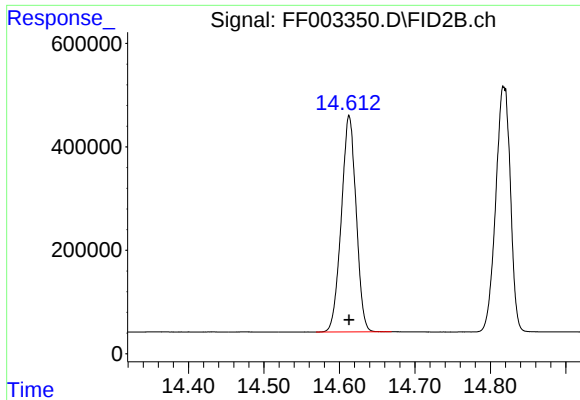


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.613 min
Delta R.T.: 0.000 min
Response: 5698059
Conc: 50.00 ug/ml

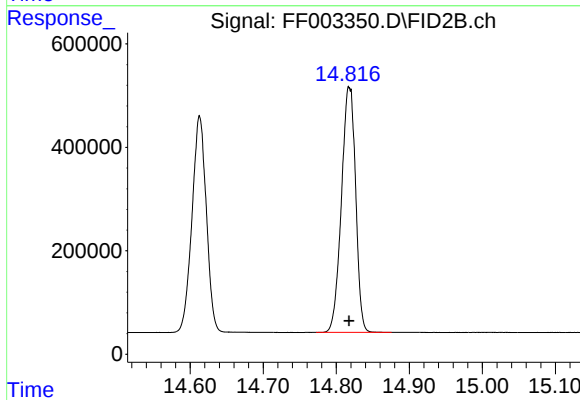


#10 N-TETRACOSANE

R.T.: 14.818 min
Delta R.T.: 0.000 min
Response: 6405345
Conc: 50.00 ug/ml

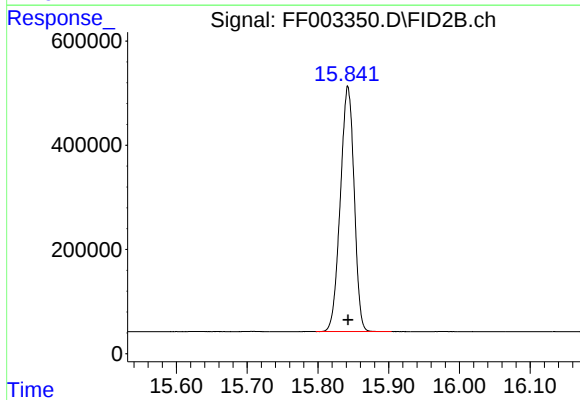


#11 N-HEXACOSANE

R.T.: 15.842 min
Delta R.T.: 0.000 min
Response: 6386111
Conc: 50.00 ug/ml

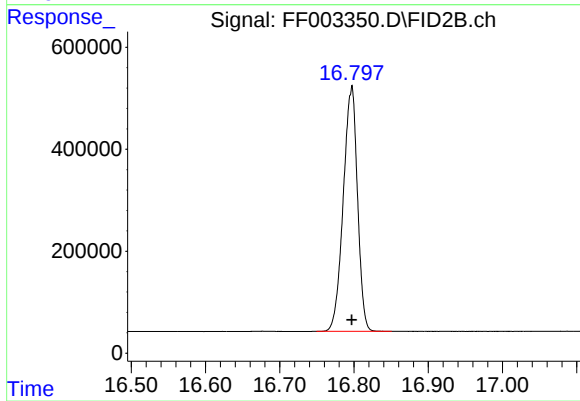


#12 N-OCTACOSANE

R.T.: 16.797 min
Delta R.T.: 0.000 min
Response: 6396422
Conc: 50.00 ug/ml

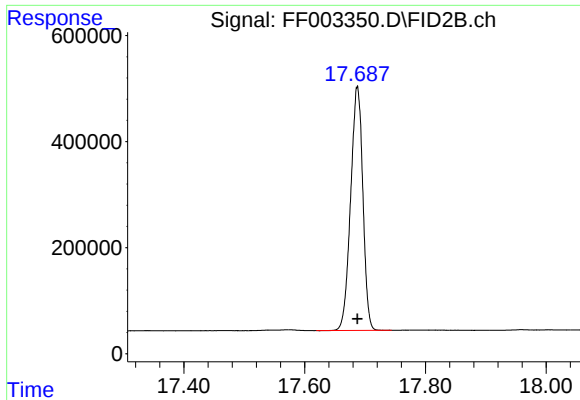


#13 N-TRIACONTANE

R.T.: 17.687 min
Delta R.T.: 0.000 min
Response: 6453946
Conc: 50.00 ug/ml

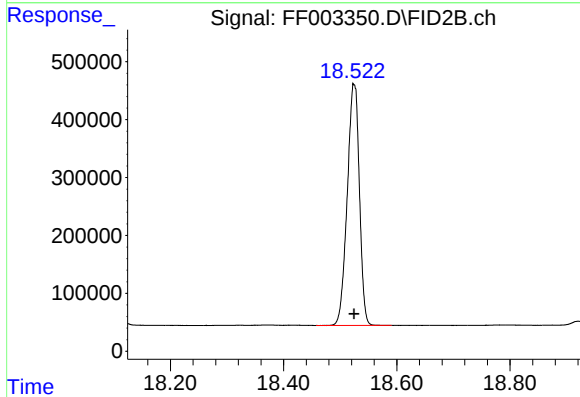


#14 N-DOTRIACONTANE

R.T.: 18.525 min
Delta R.T.: 0.000 min
Response: 6222149
Conc: 50.00 ug/ml

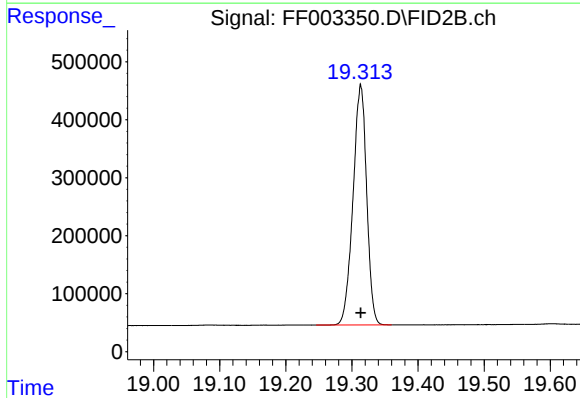


#15 N-TETRATRIACONTANE

R.T.: 19.313 min
Delta R.T.: 0.000 min
Response: 5932789
Conc: 50.00 ug/ml

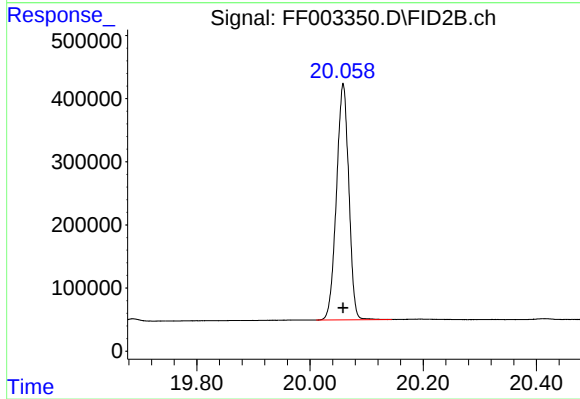


#16 N-HEXATRIACONTANE

R.T.: 20.059 min
Delta R.T.: 0.000 min
Response: 5645898
Conc: 50.00 ug/ml

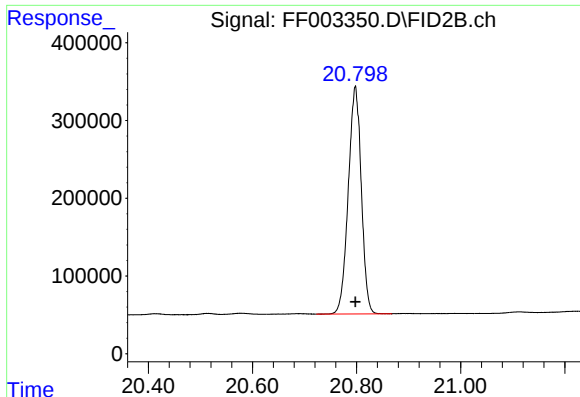

#17 N-OCTATRIACONTANE

R.T.: 20.798 min
Delta R.T.: 0.000 min
Response: 5067661
Conc: 50.00 ug/ml

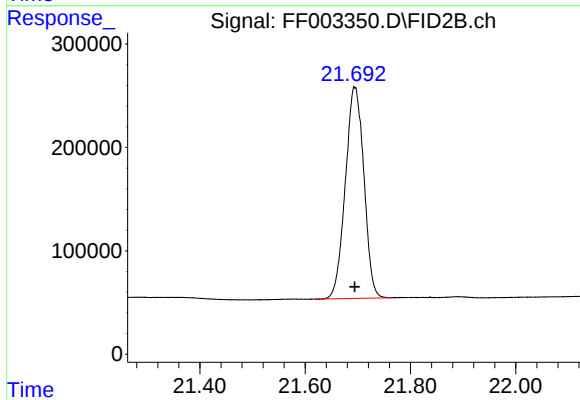

#18 N-TETRACONTANE

R.T.: 21.694 min
Delta R.T.: 0.000 min
Response: 5000023
Conc: 50.00 ug/ml