

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020122\
Data File : FF009818.D
Signal(s) : FID2B.ch
Acq On : 01 Feb 2022 09:30
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 02 01:58:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

13)	N-TRIACONTANE	17.478	69330	0.485 ug/ml
14)	N-DOTRIACONTANE	18.309	162847	1.197 ug/ml
15)	N-TETRATRIACONTANE	19.090	130939	1.102 ug/ml
16)	N-HEXATRIACONTANE	19.868	250251	2.427 ug/ml
18)	N-TETRACONTANE	21.374	145493	1.602 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020122\
Data File : FF009818.D
Signal(s) : FID2B.ch
Acq On : 01 Feb 2022 09:30
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 02 01:58:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

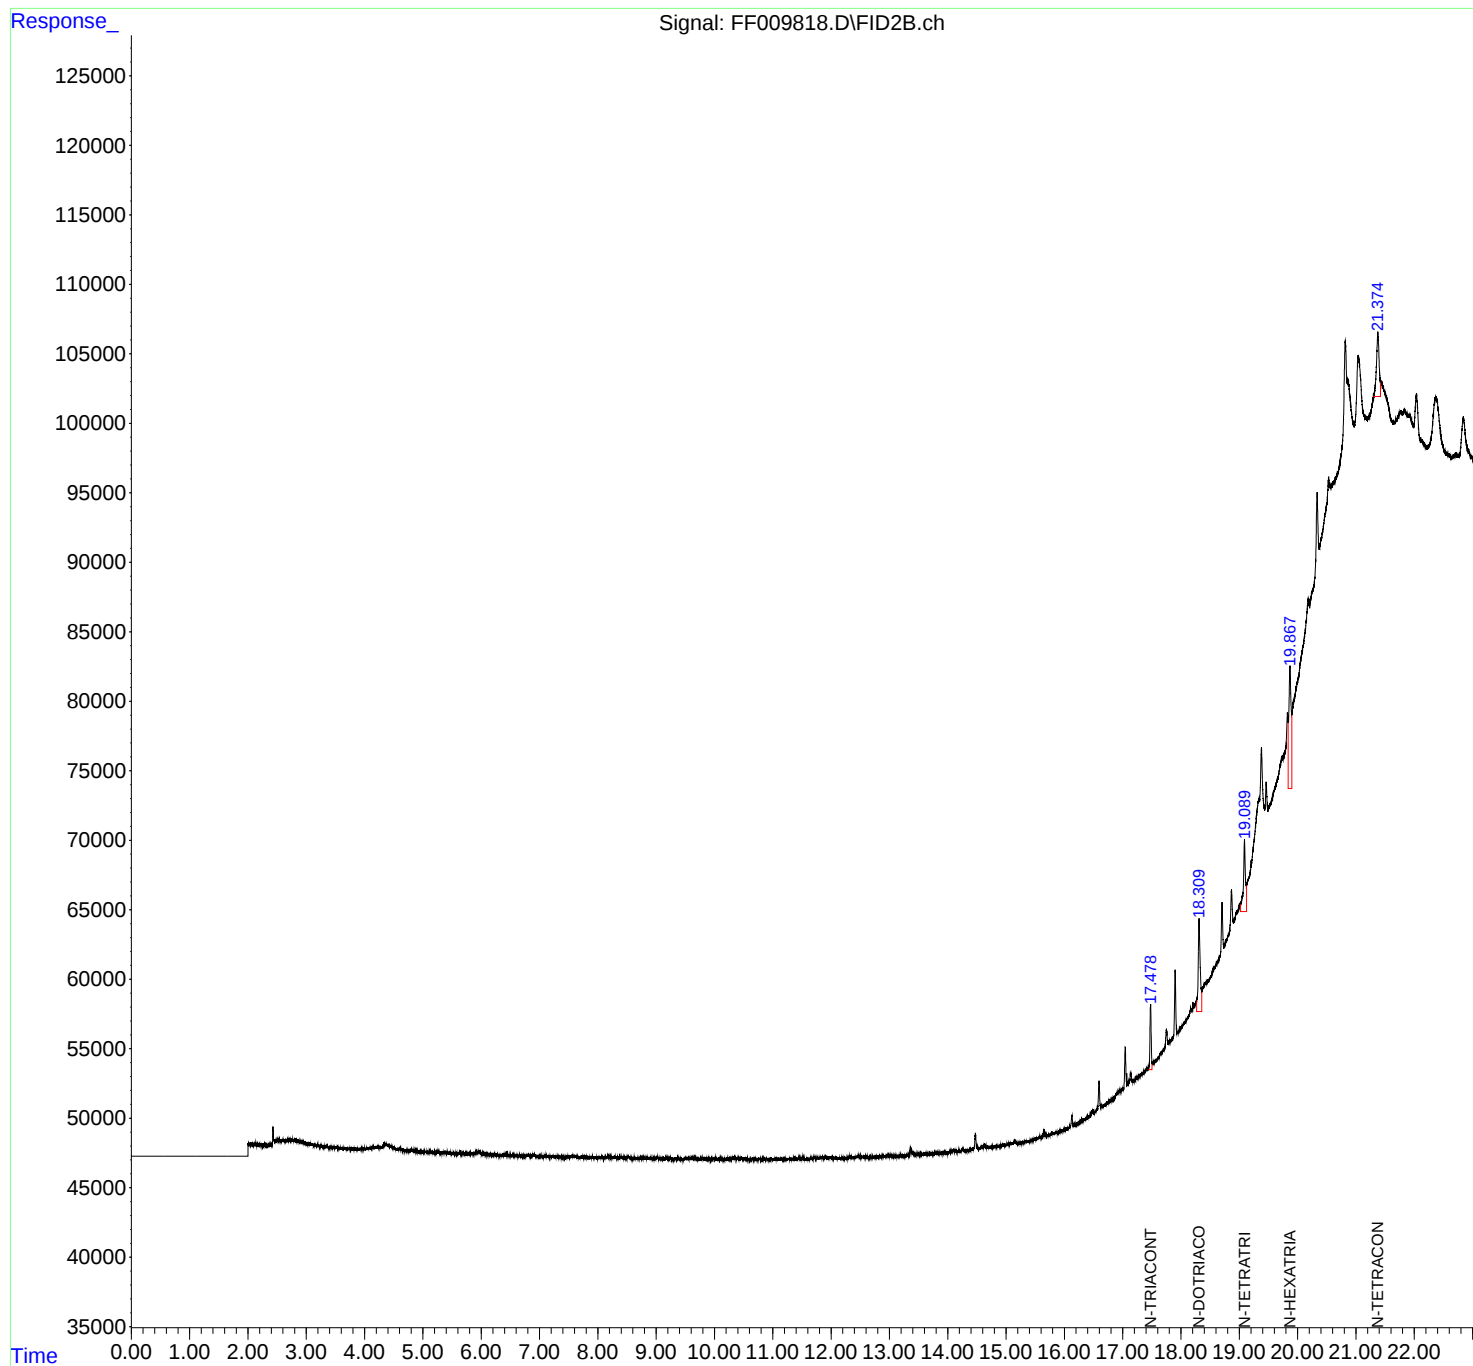


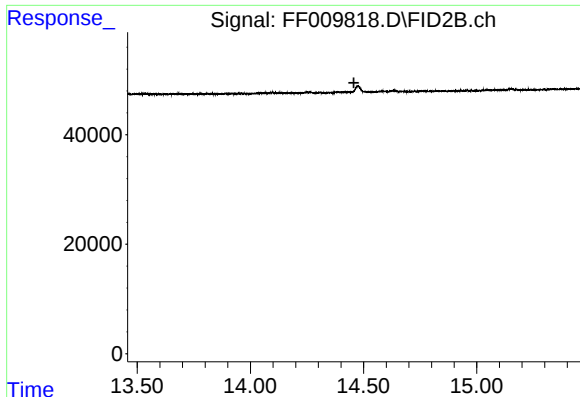

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.457 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

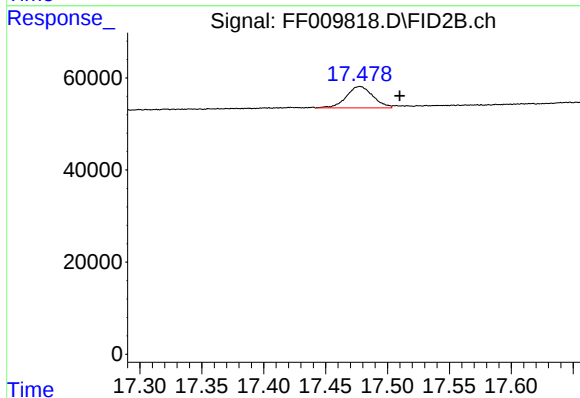


#13 N-TRIACONTANE

R.T.: 17.478 min
Delta R.T.: -0.032 min
Response: 69330
Conc: 0.48 ug/ml

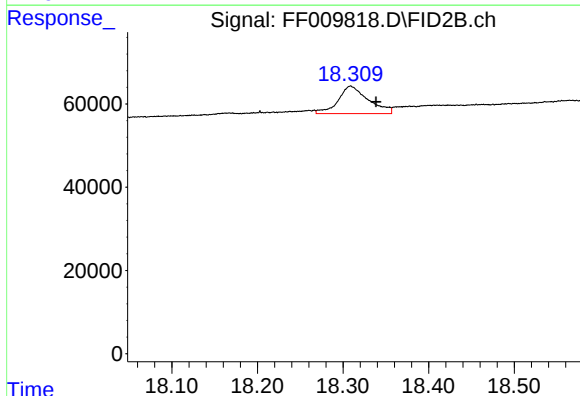


#14 N-DOTRIACONTANE

R.T.: 18.309 min
Delta R.T.: -0.029 min
Response: 162847
Conc: 1.20 ug/ml

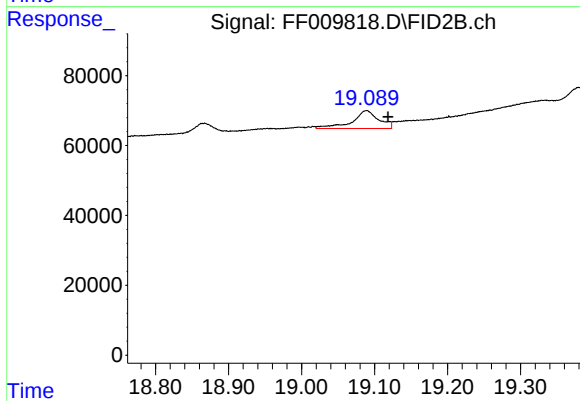

#15 N-TETRATRIACONTANE


R.T.: 19.090 min
Delta R.T.: -0.029 min
Response: 130939
Conc: 1.10 ug/ml

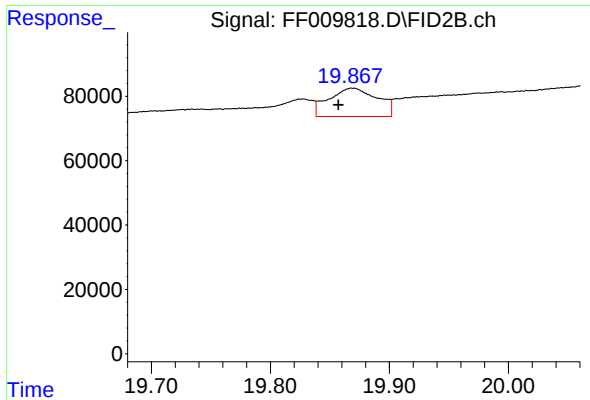

#16 N-HEXATRIACONTANE

R.T.: 19.868 min
Delta R.T.: 0.011 min
Response: 250251
Conc: 2.43 ug/ml

Instrument :
FID_F
ClientSampleId :

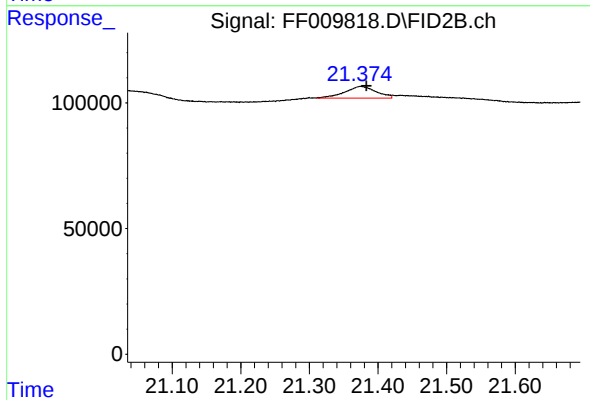

#18 N-TETRACONTANE

R.T.: 21.374 min
Delta R.T.: -0.009 min
Response: 145493
Conc: 1.60 ug/ml