

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020122\
 Data File : FF009822.D
 Signal(s) : FID2B.ch
 Acq On : 01 Feb 2022 14:23
 Operator : AJ\MA
 Sample : PB142412BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 02 02:00:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.427	2158024	16.514 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.477	58371	0.408 ug/ml
14) N-DOTRIACONTANE	18.317	185801	1.365 ug/ml
15) N-TETRATRIACONTANE	19.086	88851	0.748 ug/ml
16) N-HEXATRIACONTANE	19.867	386321	3.747 ug/ml
18) N-TETRACONTANE	21.376	239154	2.633 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020122\
Data File : FF009822.D
Signal(s) : FID2B.ch
Acq On : 01 Feb 2022 14:23
Operator : AJ\MA
Sample : PB142412BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 02 02:00:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

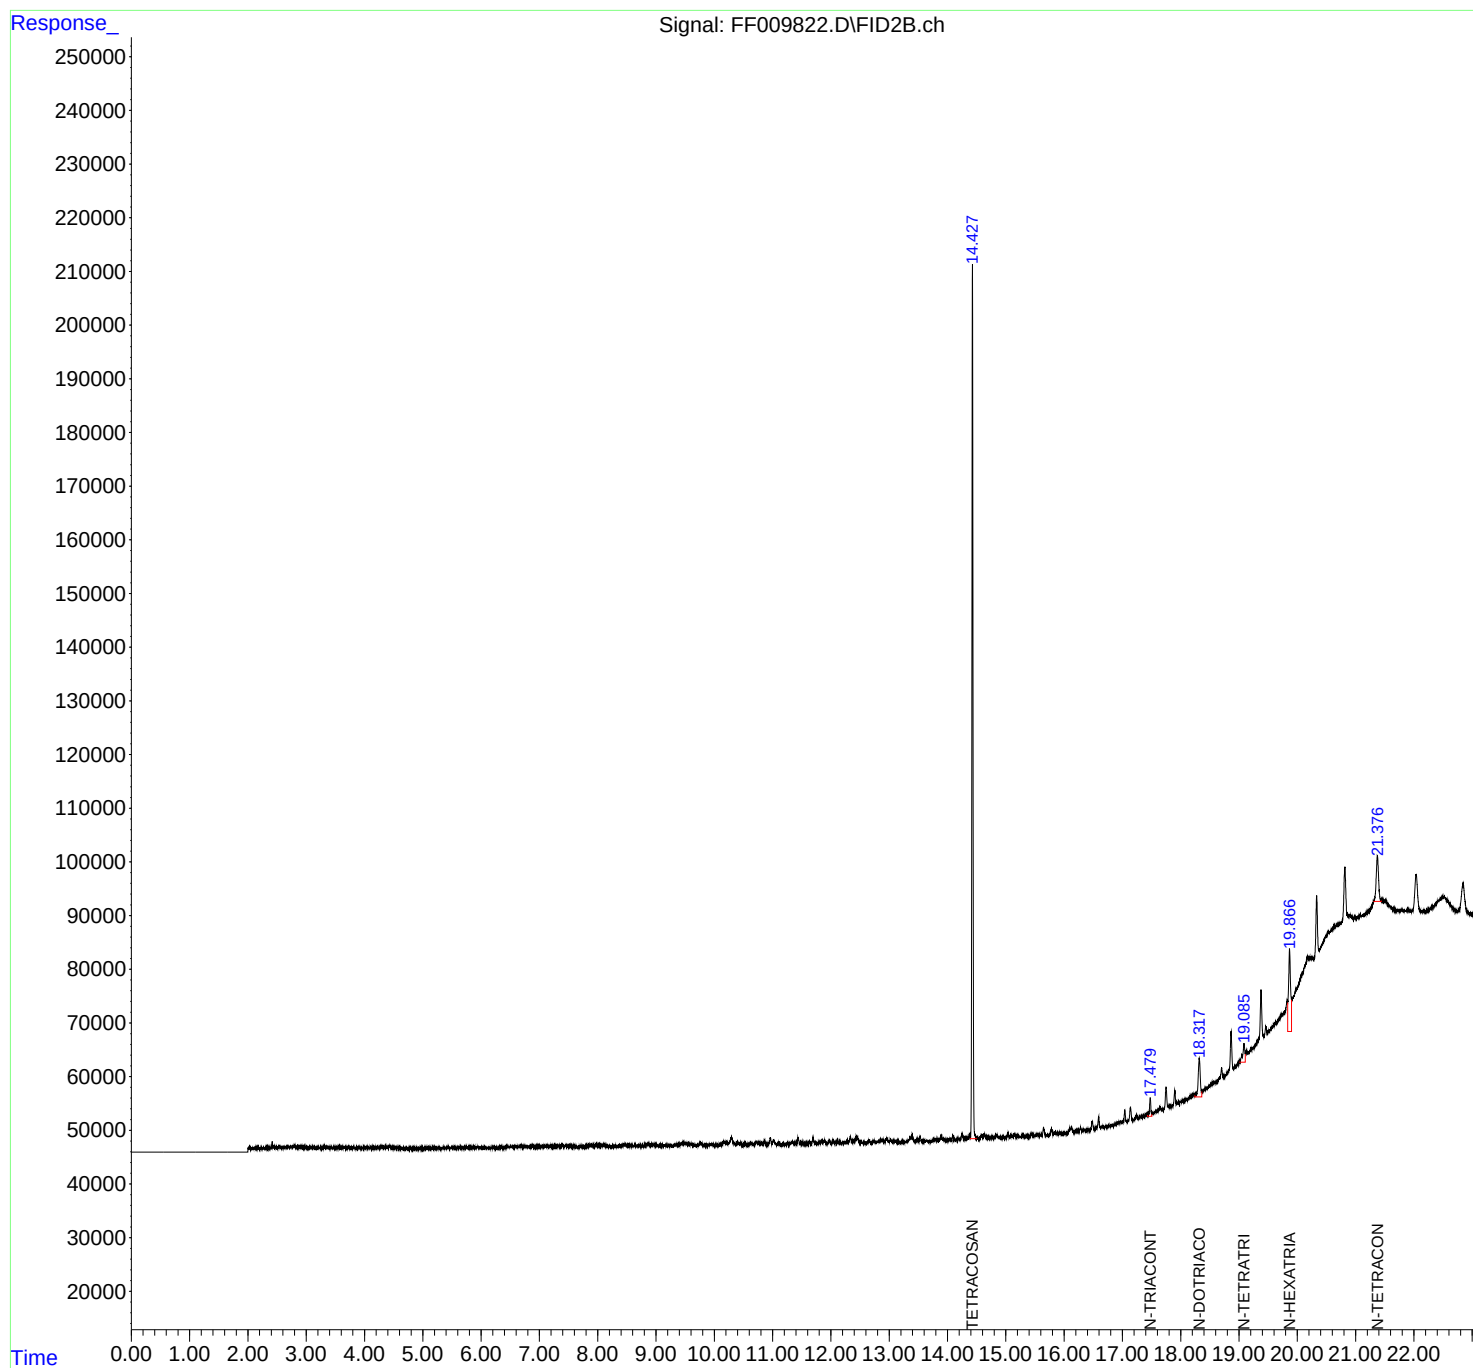


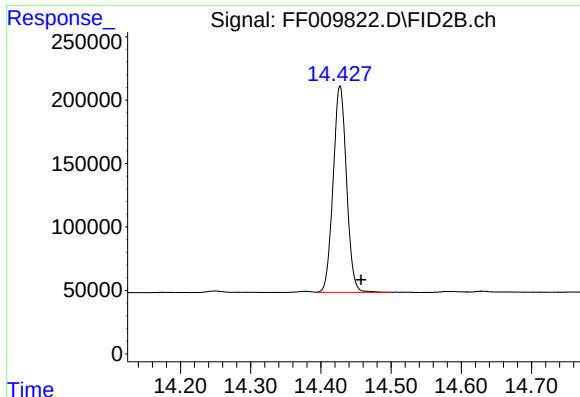

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.427 min
Delta R.T.: -0.030 min
Response: 2158024
Conc: 16.51 ug/ml

Instrument :
FID_F
ClientSampleId :

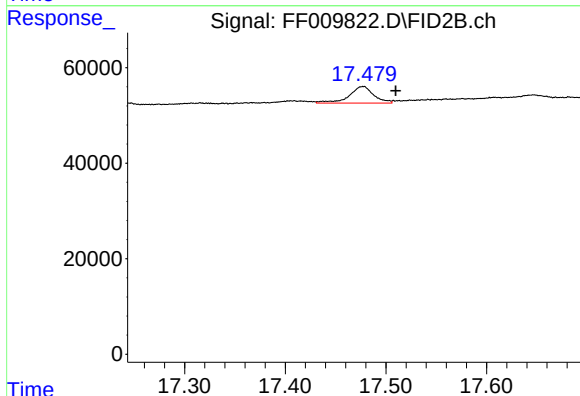


#13 N-TRIACONTANE

R.T.: 17.477 min
Delta R.T.: -0.032 min
Response: 58371
Conc: 0.41 ug/ml

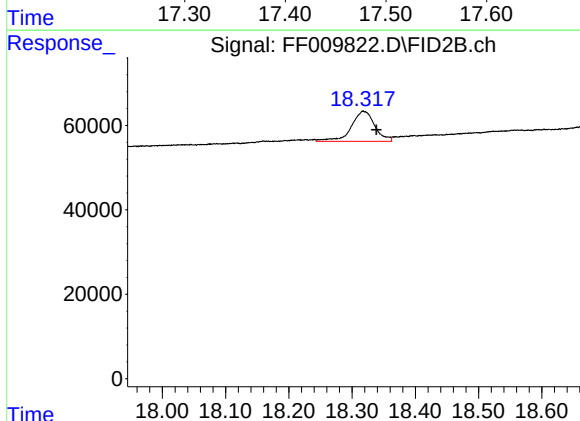


#14 N-DOTRIACONTANE

R.T.: 18.317 min
Delta R.T.: -0.021 min
Response: 185801
Conc: 1.37 ug/ml

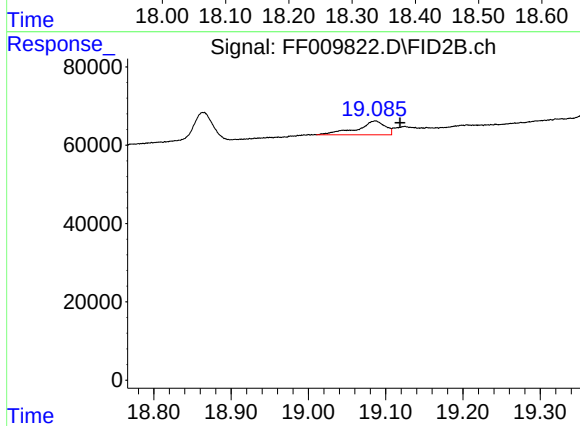

#15 N-TETRATRIACONTANE


R.T.: 19.086 min
Delta R.T.: -0.033 min
Response: 88851
Conc: 0.75 ug/ml

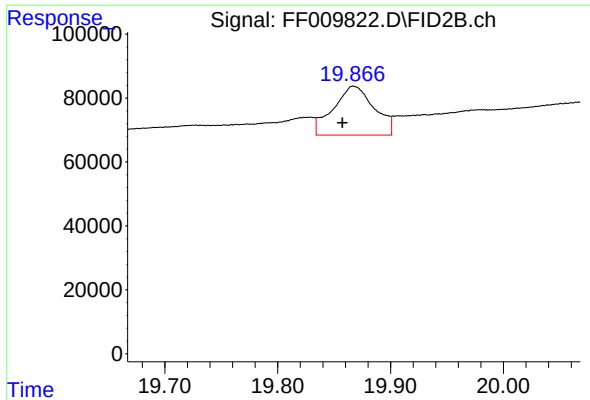

#16 N-HEXATRIACONTANE

R.T.: 19.867 min
Delta R.T.: 0.010 min
Response: 386321
Conc: 3.75 ug/ml

Instrument :
FID_F
ClientSampleId :

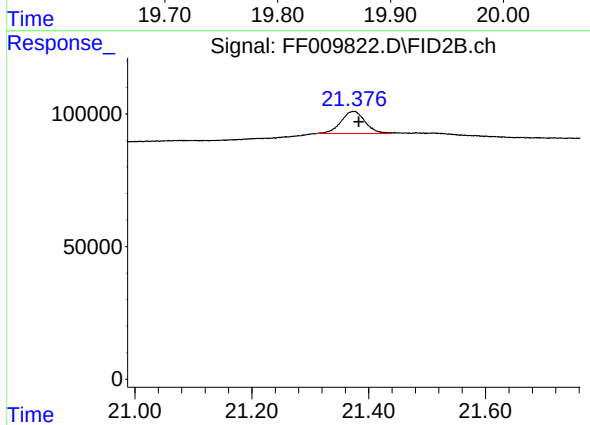

#18 N-TETRACONTANE

R.T.: 21.376 min
Delta R.T.: -0.007 min
Response: 239154
Conc: 2.63 ug/ml