

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020123\
 Data File : FF011947.D
 Signal(s) : FID2B.ch
 Acq On : 01 Feb 2023 12:18
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 02 05:38:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
 Quant Title :
 QLast Update : Fri Jan 27 14:21:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.765	2413863	20.151 ug/ml
12) N-OCTACOSANE	17.214	2356672	18.123 ug/ml
14) N-DOTRIACONTANE	18.948	99164	0.762 ug/ml
16) N-HEXATRIACONTANE	20.498	102044	0.993 ug/ml
18) N-TETRACONTANE	22.160	405377	3.911 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020123\
Data File : FF011947.D
Signal(s) : FID2B.ch
Acq On : 01 Feb 2023 12:18
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 02 05:38:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

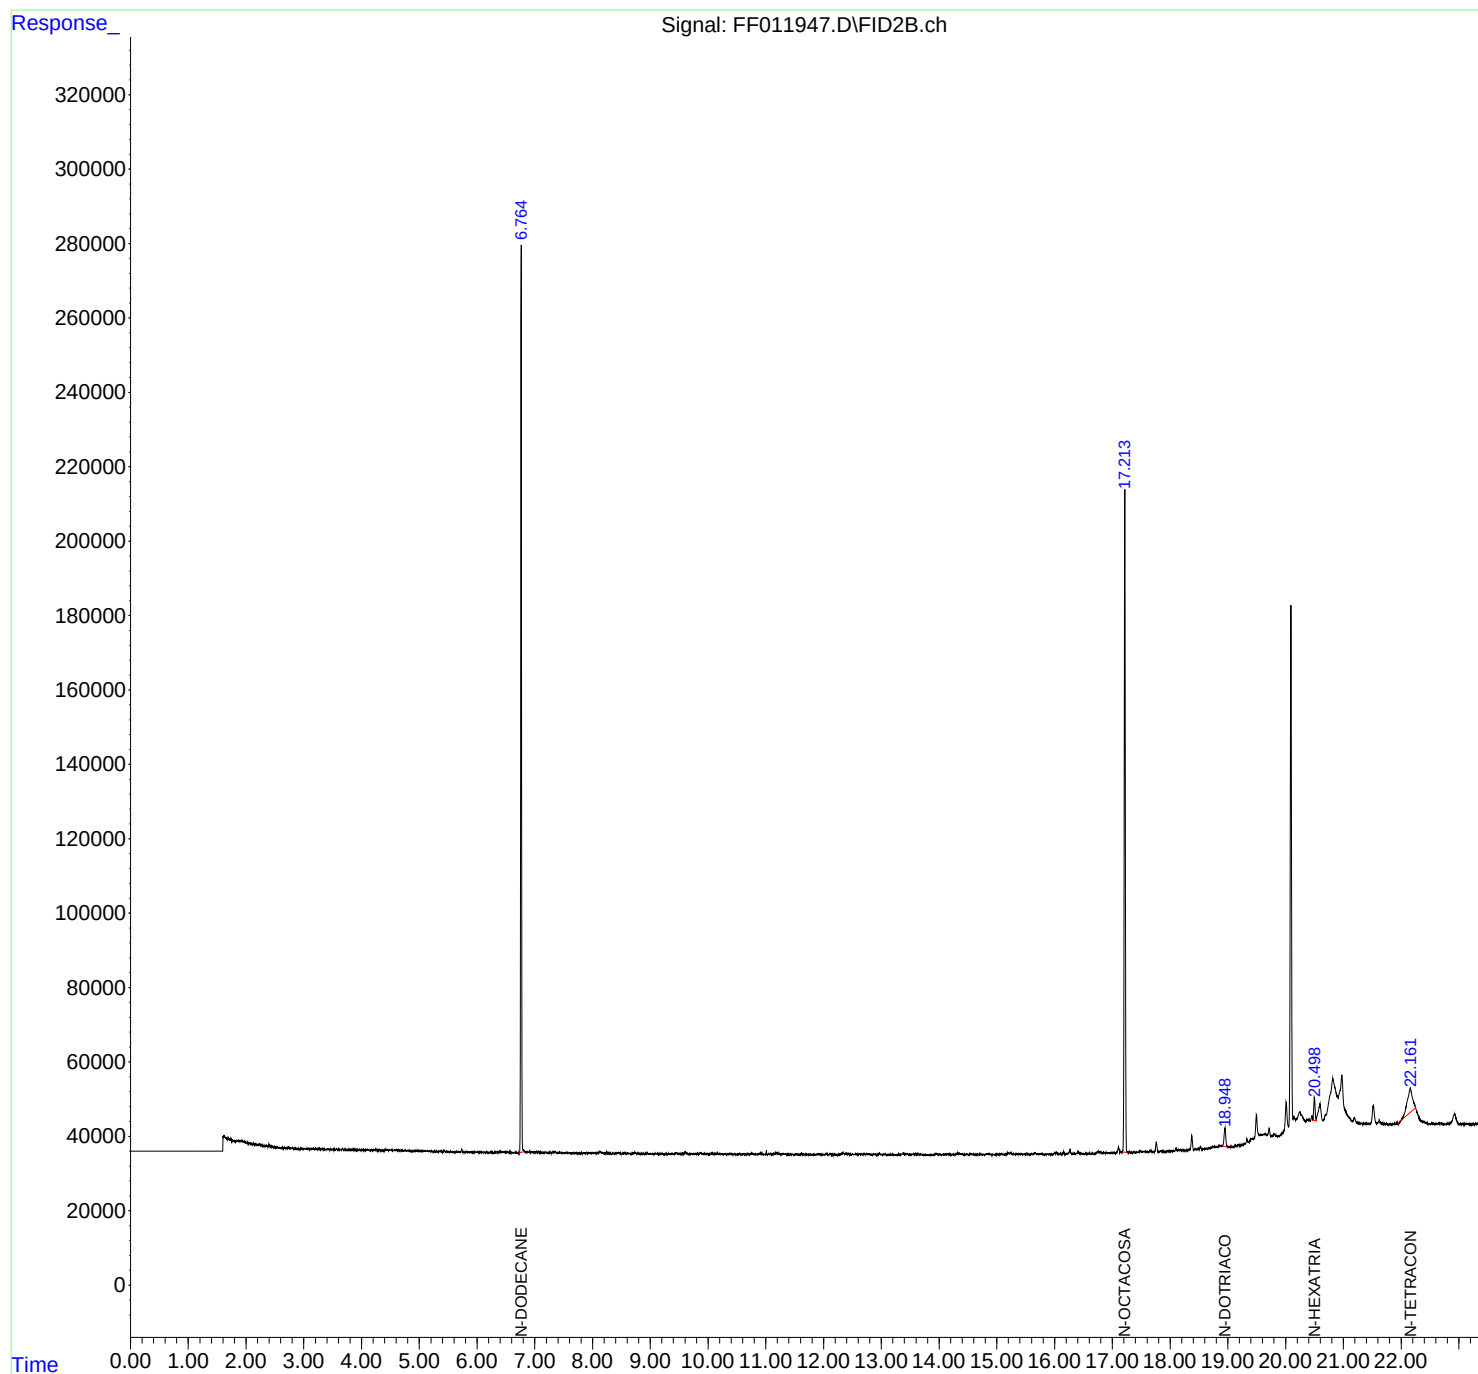

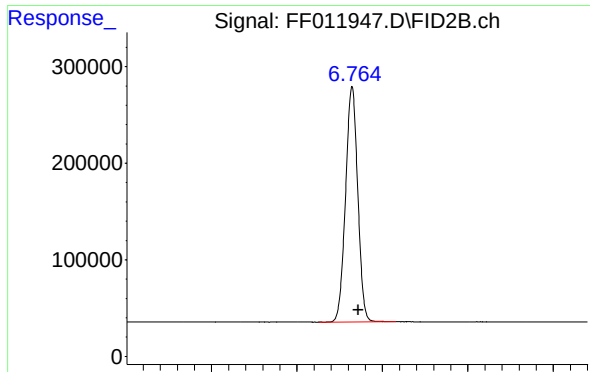


#3 N-DODECANE

R.T.: 6.765 min
Delta R.T.: -0.008 min
Response: 2413863
Conc: 20.15 ug/ml

Instrument :


FID_F

ClientSampleId :

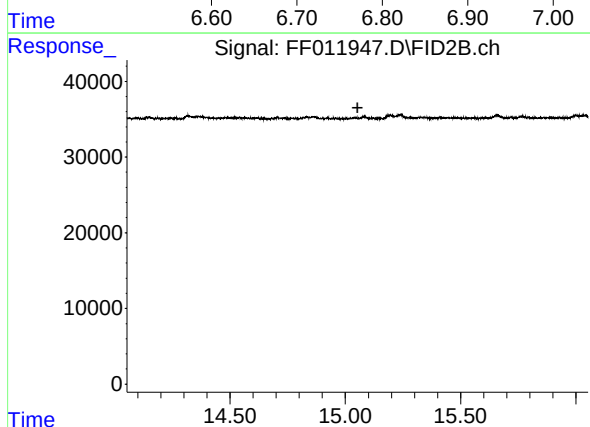


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.053 min
Response: 0
Conc: N.D.

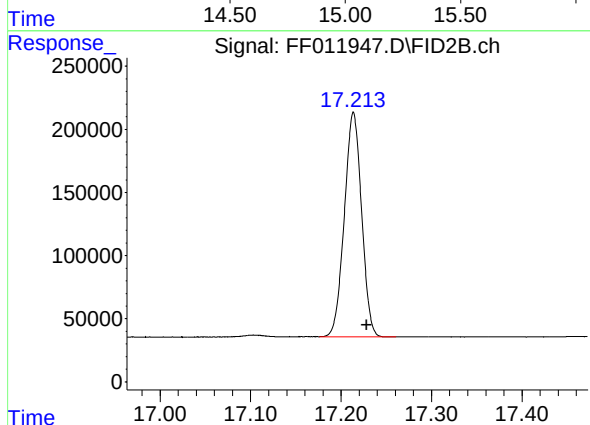


#12 N-OCTACOSANE

R.T.: 17.214 min
Delta R.T.: -0.015 min
Response: 2356672
Conc: 18.12 ug/ml

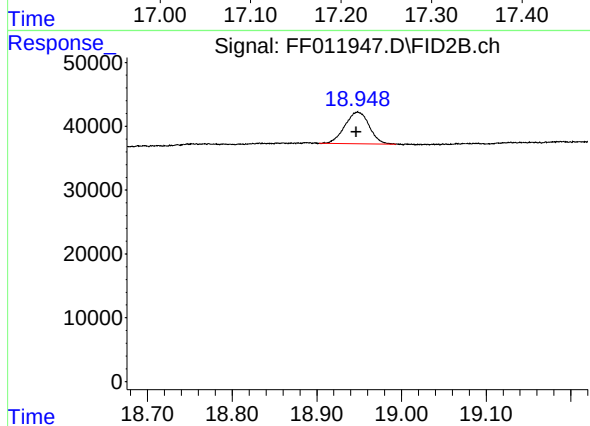

#14 N-DOTRIACONTANE


R.T.: 18.948 min
Delta R.T.: 0.002 min
Response: 99164
Conc: 0.76 ug/ml

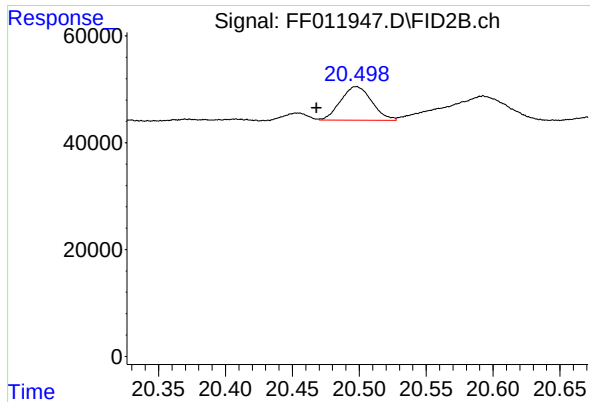

#16 N-HEXATRIACONTANE

R.T.: 20.498 min
Delta R.T.: 0.030 min
Response: 102044
Conc: 0.99 ug/ml

Instrument :
FID_F
ClientSampleId :

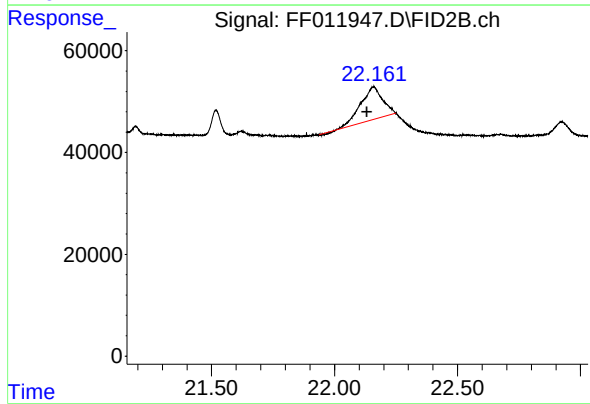

#18 N-TETRACONTANE

R.T.: 22.160 min
Delta R.T.: 0.027 min
Response: 405377
Conc: 3.91 ug/ml