

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020123\
 Data File : FF011950.D
 Signal(s) : FID2B.ch
 Acq On : 01 Feb 2023 15:45
 Operator : YP\AJ
 Sample : 01358-05
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 02 05:38:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
 Quant Title :
 QLast Update : Fri Jan 27 14:21:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.041	1707896	14.821 ug/ml
Target Compounds			
4) N-TETRADECANE	8.588	52849	0.439 ug/ml
7) N-EICOSANE	12.953	116656	0.904 ug/ml
8) N-DOCOSANE	14.171	337463	2.647 ug/ml
10) N-TETRACOSANE	15.225	1178771	9.059 ug/ml
11) N-HEXACOSANE	16.266	143394	1.102 ug/ml
12) N-OCTACOSANE	17.219	329971	2.538 ug/ml
13) N-TRIACONTANE	18.098	149563	1.159 ug/ml
14) N-DOTRIACONTANE	18.927	167325	1.286 ug/ml
16) N-HEXATRIACONTANE	20.414f	118295	1.152 ug/ml
18) N-TETRACONTANE	22.147	26310	0.254 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020123\
Data File : FF011950.D
Signal(s) : FID2B.ch
Acq On : 01 Feb 2023 15:45
Operator : YP\AJ
Sample : 01358-05
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 02 05:38:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

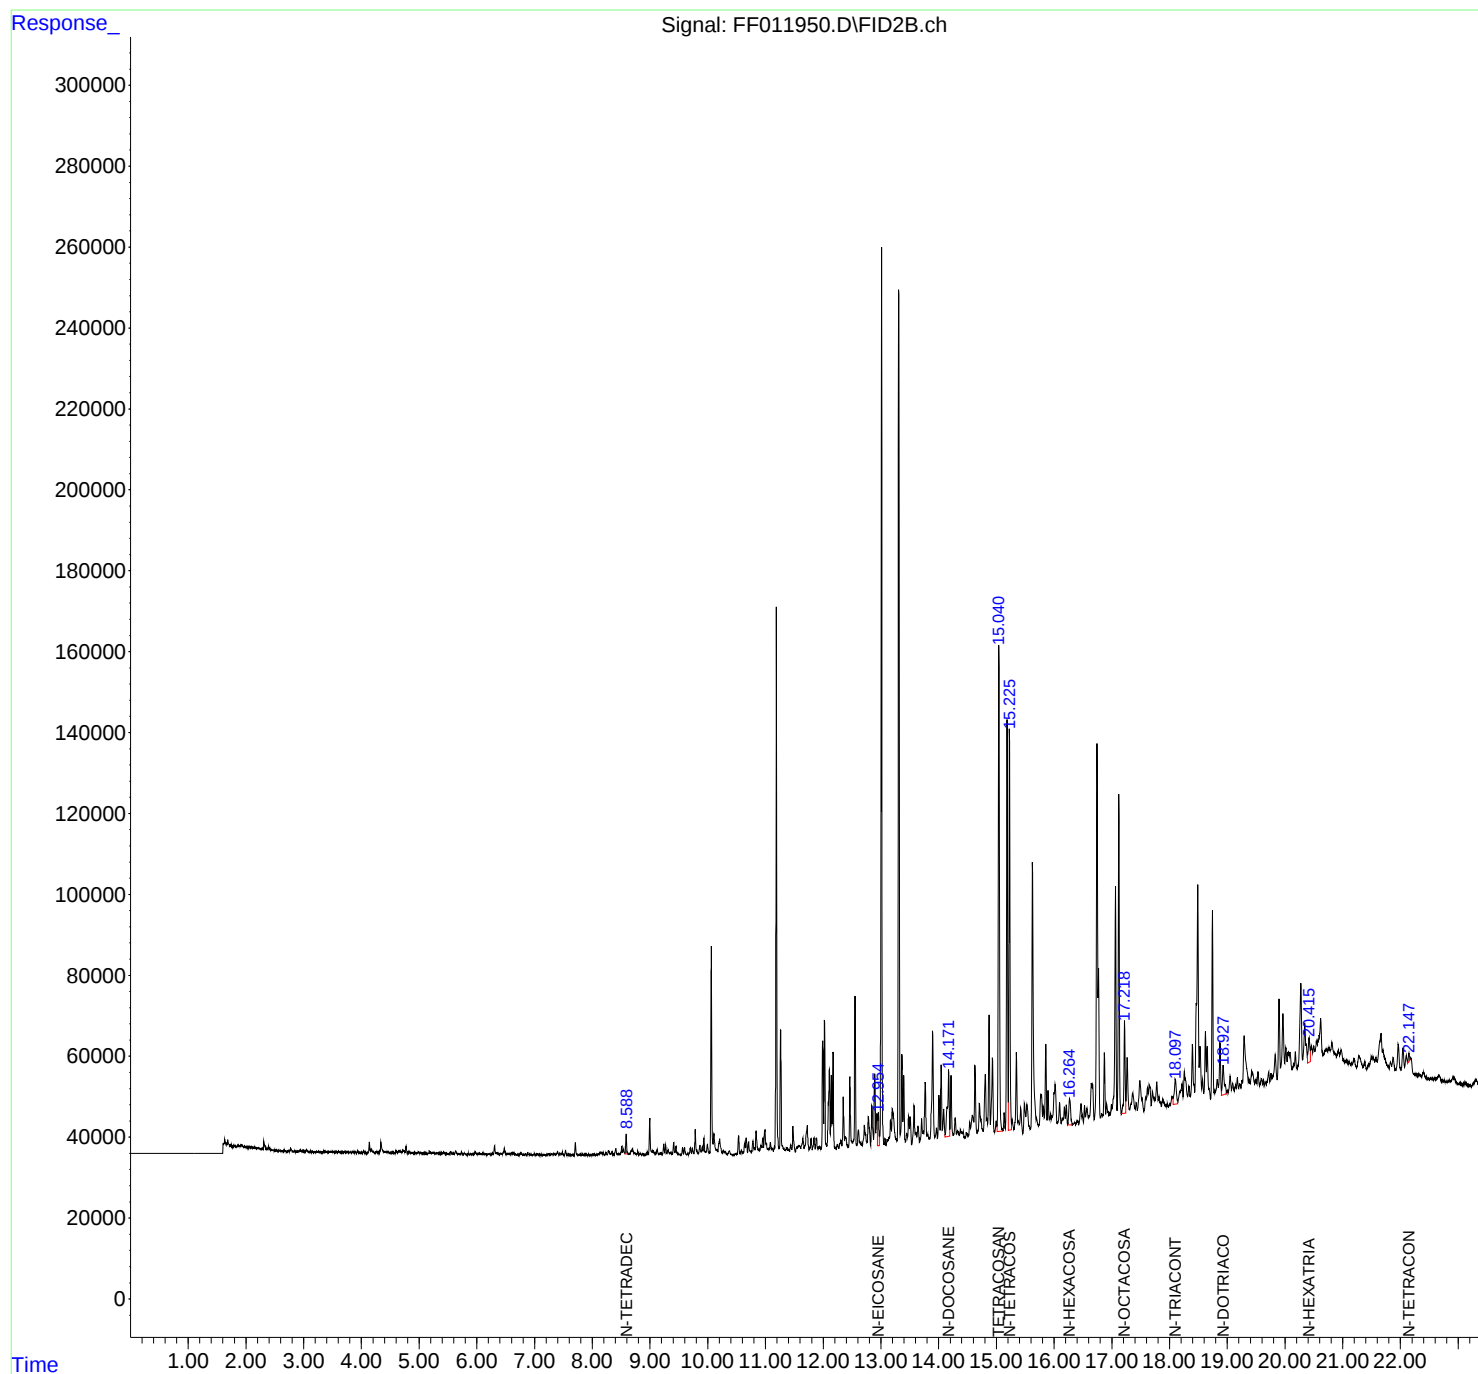


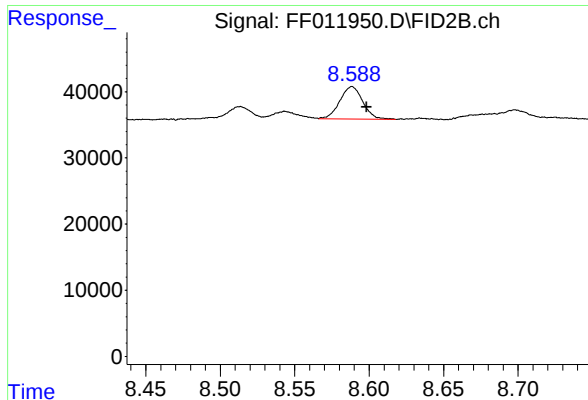

#4 N-TETRADECANE


R.T.: 8.588 min
Delta R.T.: -0.010 min
Response: 52849
Conc: 0.44 ug/ml

Instrument :
FID_F
ClientSampleId :

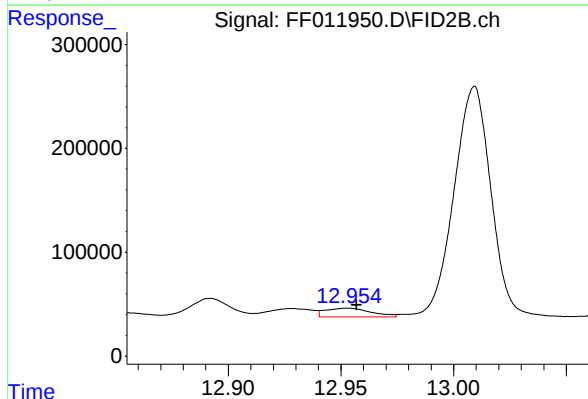


#7 N-EICOSANE

R.T.: 12.953 min
Delta R.T.: -0.004 min
Response: 116656
Conc: 0.90 ug/ml

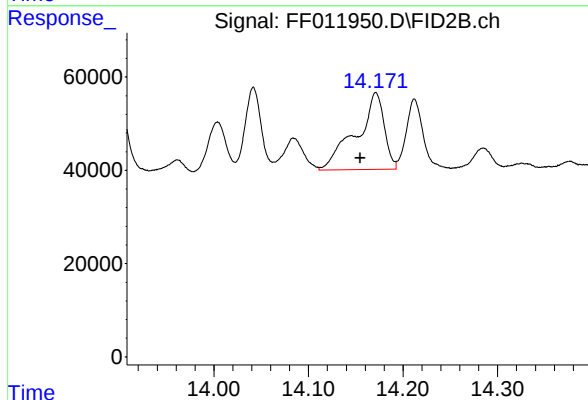


#8 N-DOCOSANE

R.T.: 14.171 min
Delta R.T.: 0.017 min
Response: 337463
Conc: 2.65 ug/ml

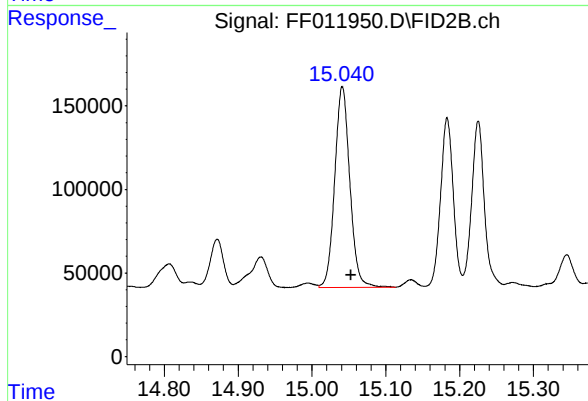

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.041 min
Delta R.T.: -0.012 min
Response: 1707896
Conc: 14.82 ug/ml

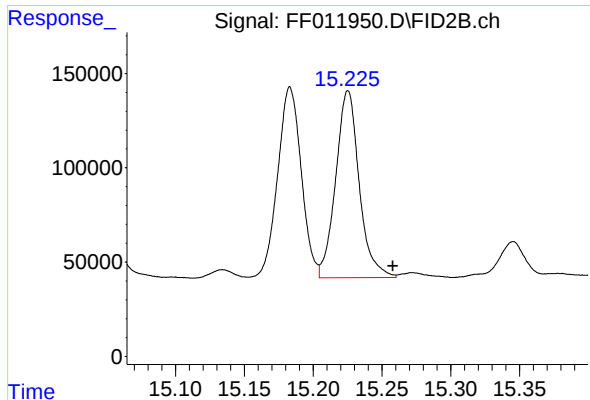

#10 N-TETRACOSANE


R.T.: 15.225 min
Delta R.T.: -0.033 min
Response: 1178771
Conc: 9.06 ug/ml

Instrument :
FID_F
ClientSampleId :

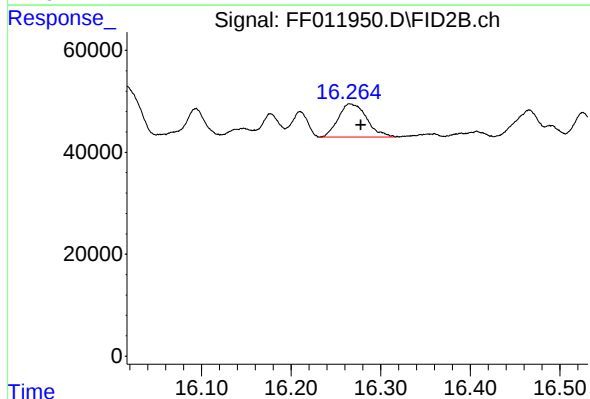


#11 N-HEXACOSANE

R.T.: 16.266 min
Delta R.T.: -0.012 min
Response: 143394
Conc: 1.10 ug/ml

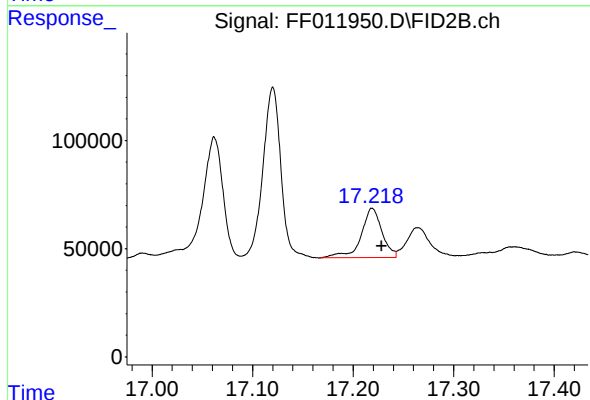


#12 N-OCTACOSANE

R.T.: 17.219 min
Delta R.T.: -0.009 min
Response: 329971
Conc: 2.54 ug/ml

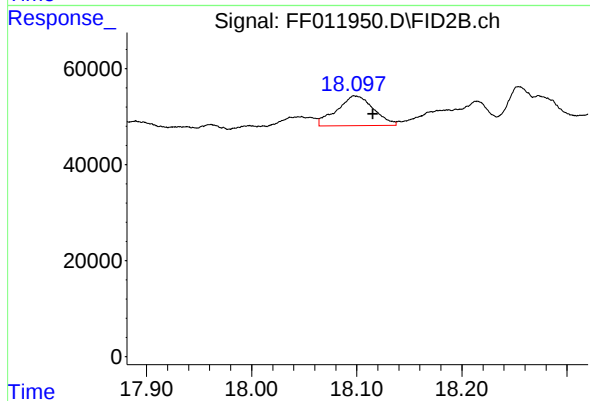

#13 N-TRIACONTANE


R.T.: 18.098 min
Delta R.T.: -0.017 min
Response: 149563
Conc: 1.16 ug/ml

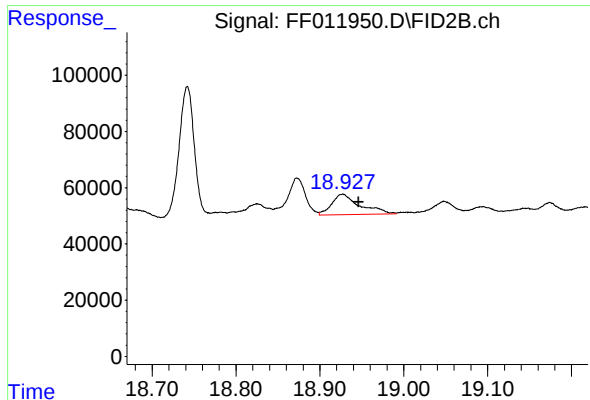

#14 N-DOTRIACONTANE


R.T.: 18.927 min
Delta R.T.: -0.019 min
Response: 167325
Conc: 1.29 ug/ml

Instrument :
FID_F
ClientSampleId :

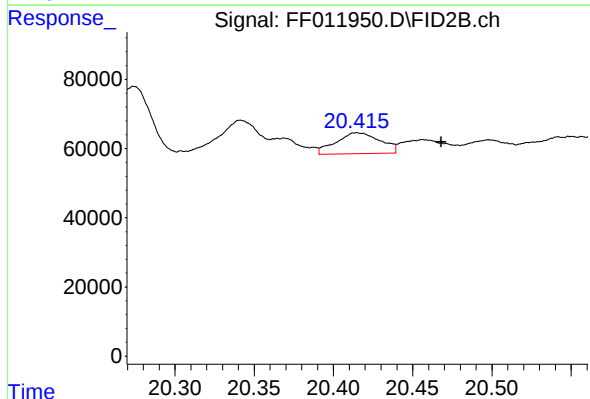

#16 N-HEXATRIACONTANE

R.T.: 20.414 min
Delta R.T.: -0.054 min
Response: 118295
Conc: 1.15 ug/ml

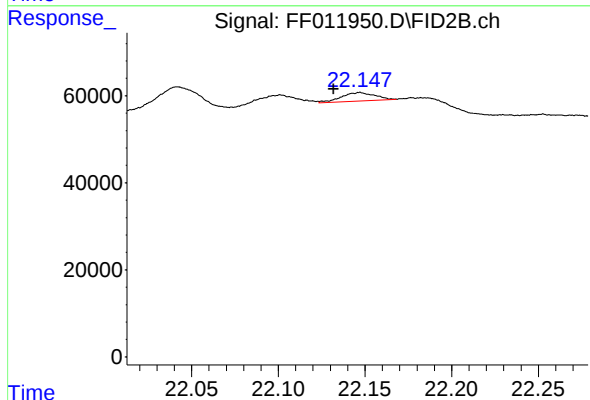

#18 N-TETRACONTANE

R.T.: 22.147 min
Delta R.T.: 0.015 min
Response: 26310
Conc: 0.25 ug/ml