

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020123\
 Data File : FF011951.D
 Signal(s) : FID2B.ch
 Acq On : 01 Feb 2023 16:15
 Operator : YP\AJ
 Sample : 01358-05MS
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 DR-2-012723MS

Integration File: autoint1.e
 Quant Time: Feb 02 05:39:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
 Quant Title :
 QLast Update : Fri Jan 27 14:21:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.041	1781474	15.460 ug/ml
Target Compounds			
2) N-DECANE	4.602	1960302	16.626 ug/ml
3) N-DODECANE	6.763	2119832	17.696 ug/ml
4) N-TETRADECANE	8.589	2190849	18.193 ug/ml
5) N-HEXADECANE	10.194	2312553	18.540 ug/ml
6) N-OCTADECANE	11.636	2323580	18.274 ug/ml
7) N-EICOSANE	12.946	2502518	19.390 ug/ml
8) N-DOCOSANE	14.143	2533279	19.873 ug/ml
10) N-TETRACOSANE	15.245	3445562	26.479 ug/ml
11) N-HEXACOSANE	16.266	2252325	17.306 ug/ml
12) N-OCTACOSANE	17.216	2386361	18.352 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020123\
Data File : FF011951.D
Signal(s) : FID2B.ch
Acq On : 01 Feb 2023 16:15
Operator : YP\AJ
Sample : 01358-05MS
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
DR-2-012723MS

Integration File: autoint1.e
Quant Time: Feb 02 05:39:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

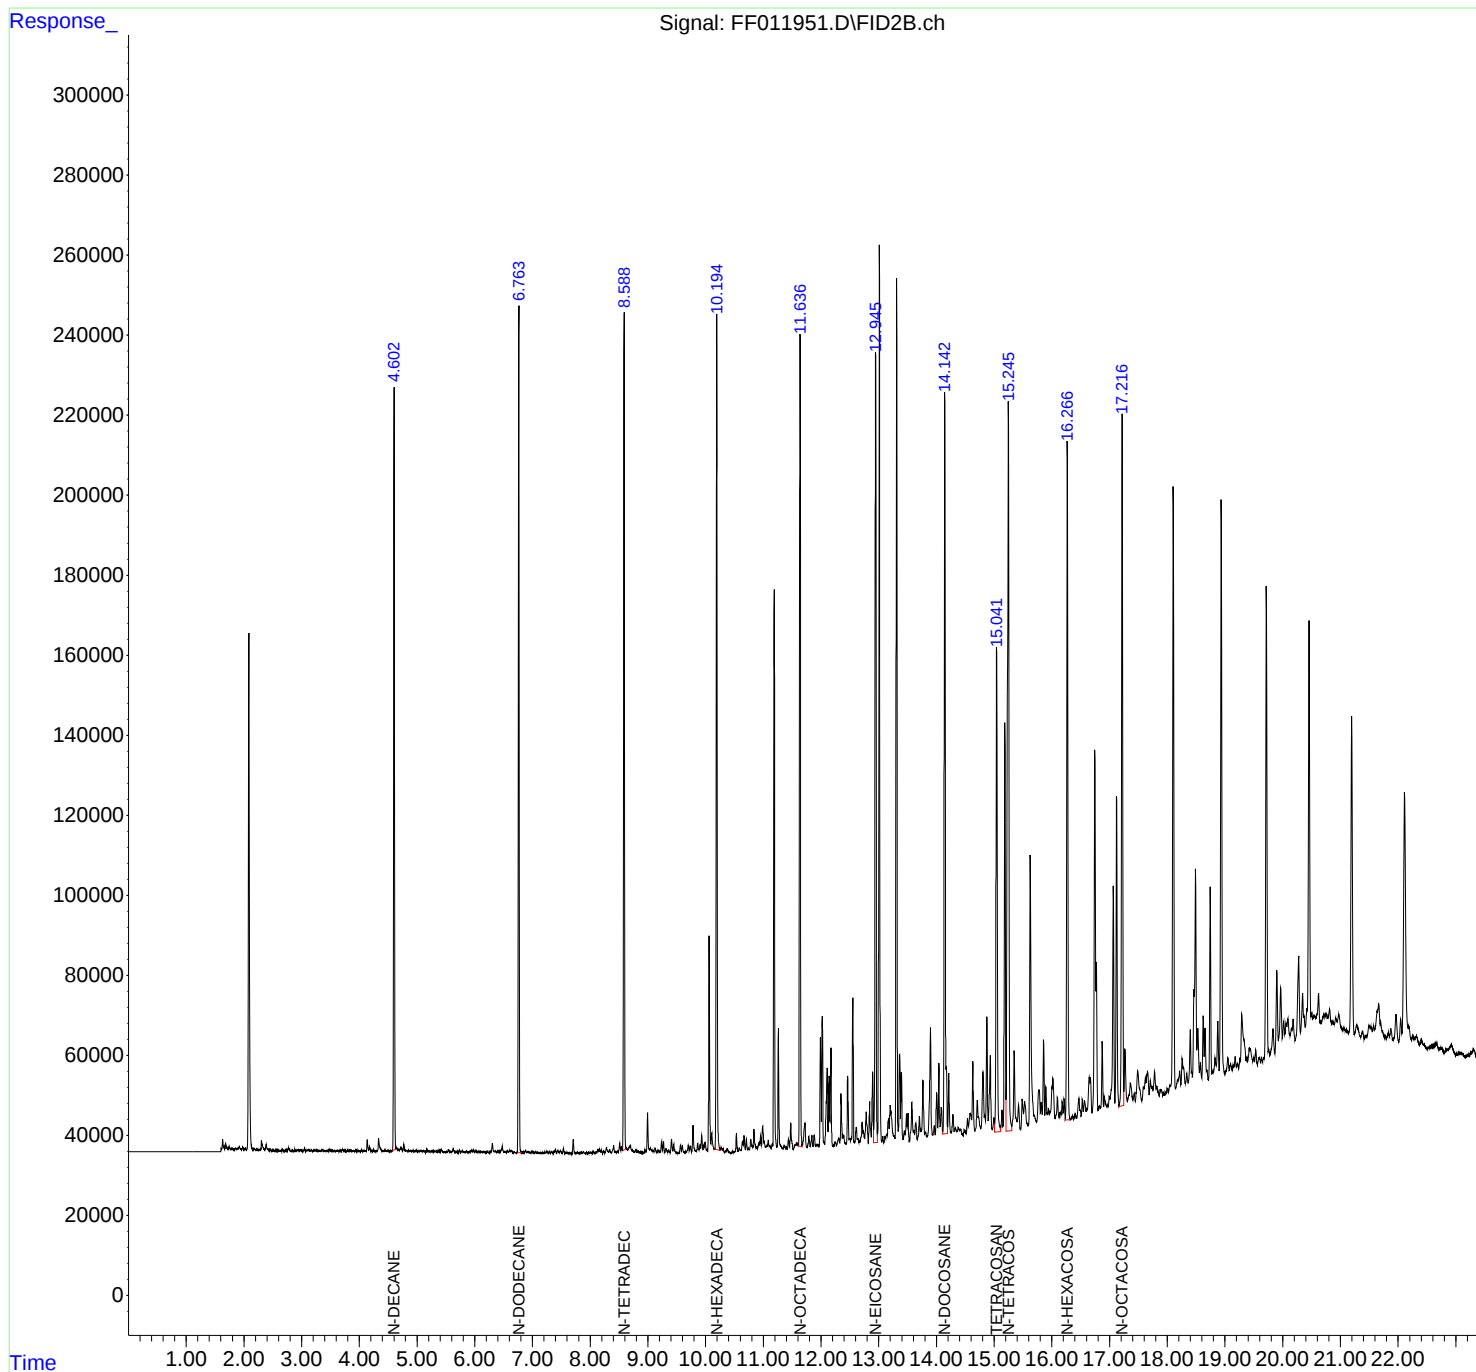


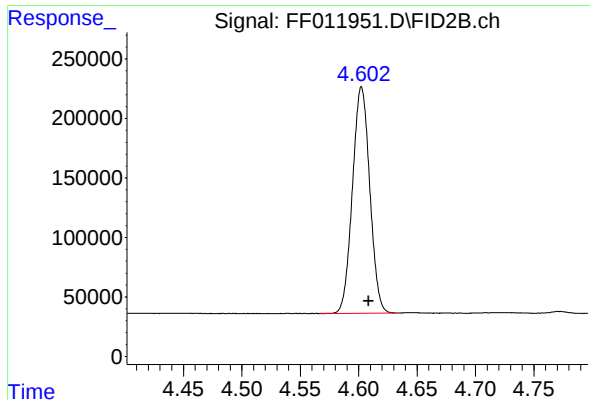

#2 N-DECANE


R.T.: 4.602 min
Delta R.T.: -0.006 min
Response: 1960302
Conc: 16.63 ug/ml

Instrument :
FID_F
ClientSampleId :
DR-2-012723MS

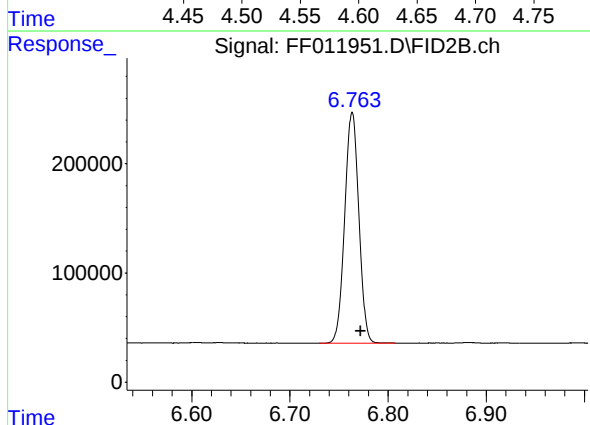


#3 N-DODECANE

R.T.: 6.763 min
Delta R.T.: -0.009 min
Response: 2119832
Conc: 17.70 ug/ml

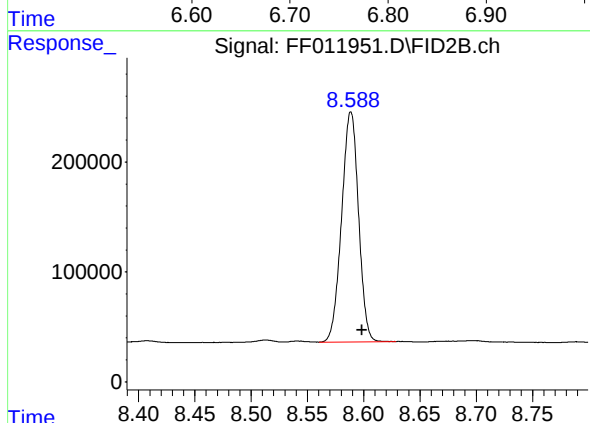


#4 N-TETRADECANE

R.T.: 8.589 min
Delta R.T.: -0.010 min
Response: 2190849
Conc: 18.19 ug/ml

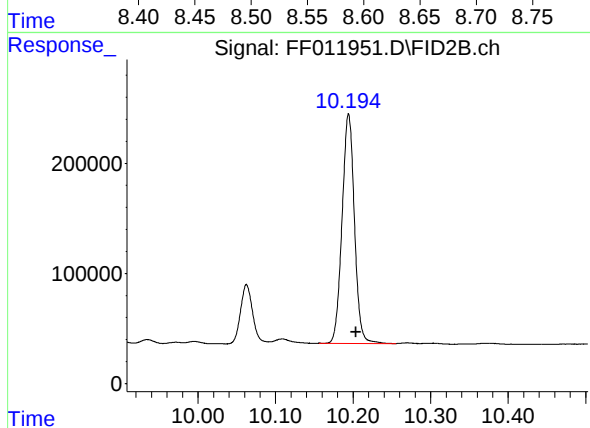

#5 N-HEXADECANE


R.T.: 10.194 min
Delta R.T.: -0.010 min
Response: 2312553
Conc: 18.54 ug/ml

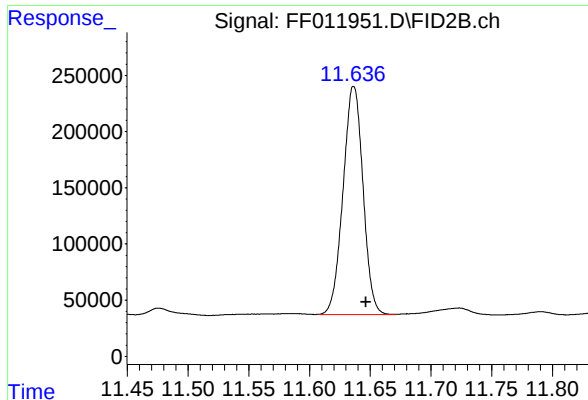

#6 N-OCTADECANE


R.T.: 11.636 min
Delta R.T.: -0.010 min
Response: 2323580
Conc: 18.27 ug/ml

Instrument :
FID_F
ClientSampleId :
DR-2-012723MS

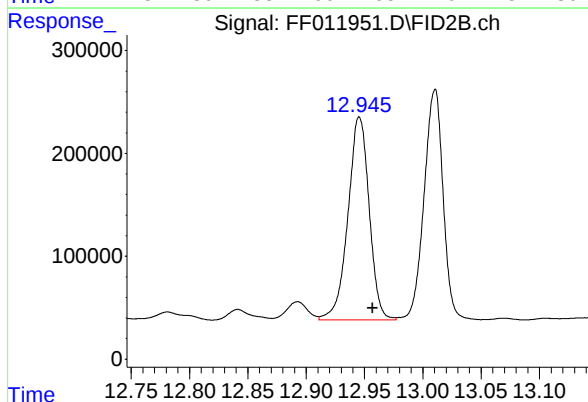


#7 N-EICOSANE

R.T.: 12.946 min
Delta R.T.: -0.011 min
Response: 2502518
Conc: 19.39 ug/ml

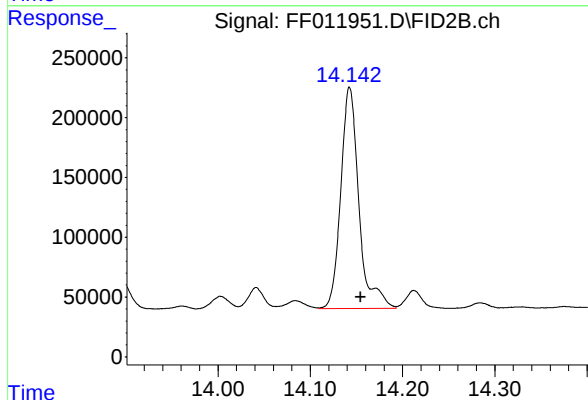


#8 N-DOCOSANE

R.T.: 14.143 min
Delta R.T.: -0.012 min
Response: 2533279
Conc: 19.87 ug/ml

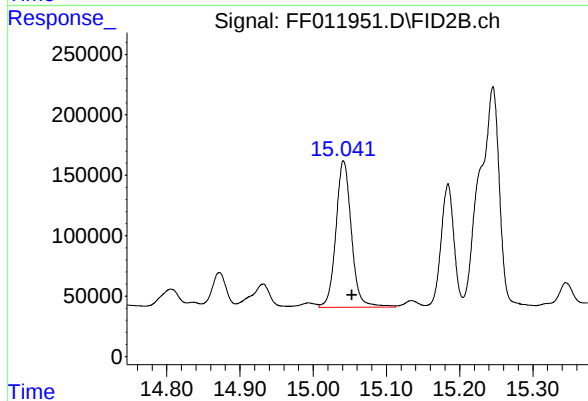

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.041 min
Delta R.T.: -0.011 min
Response: 1781474
Conc: 15.46 ug/ml

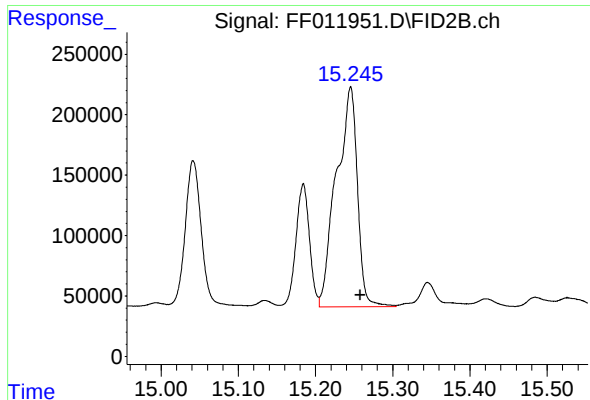

#10 N-TETRACOSANE


R.T.: 15.245 min
Delta R.T.: -0.012 min
Response: 3445562
Conc: 26.48 ug/ml

Instrument :
FID_F
ClientSampleId :
DR-2-012723MS

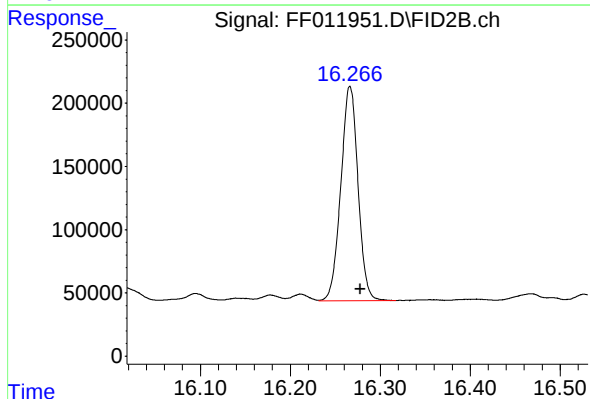

#11 N-HEXACOSANE

R.T.: 16.266 min
Delta R.T.: -0.012 min
Response: 2252325
Conc: 17.31 ug/ml

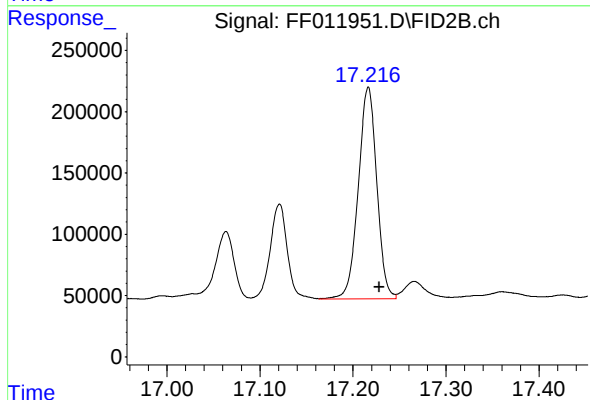

#12 N-OCTACOSANE

R.T.: 17.216 min
Delta R.T.: -0.012 min
Response: 2386361
Conc: 18.35 ug/ml