

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020223\
 Data File : FF011974.D
 Signal(s) : FID2B.ch
 Acq On : 02 Feb 2023 13:57
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 03 00:09:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
 Quant Title :
 QLast Update : Fri Jan 27 14:21:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.048	1938785	16.825 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.942	89213	0.685 ug/ml
16) N-HEXATRIACONTANE	20.503	40557	0.395 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020223\
Data File : FF011974.D
Signal(s) : FID2B.ch
Acq On : 02 Feb 2023 13:57
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 03 00:09:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

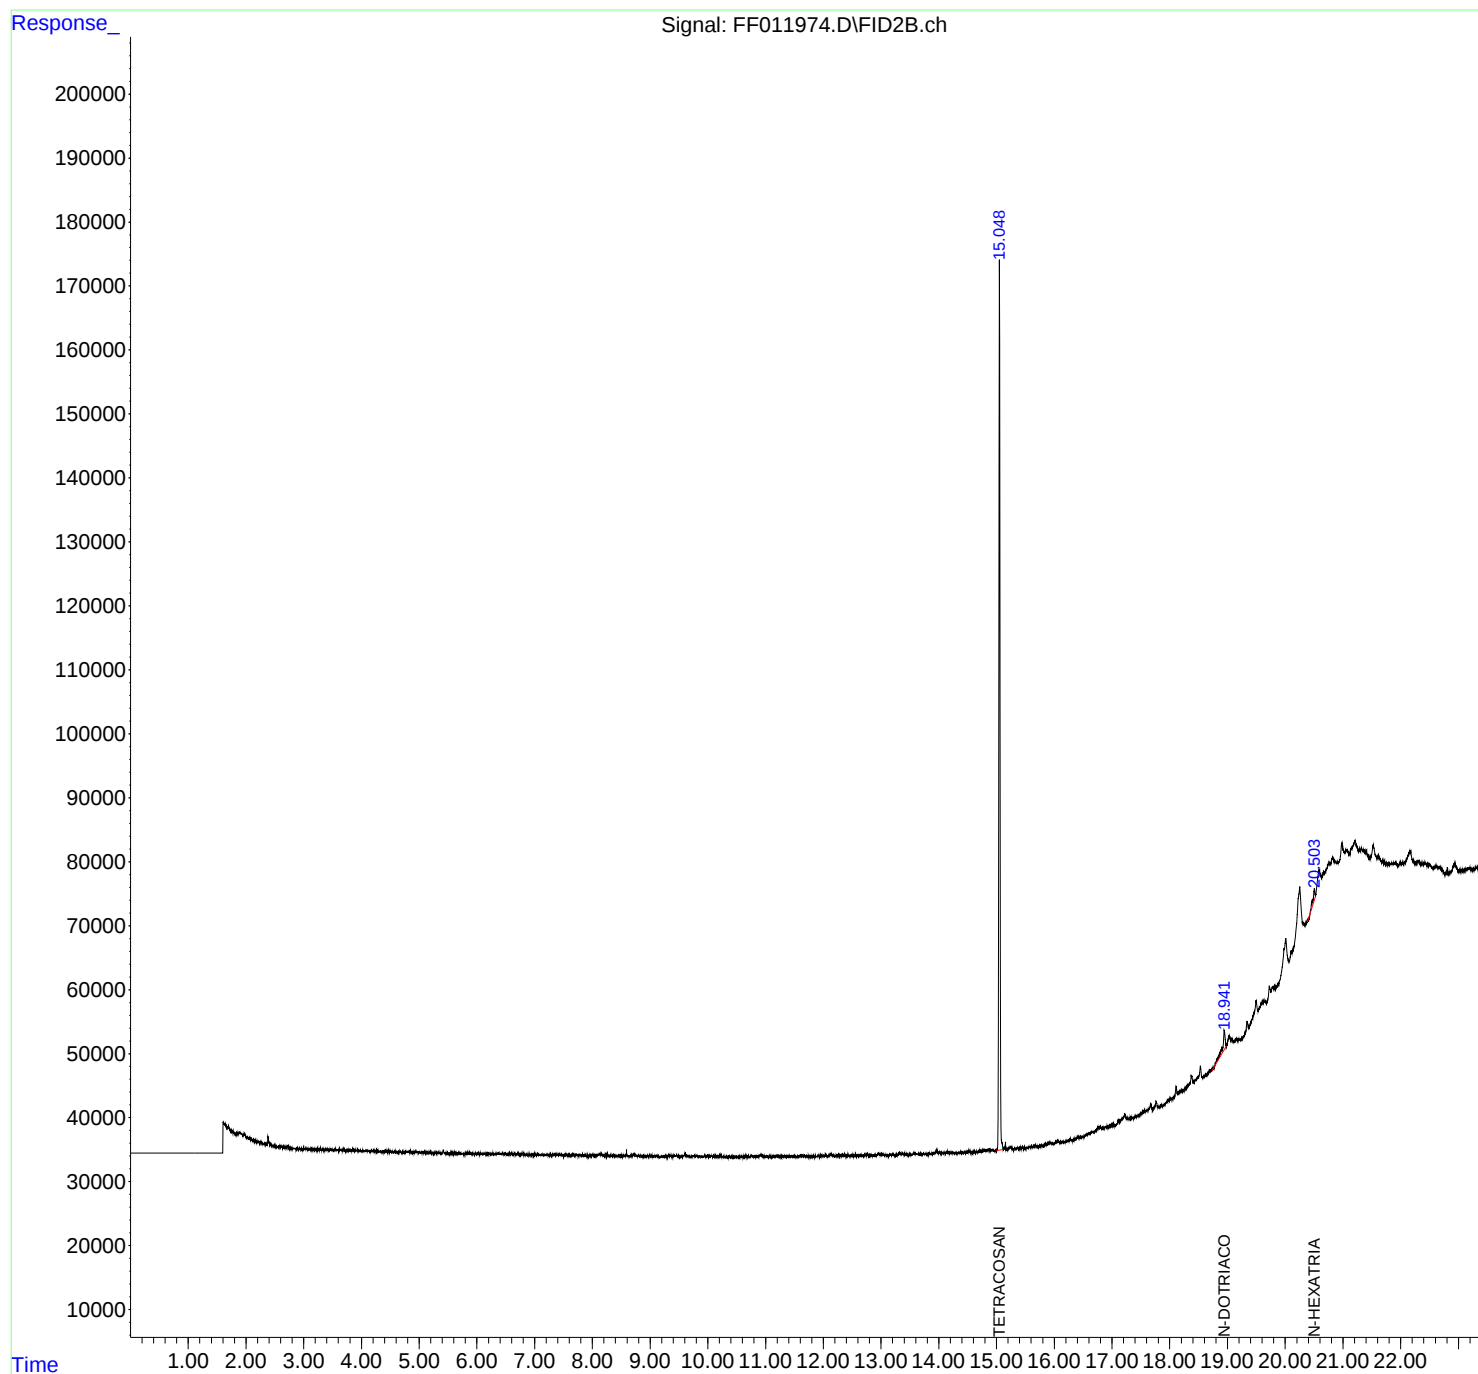

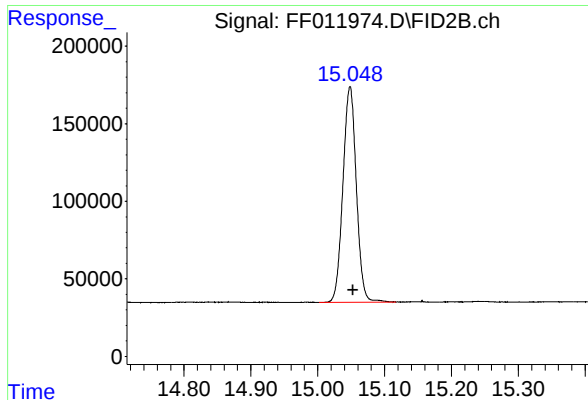


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.048 min
Delta R.T.: -0.005 min
Response: 1938785
Conc: 16.83 ug/ml

Instrument :


FID_F

ClientSampleId :

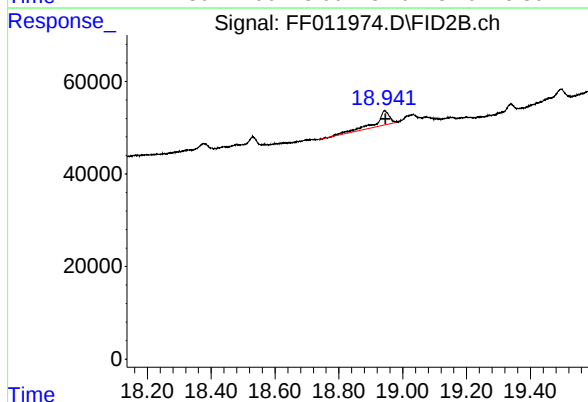

#14 N-DOTRIACONTANE

R.T.: 18.942 min
Delta R.T.: -0.004 min
Response: 89213
Conc: 0.69 ug/ml

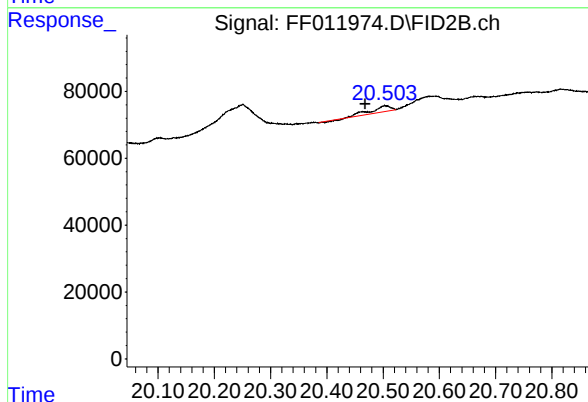

#16 N-HEXATRIACONTANE

R.T.: 20.503 min
Delta R.T.: 0.035 min
Response: 40557
Conc: 0.39 ug/ml