

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
 Data File : FF009833.D
 Signal(s) : FID2B.ch
 Acq On : 03 Feb 2022 12:15
 Operator : AJ\MA
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 03 22:36:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.227	2183699	15.260 ug/ml
12) N-OCTACOSANE	16.601	1919313	13.222 ug/ml
13) N-TRIACONTANE	17.482	66824	0.467 ug/ml
14) N-DOTRIACONTANE	18.318	233129	1.713 ug/ml
15) N-TETRATRIACONTANE	19.093	281452	2.370 ug/ml
16) N-HEXATRIACONTANE	19.869	937954	9.097 ug/ml
17) N-OCTATRIACONTANE	20.497f	856355	9.603 ug/ml
18) N-TETRACONTANE	21.375	350735	3.861 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
Data File : FF009833.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2022 12:15
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 03 22:36:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

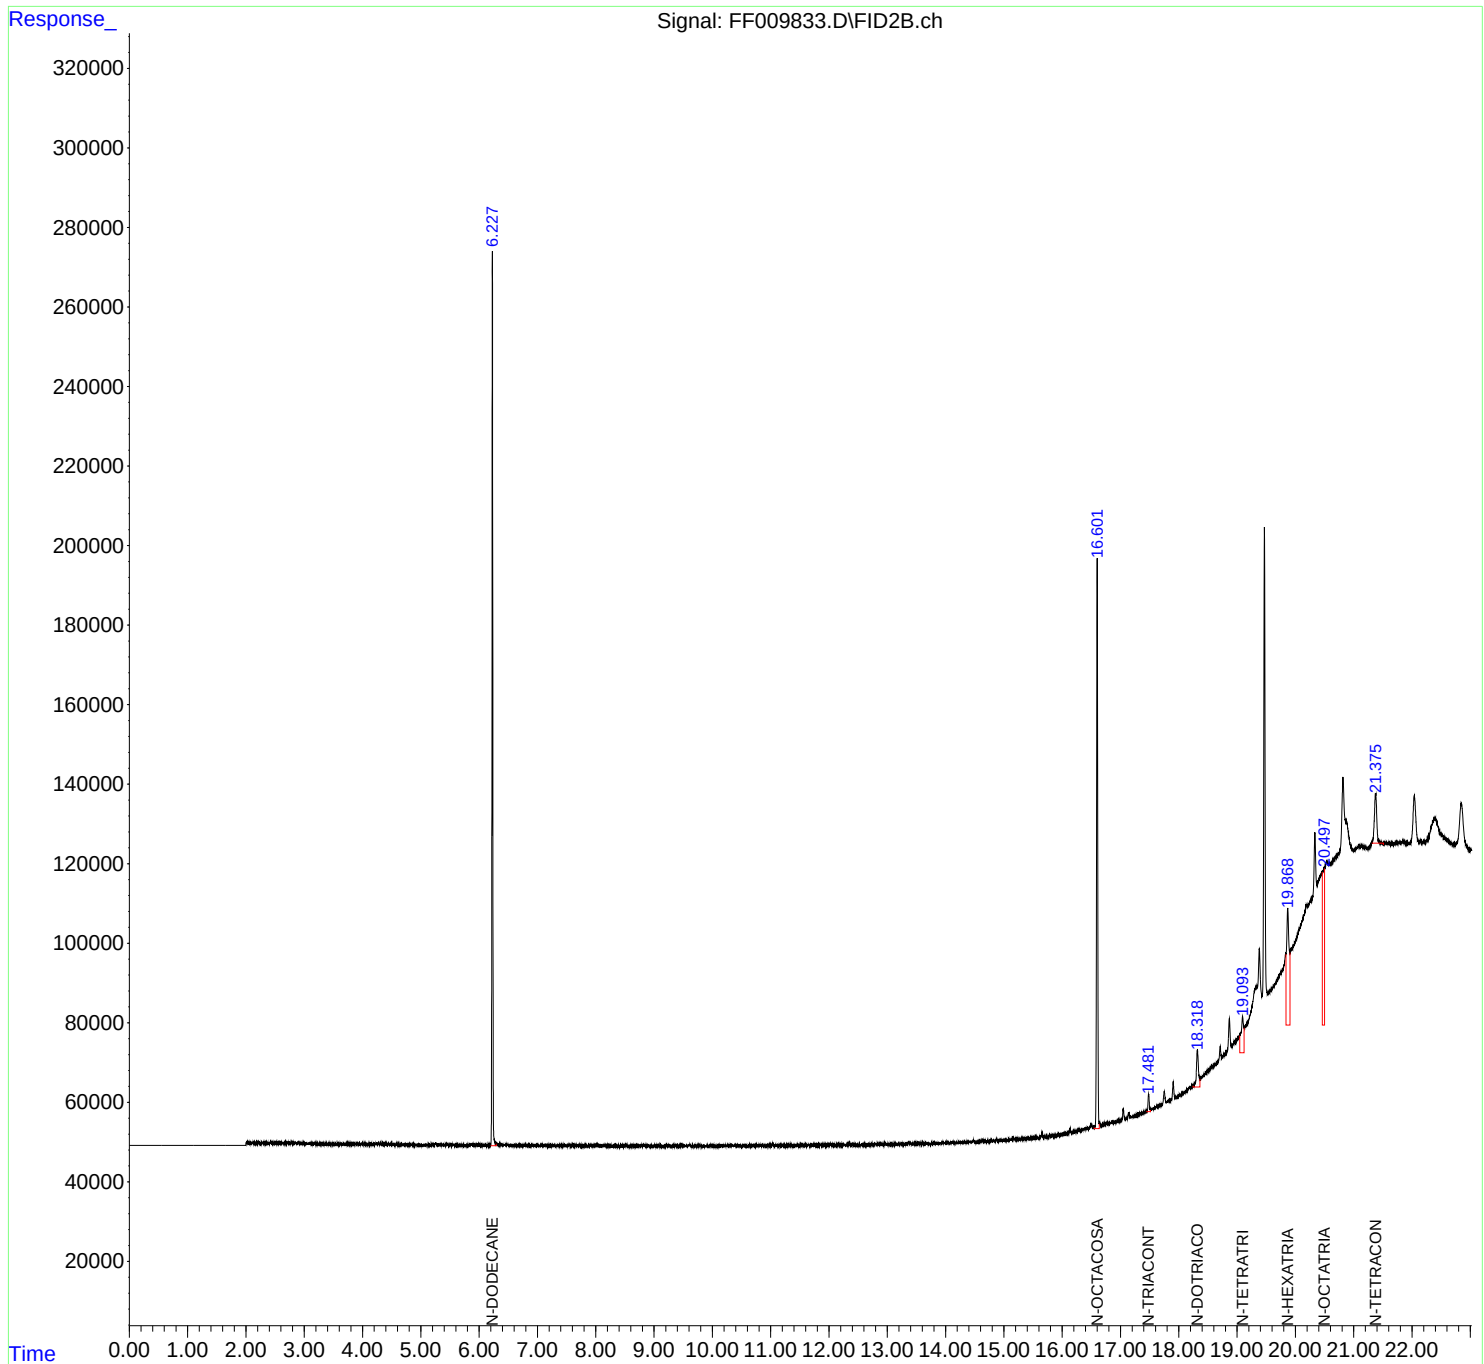


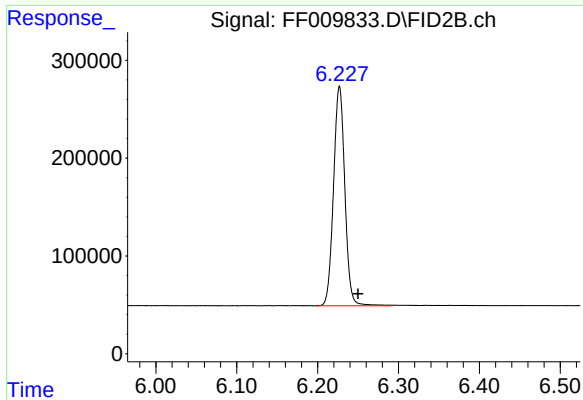

#3 N-DODECANE


R.T.: 6.227 min
Delta R.T.: -0.023 min
Response: 2183699
Conc: 15.26 ug/ml

Instrument :
FID_F
ClientSampleId :

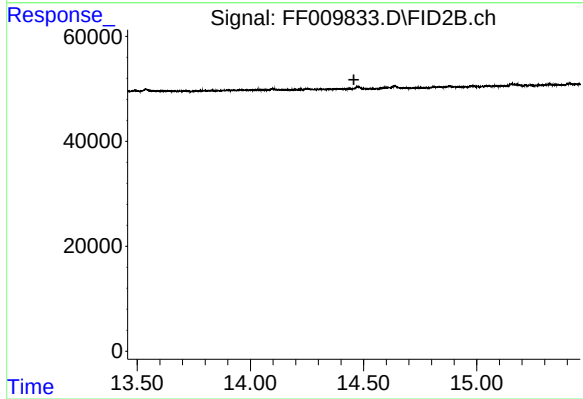


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.457 min
Response: 0
Conc: N.D.

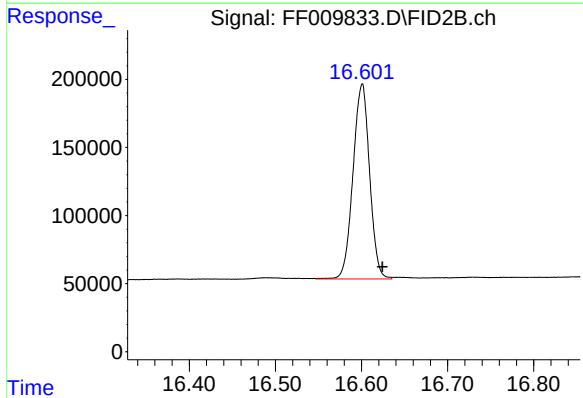


#12 N-OCTACOSANE

R.T.: 16.601 min
Delta R.T.: -0.023 min
Response: 1919313
Conc: 13.22 ug/ml

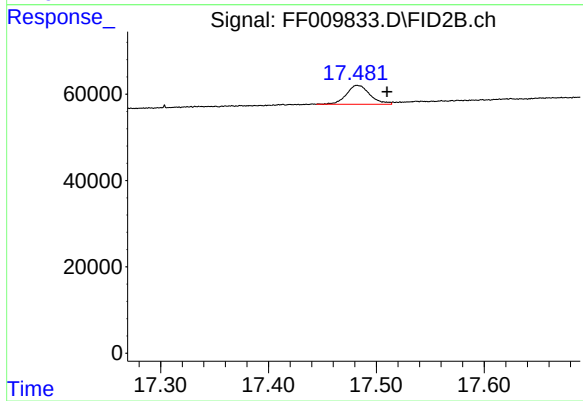

#13 N-TRIACONTANE


R.T.: 17.482 min
Delta R.T.: -0.028 min
Response: 66824
Conc: 0.47 ug/ml

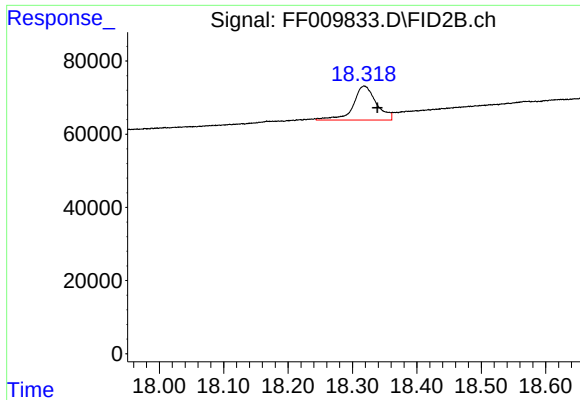

#14 N-DOTRIACONTANE


R.T.: 18.318 min
Delta R.T.: -0.020 min
Response: 233129
Conc: 1.71 ug/ml

Instrument :
FID_F
ClientSampleId :

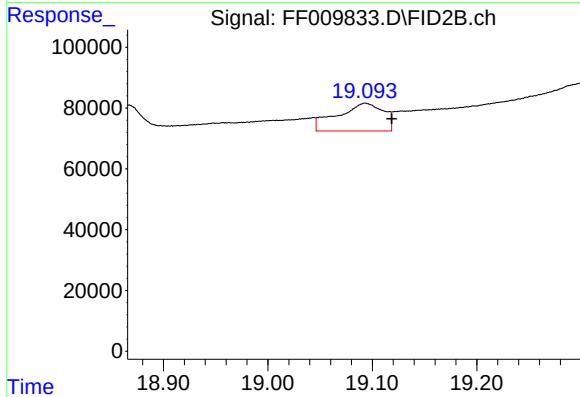


#15 N-TETRATRIACONTANE

R.T.: 19.093 min
Delta R.T.: -0.025 min
Response: 281452
Conc: 2.37 ug/ml

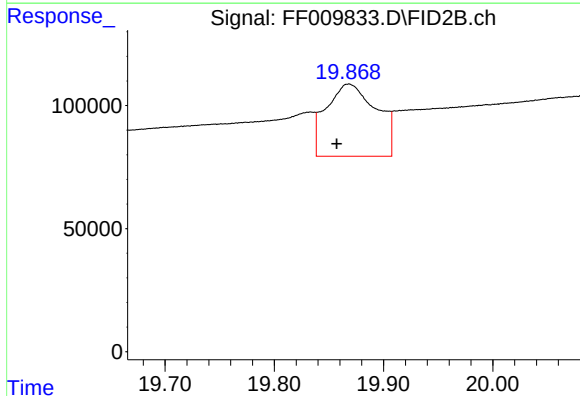


#16 N-HEXATRIACONTANE

R.T.: 19.869 min
Delta R.T.: 0.011 min
Response: 937954
Conc: 9.10 ug/ml

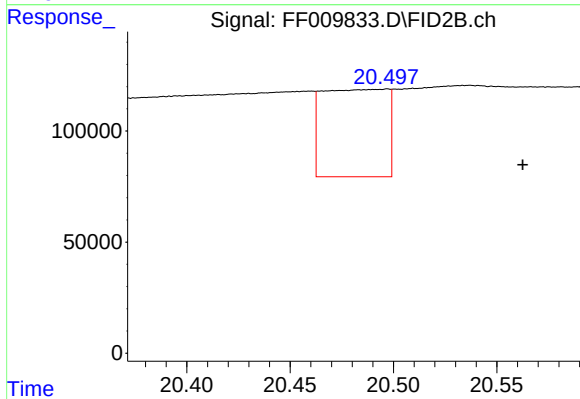

#17 N-OCTATRIACONTANE

R.T.: 20.497 min
Delta R.T.: -0.065 min
Response: 856355
Conc: 9.60 ug/ml

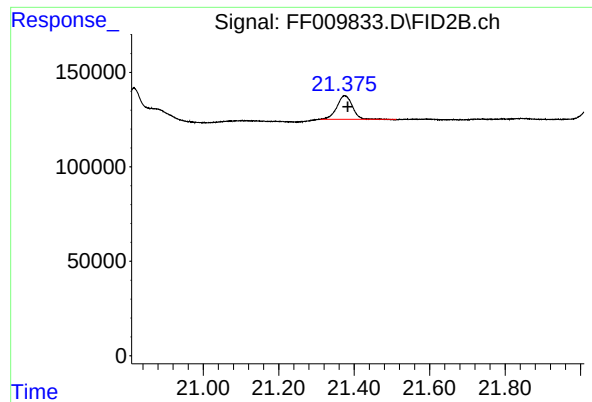

#18 N-TETRACONTANE

R.T.: 21.375 min
Delta R.T.: -0.008 min
Response: 350735
Conc: 3.86 ug/ml

Instrument :

FID_F

ClientSampleId :