

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
 Data File : FF009834.D
 Signal(s) : FID2B.ch
 Acq On : 03 Feb 2022 13:50
 Operator : AJ\MA
 Sample : PB142456BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 03 22:36:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.430	2067700	15.823 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.317	107018	0.786 ug/ml
15) N-TETRATRIACONTANE	19.092	193219	1.627 ug/ml
16) N-HEXATRIACONTANE	19.869	2907471	28.200 ug/ml
18) N-TETRACONTANE	21.375	77425	0.852 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
Data File : FF009834.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2022 13:50
Operator : AJ\MA
Sample : PB142456BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 03 22:36:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

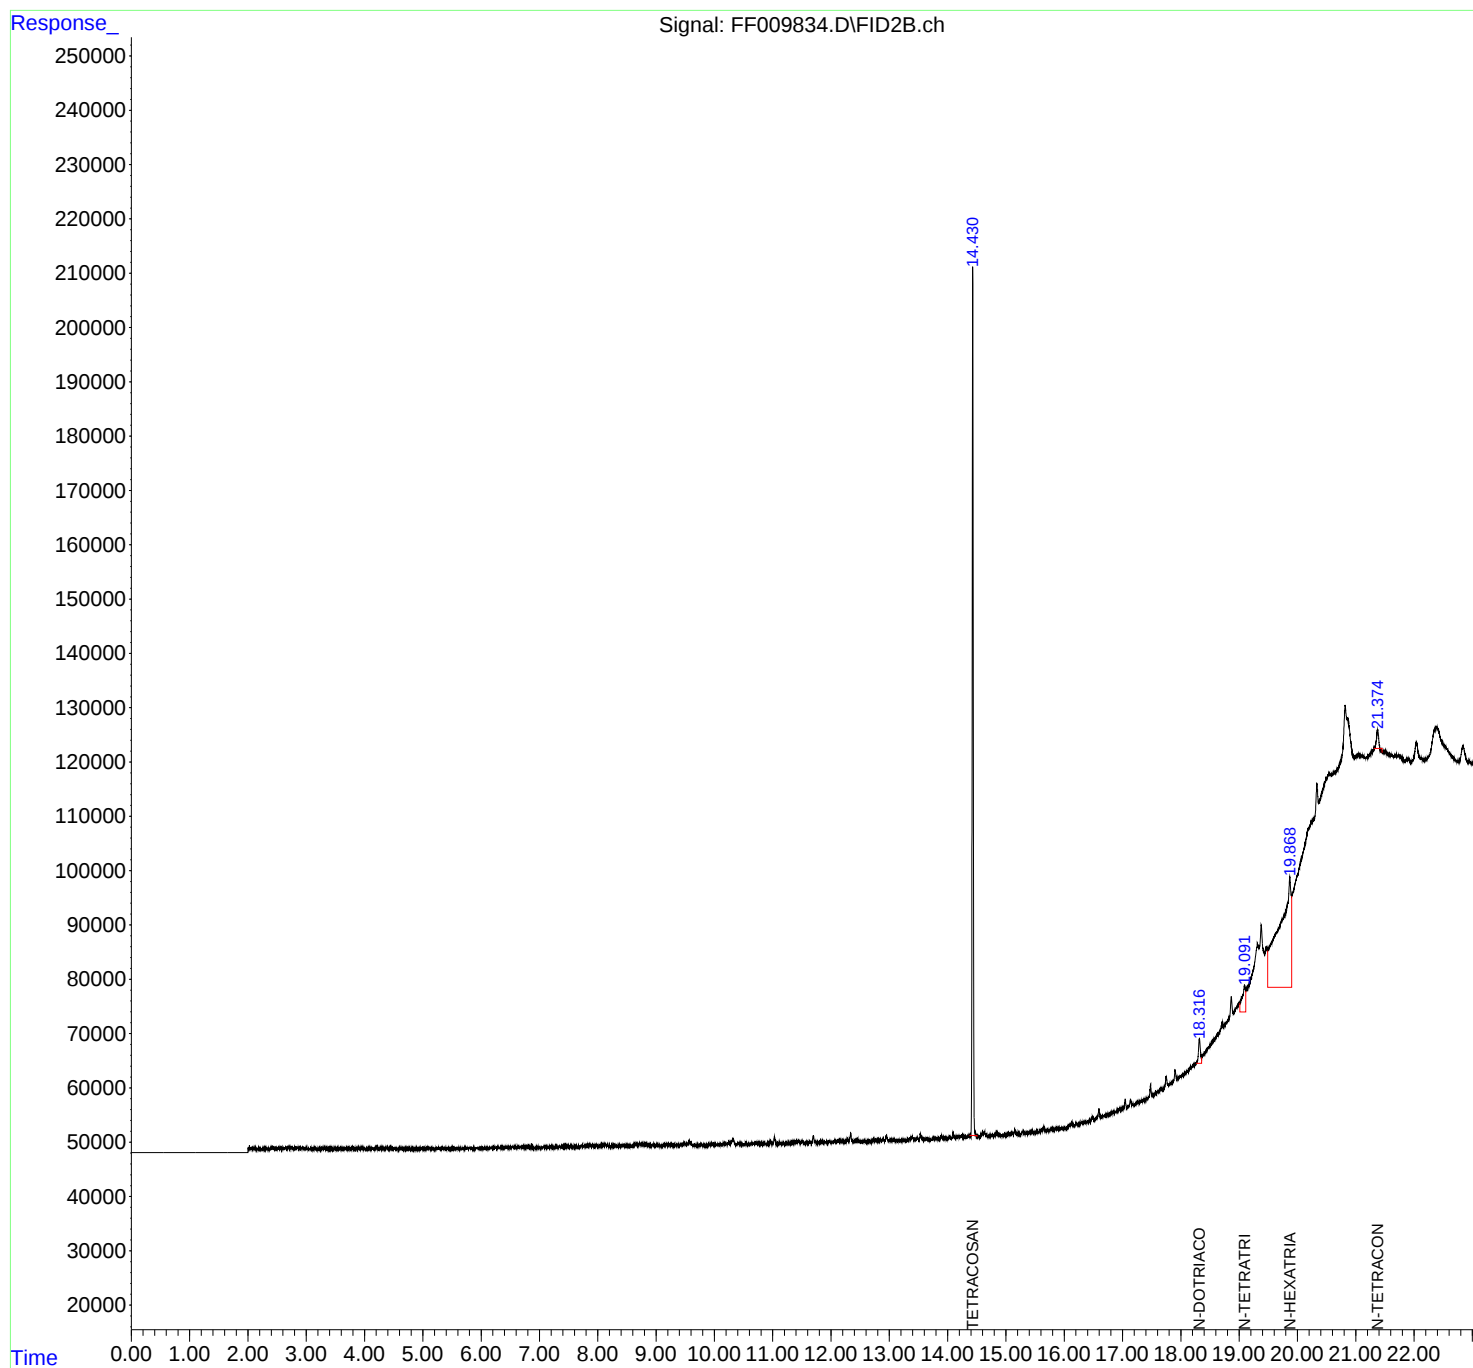


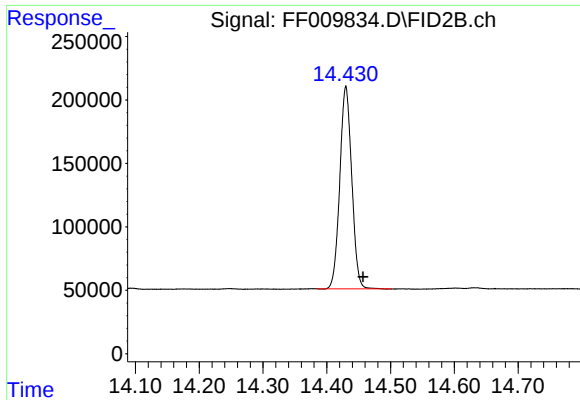

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.430 min
Delta R.T.: -0.027 min
Response: 2067700
Conc: 15.82 ug/ml

Instrument :
FID_F
ClientSampleId :

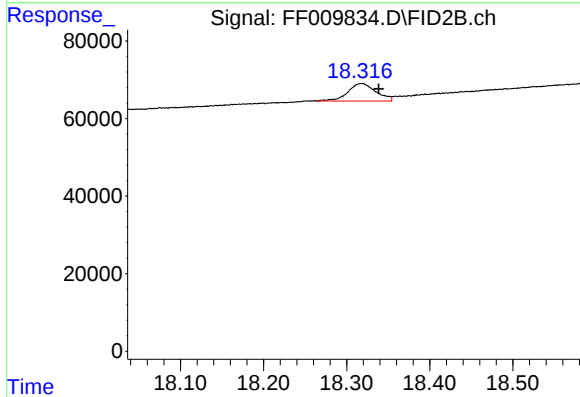


#14 N-DOTRIACONTANE

R.T.: 18.317 min
Delta R.T.: -0.021 min
Response: 107018
Conc: 0.79 ug/ml

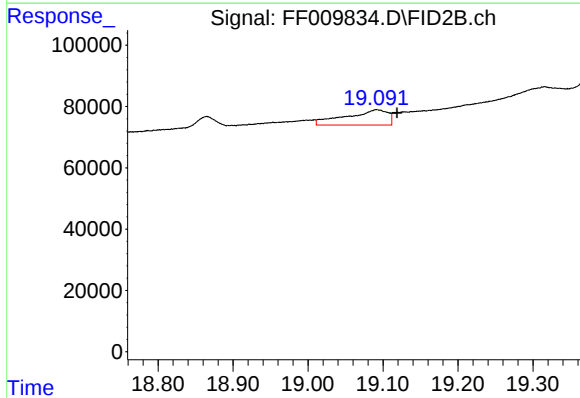


#15 N-TETRATRIACONTANE

R.T.: 19.092 min
Delta R.T.: -0.027 min
Response: 193219
Conc: 1.63 ug/ml

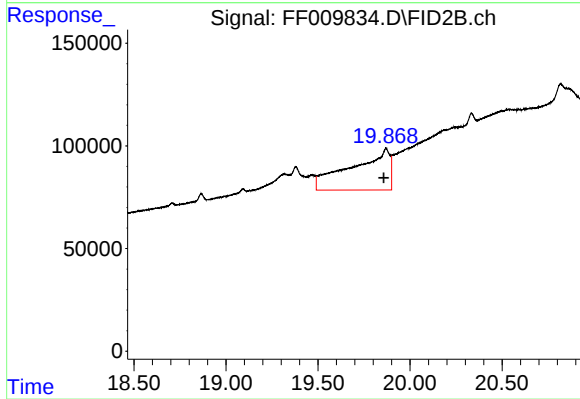

#16 N-HEXATRIACONTANE

R.T.: 19.869 min
Delta R.T.: 0.012 min
Response: 2907471
Conc: 28.20 ug/ml

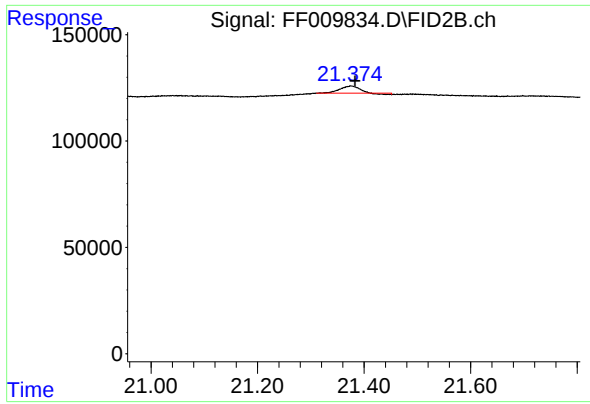

#18 N-TETRACONTANE

R.T.: 21.375 min
Delta R.T.: -0.008 min
Response: 77425
Conc: 0.85 ug/ml

Instrument :

FID_F

ClientSampleId :