

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
 Data File : FF009840.D
 Signal(s) : FID2B.ch
 Acq On : 03 Feb 2022 16:48
 Operator : AJ\MA
 Sample : N1381-04
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 03 22:36:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.434	1443520	11.046 ug/ml
Target Compounds			
4) N-TETRADECANE	8.052	203721	1.386 ug/ml
6) N-OCTADECANE	11.128f	53318	0.346 ug/ml
11) N-HEXACOSANE	15.651	86505	0.592 ug/ml
12) N-OCTACOSANE	16.600	90456	0.623 ug/ml
13) N-TRIACONTANE	17.482	247675	1.731 ug/ml
14) N-DOTRIACONTANE	18.318	470720	3.459 ug/ml
15) N-TETRATRIACONTANE	19.112	441818	3.720 ug/ml
16) N-HEXATRIACONTANE	19.873	1607413	15.590 ug/ml
18) N-TETRACONTANE	21.378	512371	5.641 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
Data File : FF009840.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2022 16:48
Operator : AJ\MA
Sample : N1381-04
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 03 22:36:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

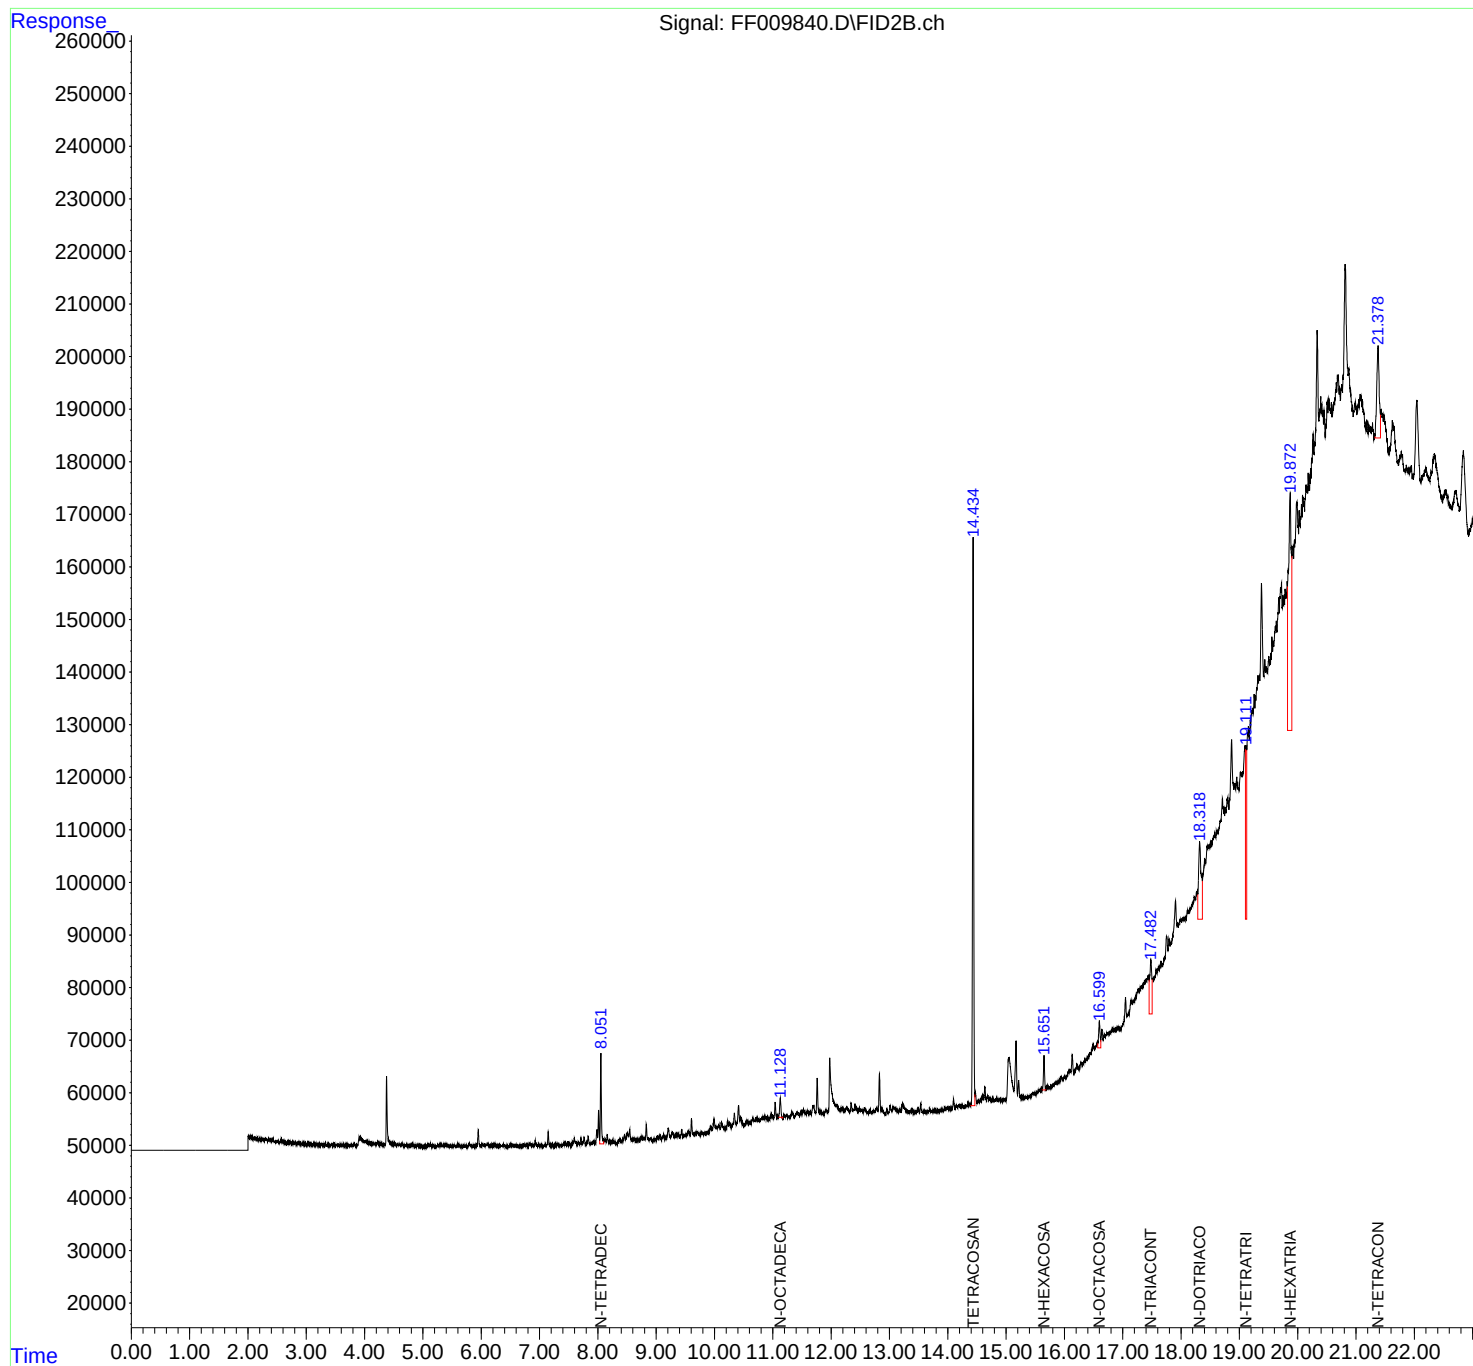


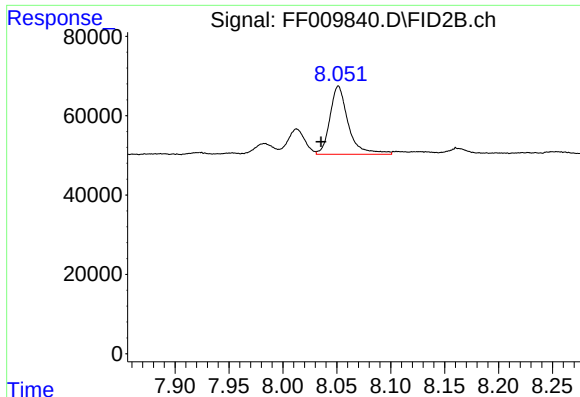

#4 N-TETRADECANE


R.T.: 8.052 min
Delta R.T.: 0.016 min
Response: 203721
Conc: 1.39 ug/ml

Instrument :
FID_F
ClientSampleId :

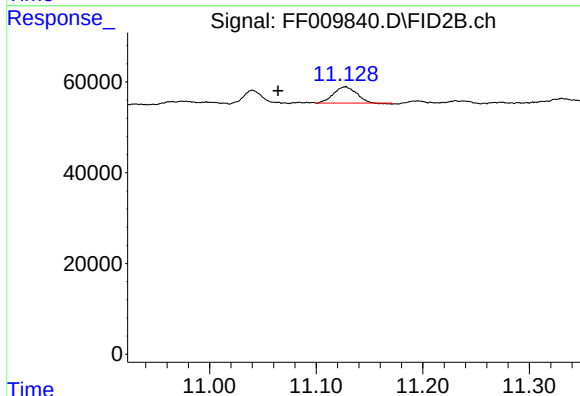


#6 N-OCTADECANE

R.T.: 11.128 min
Delta R.T.: 0.064 min
Response: 53318
Conc: 0.35 ug/ml

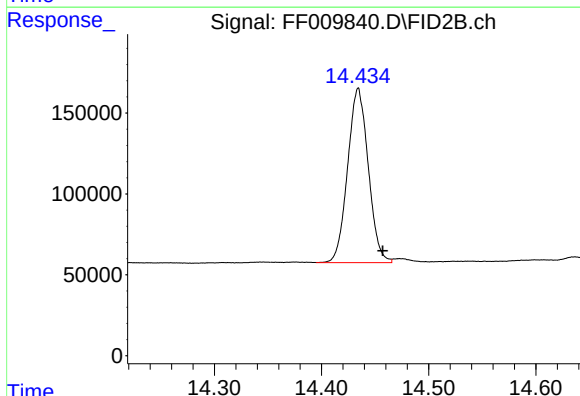


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.434 min
Delta R.T.: -0.023 min
Response: 1443520
Conc: 11.05 ug/ml

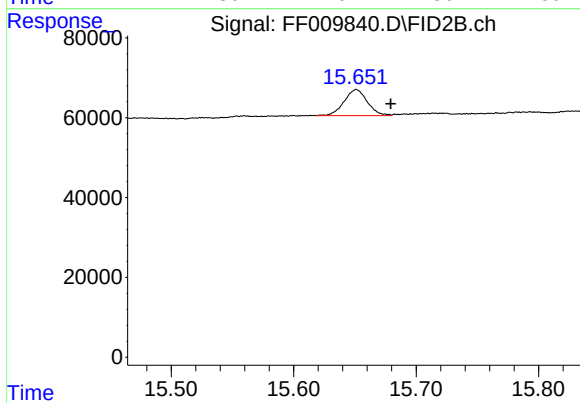

#11 N-HEXACOSANE


R.T.: 15.651 min
Delta R.T.: -0.028 min
Response: 86505
Conc: 0.59 ug/ml

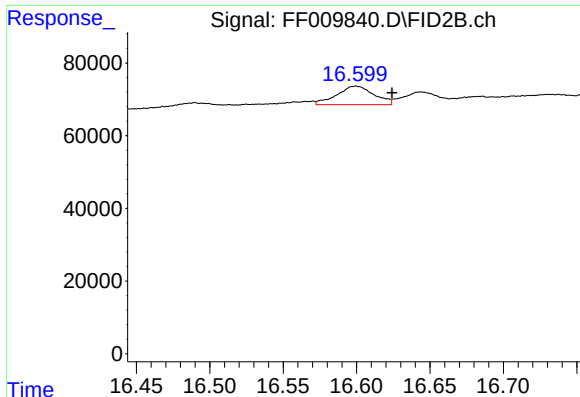

#12 N-OCTACOSANE


R.T.: 16.600 min
Delta R.T.: -0.025 min
Response: 90456
Conc: 0.62 ug/ml

Instrument :
FID_F
ClientSampleId :

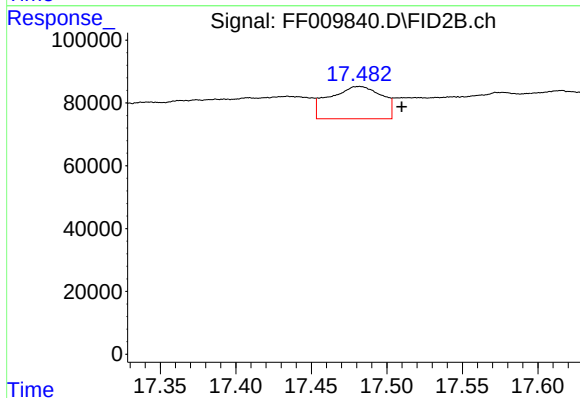


#13 N-TRIACONTANE

R.T.: 17.482 min
Delta R.T.: -0.028 min
Response: 247675
Conc: 1.73 ug/ml

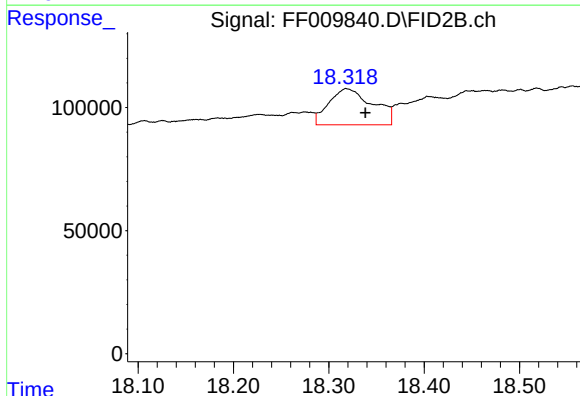


#14 N-DOTRIACONTANE

R.T.: 18.318 min
Delta R.T.: -0.020 min
Response: 470720
Conc: 3.46 ug/ml

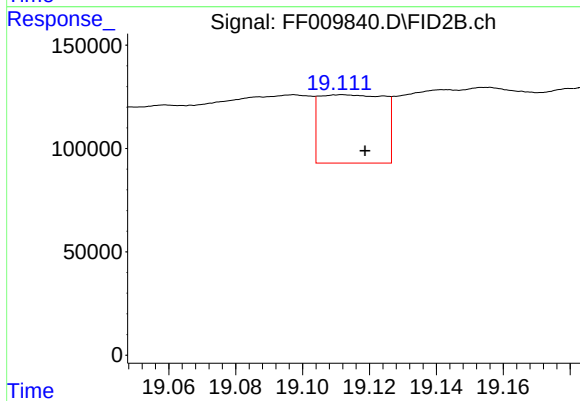

#15 N-TETRATRIACONTANE


R.T.: 19.112 min
Delta R.T.: -0.007 min
Response: 441818
Conc: 3.72 ug/ml

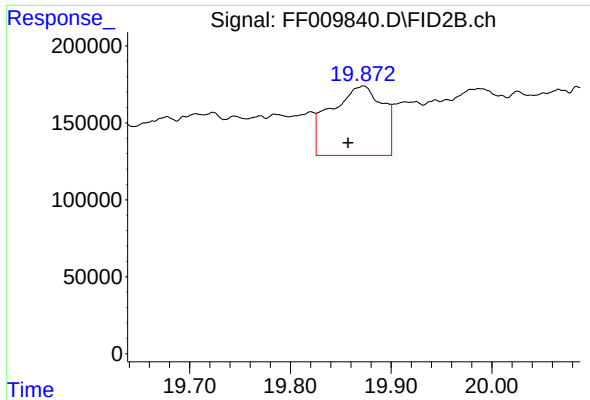

#16 N-HEXATRIACONTANE

R.T.: 19.873 min
Delta R.T.: 0.015 min
Response: 1607413
Conc: 15.59 ug/ml

Instrument :
FID_F
ClientSampleId :

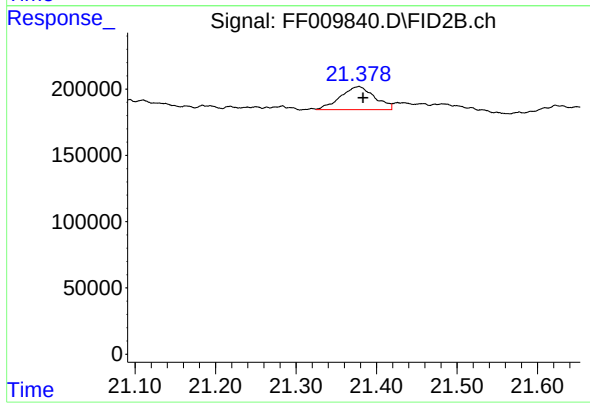

#18 N-TETRACONTANE

R.T.: 21.378 min
Delta R.T.: -0.005 min
Response: 512371
Conc: 5.64 ug/ml