

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
Data File : FF009843.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2022 18:17
Operator : AJ\MA
Sample : N1381-07
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 03 22:37:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.268	93838	0.656 ug/ml
4) N-TETRADECANE	8.045	461155	3.138 ug/ml
5) N-HEXADECANE	9.614	2903247	19.408 ug/ml
6) N-OCTADECANE	11.062	1517322	9.842 ug/ml
7) N-EICOSANE	12.370	18365	0.121 ug/ml
8) N-DOCOSANE	13.558	19863	0.134 ug/ml
16) N-HEXATRIACONTANE	19.853	114739	1.113 ug/ml
17) N-OCTATRIACONTANE	20.575	56155	0.630 ug/ml
18) N-TETRACONTANE	21.383	21784	0.240 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
Data File : FF009843.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2022 18:17
Operator : AJ\MA
Sample : N1381-07
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 03 22:37:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

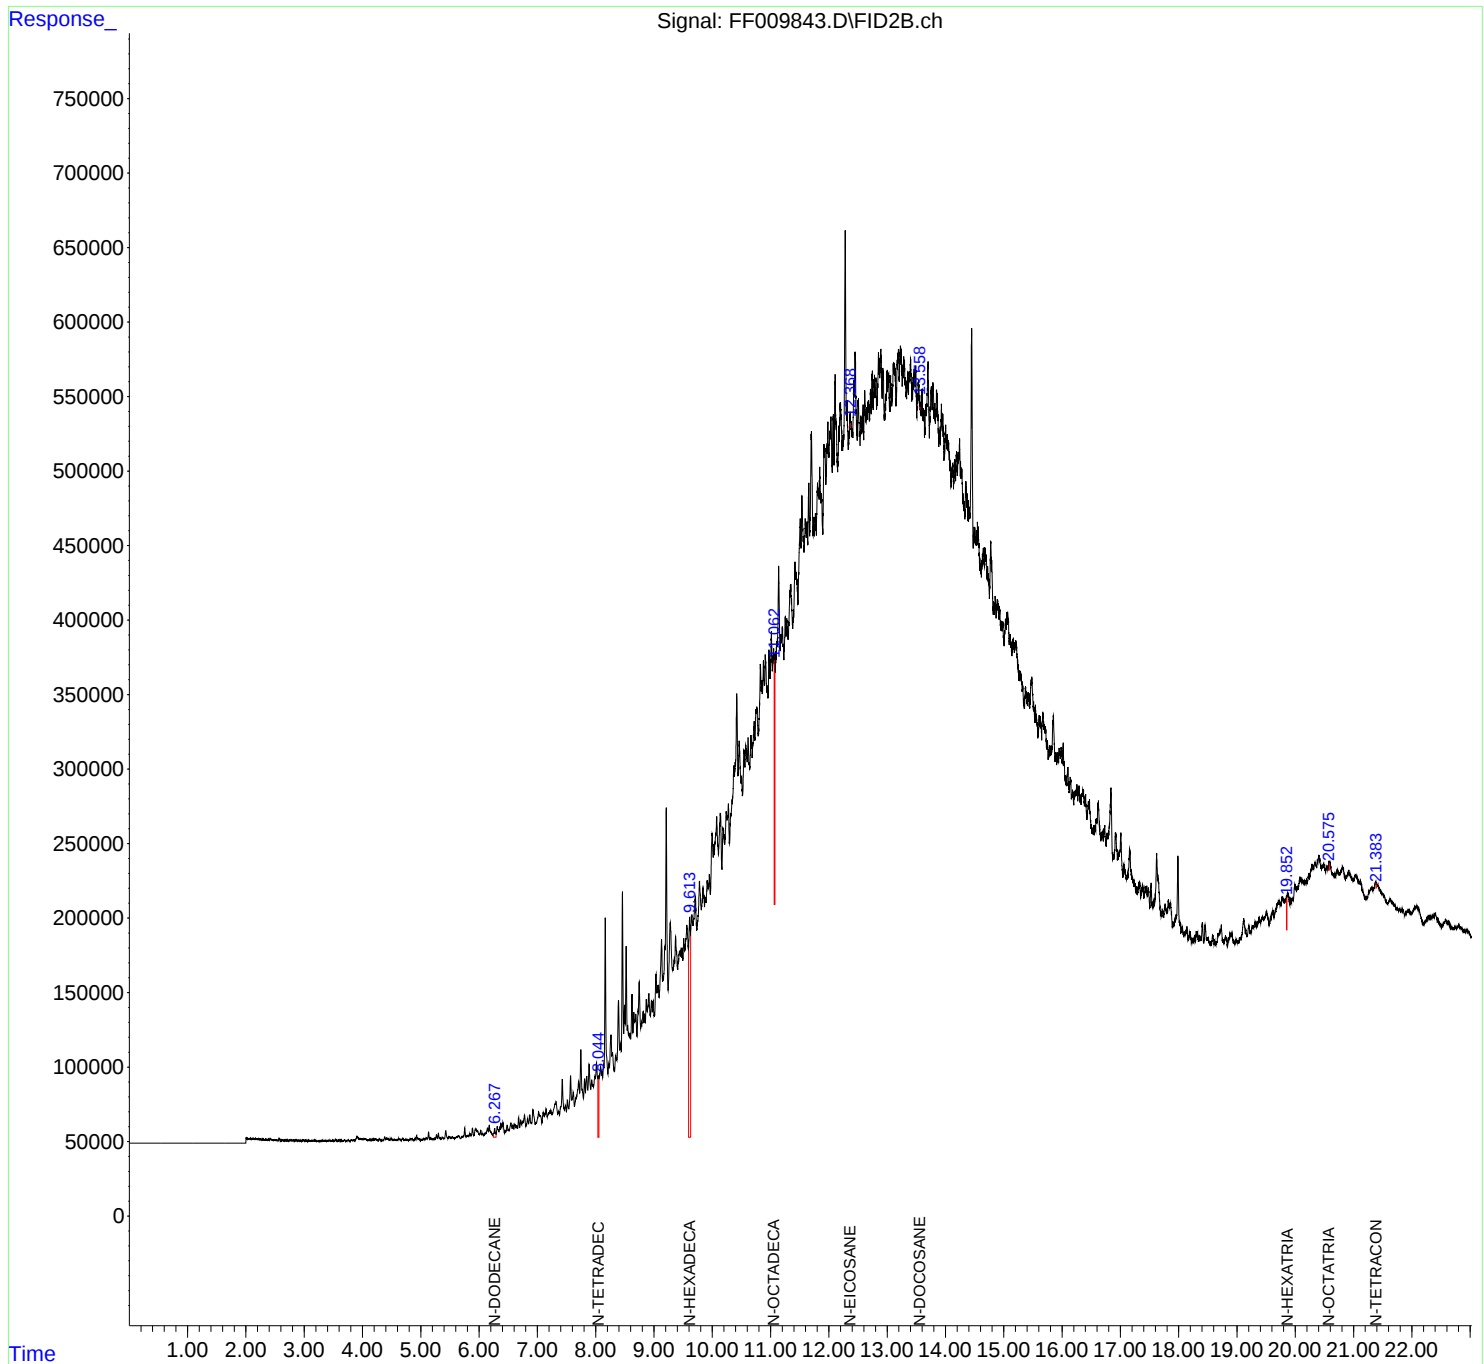


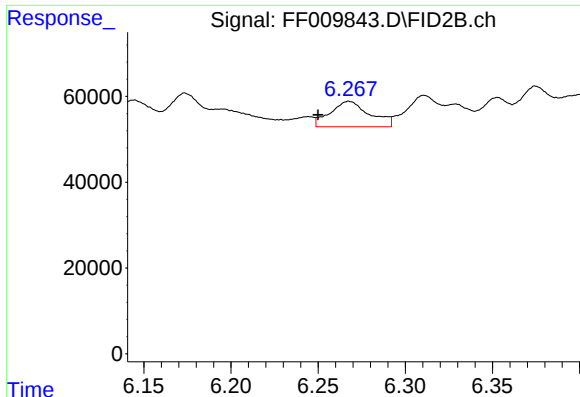

#3 N-DODECANE


R.T.: 6.268 min
Delta R.T.: 0.018 min
Response: 93838
Conc: 0.66 ug/ml

Instrument :
FID_F
ClientSampleId :

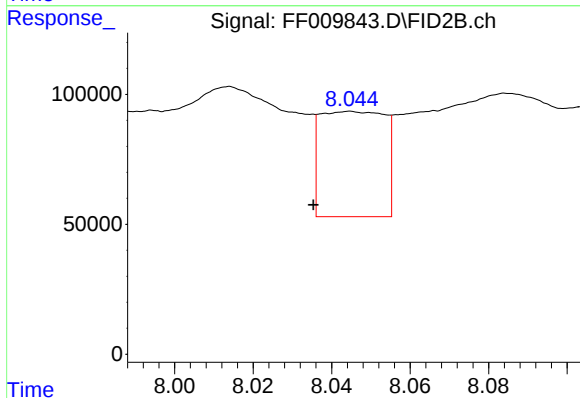


#4 N-TETRADECANE

R.T.: 8.045 min
Delta R.T.: 0.009 min
Response: 461155
Conc: 3.14 ug/ml

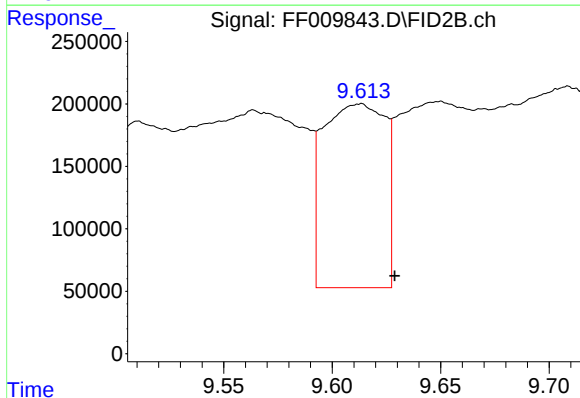


#5 N-HEXADECANE

R.T.: 9.614 min
Delta R.T.: -0.015 min
Response: 2903247
Conc: 19.41 ug/ml

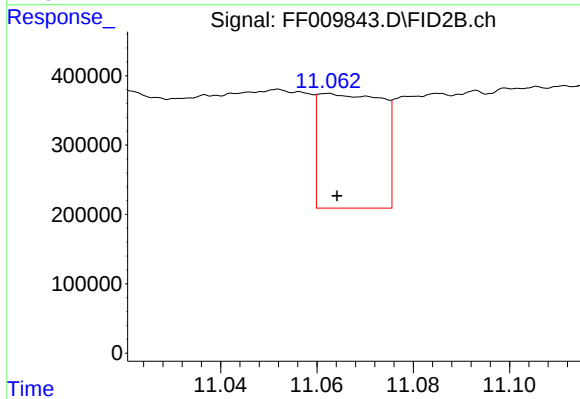

#6 N-OCTADECANE


R.T.: 11.062 min
Delta R.T.: -0.002 min
Response: 1517322
Conc: 9.84 ug/ml

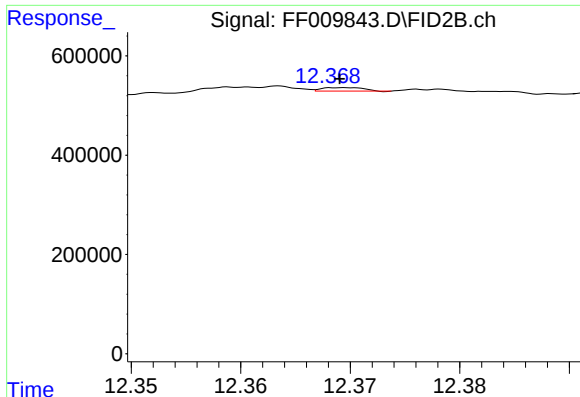

#7 N-EICOSANE


R.T.: 12.370 min
Delta R.T.: 0.000 min
Response: 18365
Conc: 0.12 ug/ml

Instrument :
FID_F
ClientSampleId :

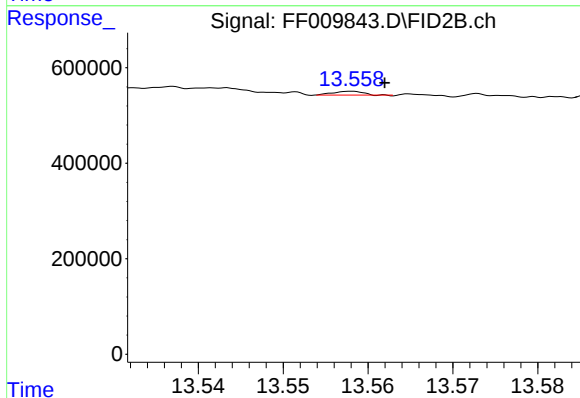


#8 N-DOCOSANE

R.T.: 13.558 min
Delta R.T.: -0.004 min
Response: 19863
Conc: 0.13 ug/ml

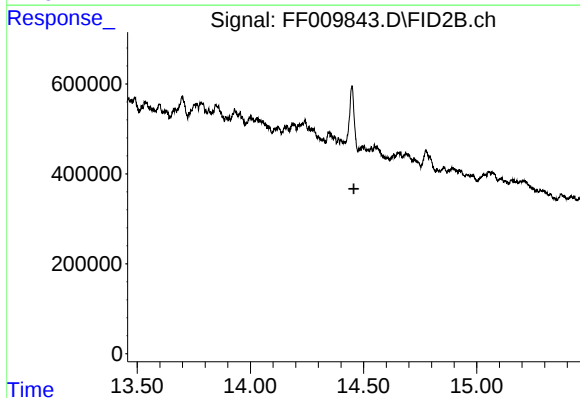


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.449 min
Delta R.T.: -0.008 min
Response: -811107
Conc: N.D.

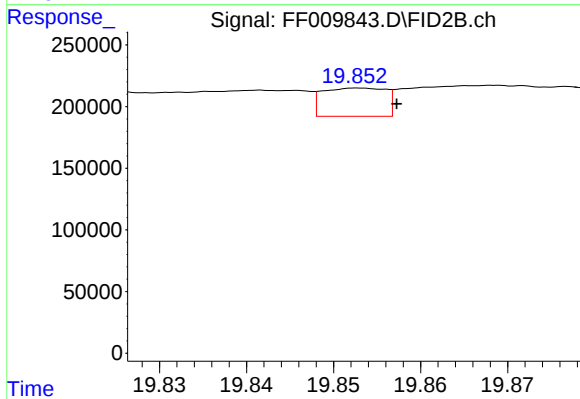

#16 N-HEXATRIACONTANE


R.T.: 19.853 min
Delta R.T.: -0.004 min
Response: 114739
Conc: 1.11 ug/ml

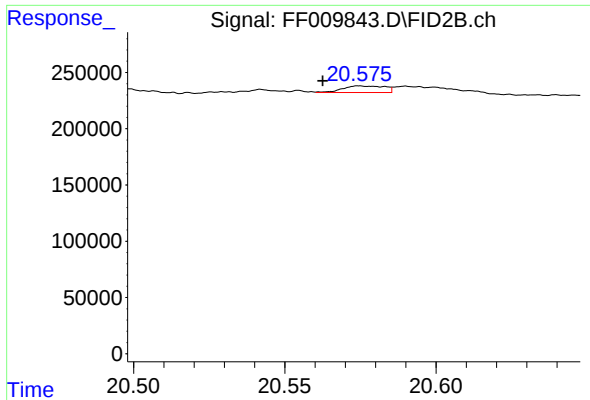

#17 N-OCTATRIACONTANE

R.T.: 20.575 min
Delta R.T.: 0.012 min
Response: 56155
Conc: 0.63 ug/ml

Instrument :
FID_F
ClientSampleId :

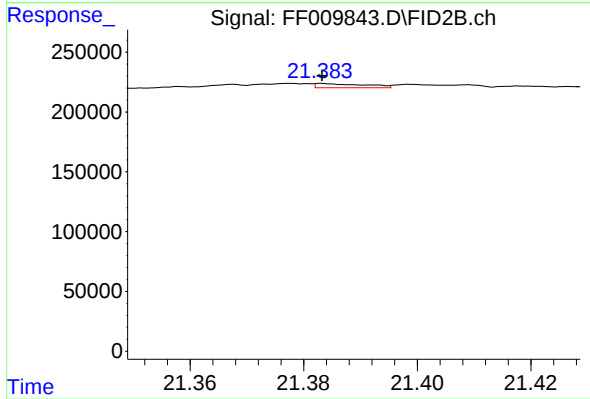

#18 N-TETRACONTANE

R.T.: 21.383 min
Delta R.T.: 0.000 min
Response: 21784
Conc: 0.24 ug/ml