

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
 Data File : FF009846.D
 Signal(s) : FID2B.ch
 Acq On : 03 Feb 2022 19:45
 Operator : AJ\MA
 Sample : N1381-08
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 03 22:37:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.434	2341463	17.918 ug/ml
Target Compounds			
4) N-TETRADECANE	8.012	61132	0.416 ug/ml
5) N-HEXADECANE	9.605	26874	0.180 ug/ml
6) N-OCTADECANE	11.040	51111	0.332 ug/ml
10) N-TETRACOSANE	14.636	54749	0.369 ug/ml
11) N-HEXACOSANE	15.652	56365	0.386 ug/ml
12) N-OCTACOSANE	16.597	80430	0.554 ug/ml
13) N-TRIACONTANE	17.482	147313	1.030 ug/ml
14) N-DOTRIACONTANE	18.307	236258	1.736 ug/ml
15) N-TETRATRIACONTANE	19.090	730351	6.149 ug/ml
16) N-HEXATRIACONTANE	19.868	772432	7.492 ug/ml
17) N-OCTATRIACONTANE	20.533	72832	0.817 ug/ml
18) N-TETRACONTANE	21.373	160659	1.769 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
Data File : FF009846.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2022 19:45
Operator : AJ\MA
Sample : N1381-08
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 03 22:37:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

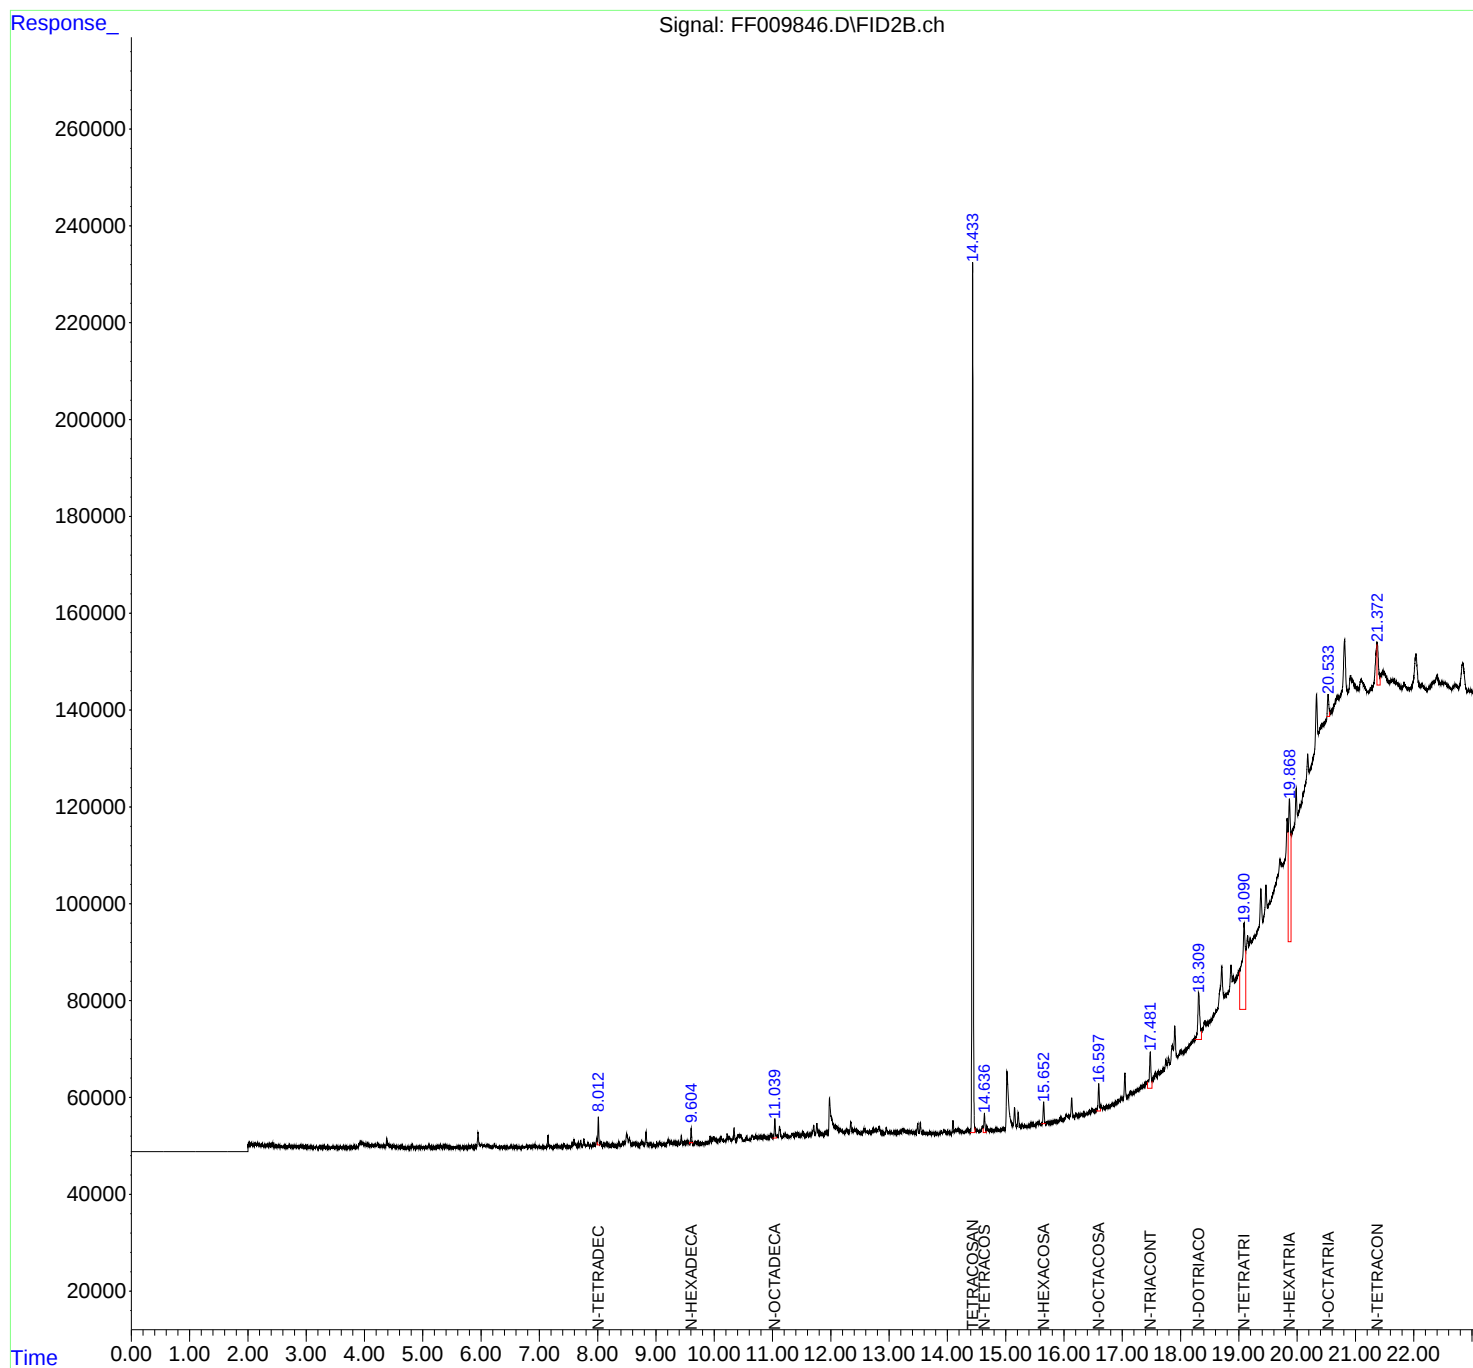


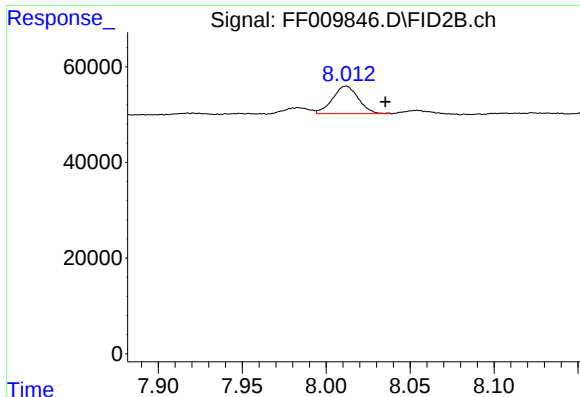

#4 N-TETRADECANE


R.T.: 8.012 min
Delta R.T.: -0.023 min
Response: 61132
Conc: 0.42 ug/ml

Instrument :
FID_F
ClientSampleId :

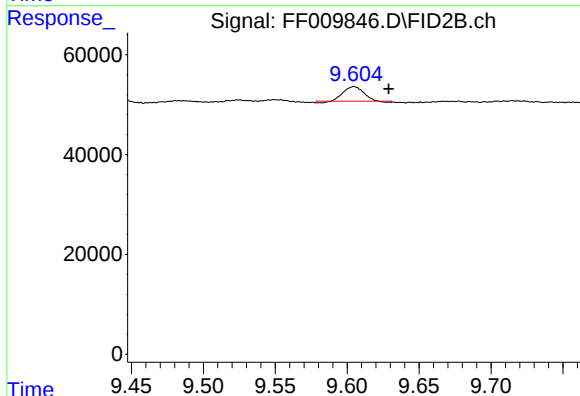


#5 N-HEXADECANE

R.T.: 9.605 min
Delta R.T.: -0.024 min
Response: 26874
Conc: 0.18 ug/ml

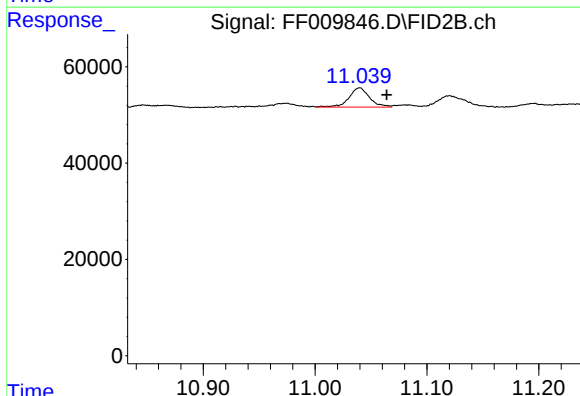


#6 N-OCTADECANE

R.T.: 11.040 min
Delta R.T.: -0.024 min
Response: 51111
Conc: 0.33 ug/ml

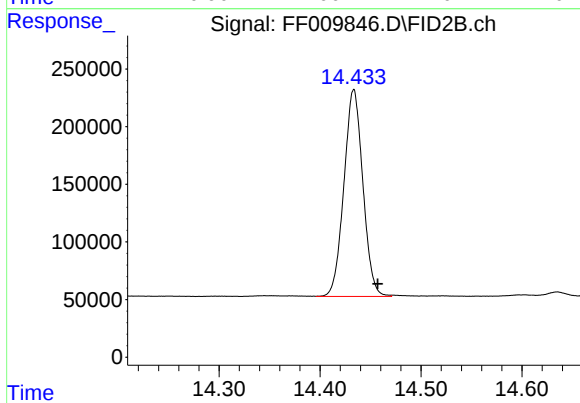

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.434 min
Delta R.T.: -0.023 min
Response: 2341463
Conc: 17.92 ug/ml

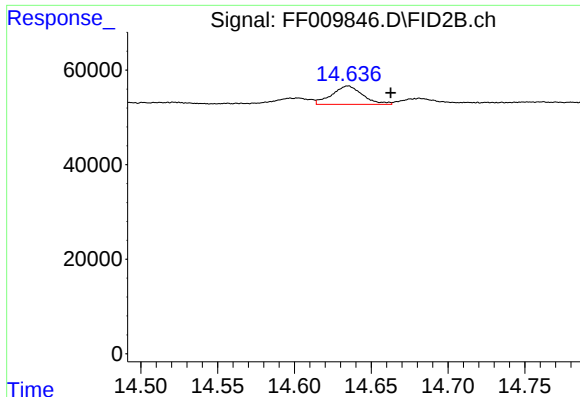

#10 N-TETRACOSANE


R.T.: 14.636 min
Delta R.T.: -0.027 min
Response: 54749
Conc: 0.37 ug/ml

Instrument :
FID_F
ClientSampleId :

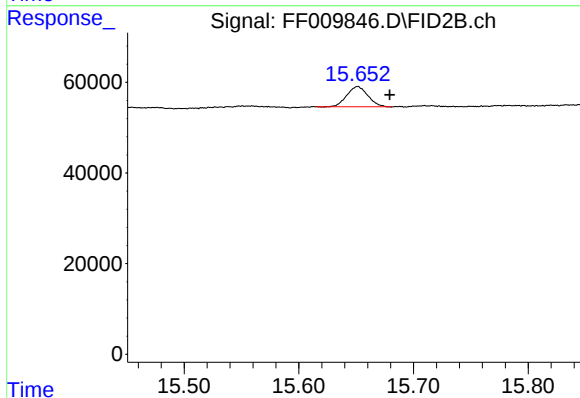


#11 N-HEXACOSANE

R.T.: 15.652 min
Delta R.T.: -0.028 min
Response: 56365
Conc: 0.39 ug/ml

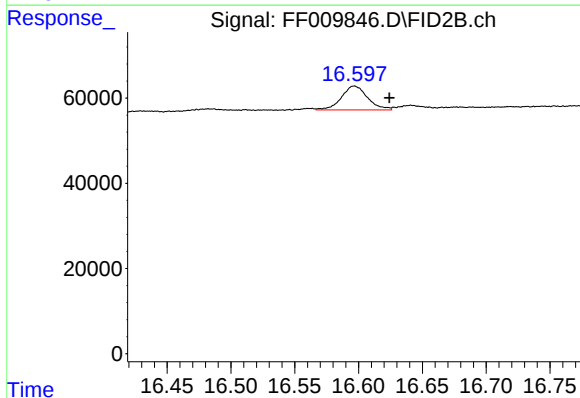


#12 N-OCTACOSANE

R.T.: 16.597 min
Delta R.T.: -0.027 min
Response: 80430
Conc: 0.55 ug/ml

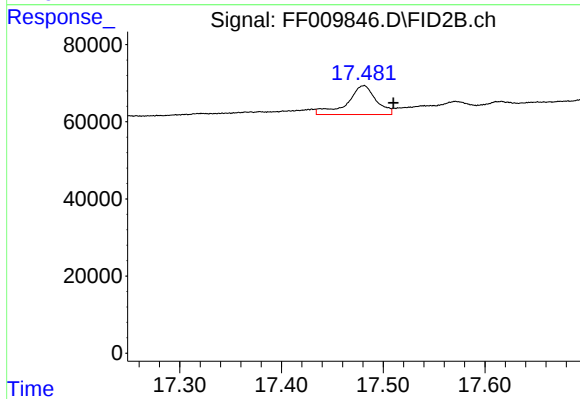

#13 N-TRIACONTANE


R.T.: 17.482 min
Delta R.T.: -0.028 min
Response: 147313
Conc: 1.03 ug/ml

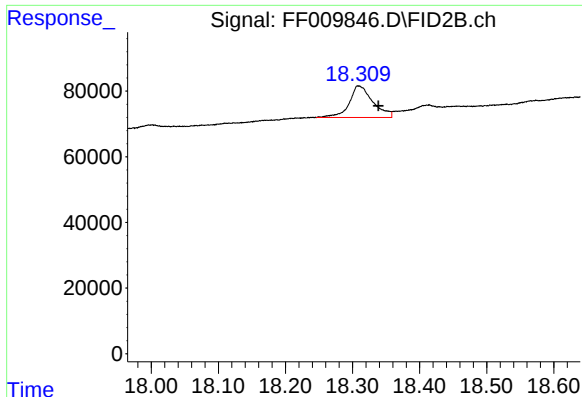

#14 N-DOTRIACONTANE


R.T.: 18.307 min
Delta R.T.: -0.031 min
Response: 236258
Conc: 1.74 ug/ml

Instrument :
FID_F
ClientSampleId :

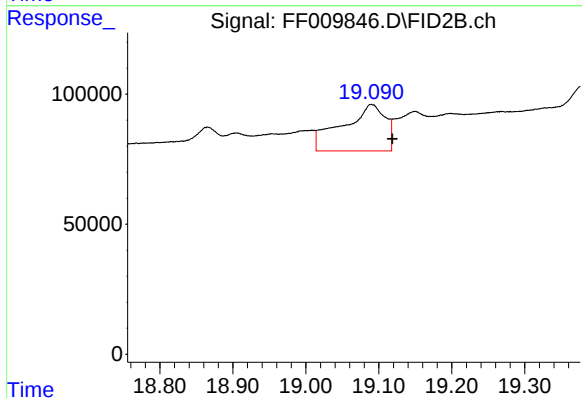


#15 N-TETRATRIACONTANE

R.T.: 19.090 min
Delta R.T.: -0.028 min
Response: 730351
Conc: 6.15 ug/ml

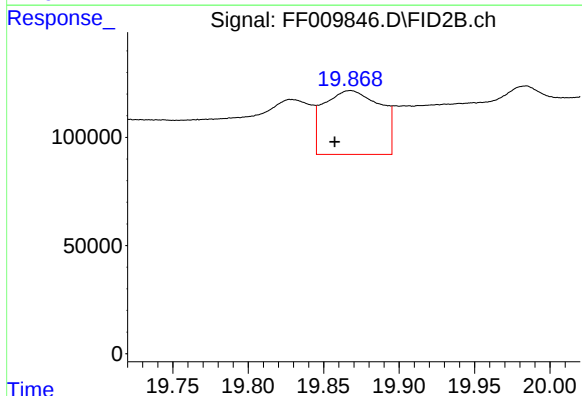


#16 N-HEXATRIACONTANE

R.T.: 19.868 min
Delta R.T.: 0.011 min
Response: 772432
Conc: 7.49 ug/ml

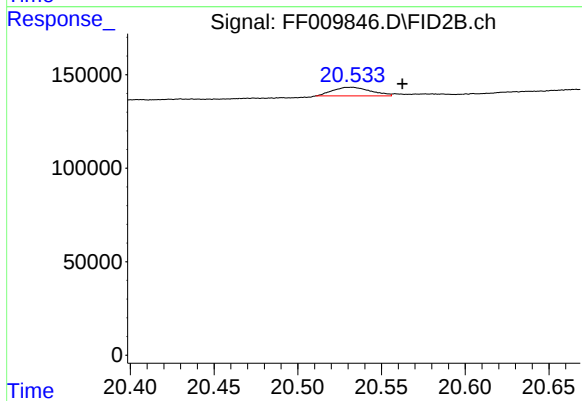

#17 N-OCTATRIACONTANE

R.T.: 20.533 min
Delta R.T.: -0.029 min
Response: 72832
Conc: 0.82 ug/ml

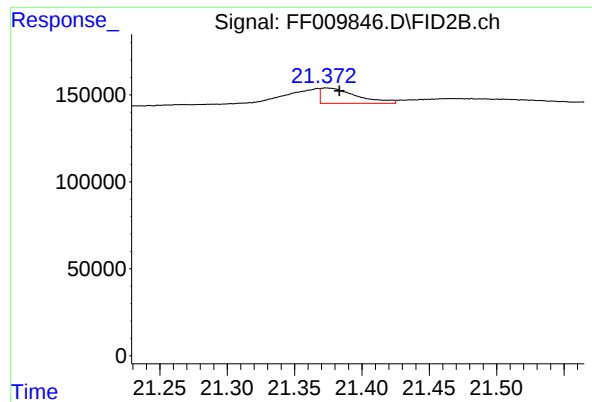

#18 N-TETRACONTANE

R.T.: 21.373 min
Delta R.T.: -0.011 min
Response: 160659
Conc: 1.77 ug/ml

Instrument :

FID_F

ClientSampleId :