

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
Data File : FF009852.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2022 22:42
Operator : AJ\MA
Sample : N1381-03 100X
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 03 23:33:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
6)	N-OCTADECANE	11.128f	49983	0.324 ug/ml
14)	N-DOTRIACONTANE	18.315	484777	3.562 ug/ml
15)	N-TETRATRIACONTANE	19.109	267400	2.251 ug/ml
16)	N-HEXATRIACONTANE	19.870	4080766	39.579 ug/ml
18)	N-TETRACONTANE	21.374	442316	4.869 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
Data File : FF009852.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2022 22:42
Operator : AJ\MA
Sample : N1381-03 100X
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 03 23:33:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

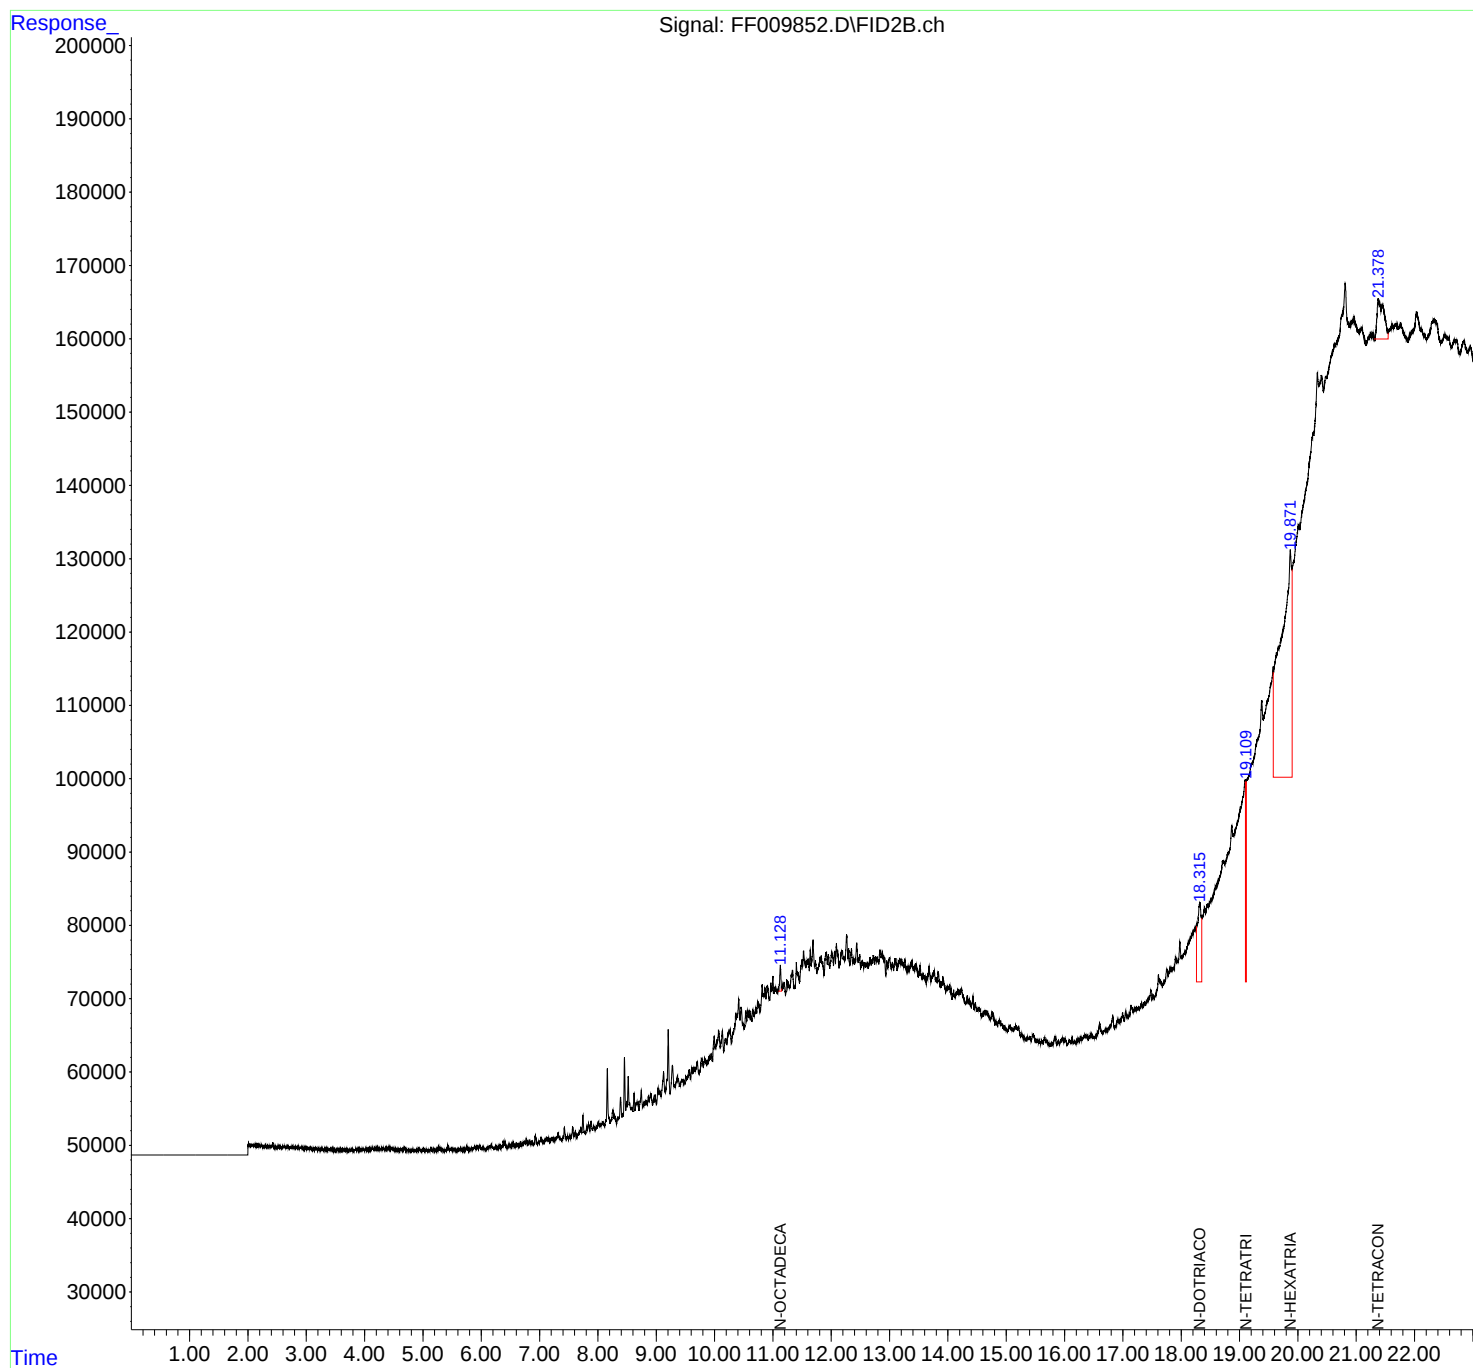


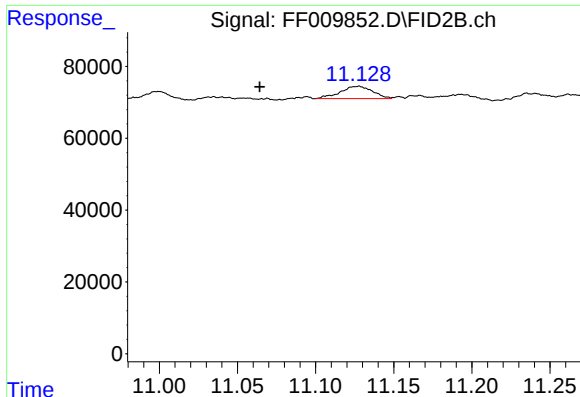

#6 N-OCTADECANE


R.T.: 11.128 min
Delta R.T.: 0.064 min
Response: 49983
Conc: 0.32 ug/ml

Instrument :
FID_F
ClientSampleId :

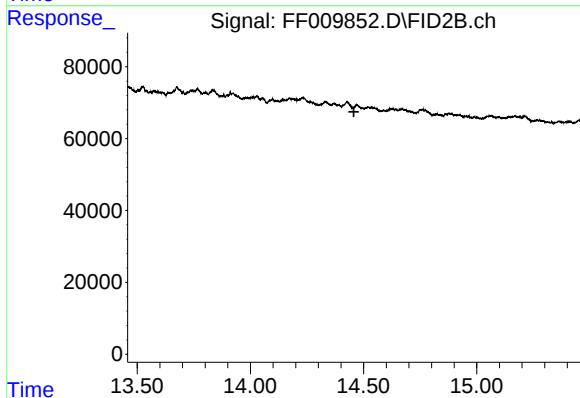


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.457 min
Response: 0
Conc: N.D.

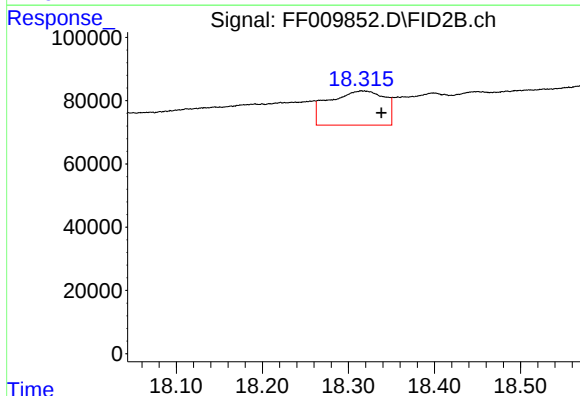


#14 N-DOTRIACONTANE

R.T.: 18.315 min
Delta R.T.: -0.023 min
Response: 484777
Conc: 3.56 ug/ml

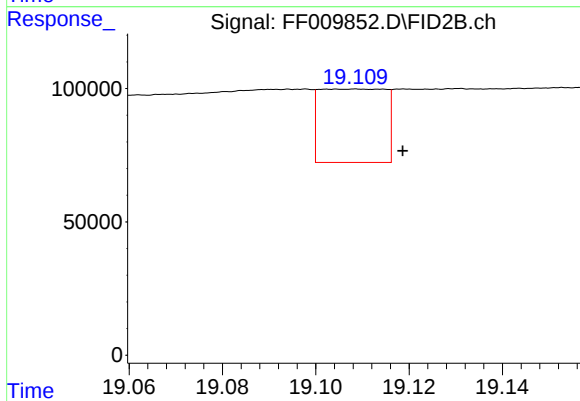

#15 N-TETRATRIACONTANE


R.T.: 19.109 min
Delta R.T.: -0.010 min
Response: 267400
Conc: 2.25 ug/ml

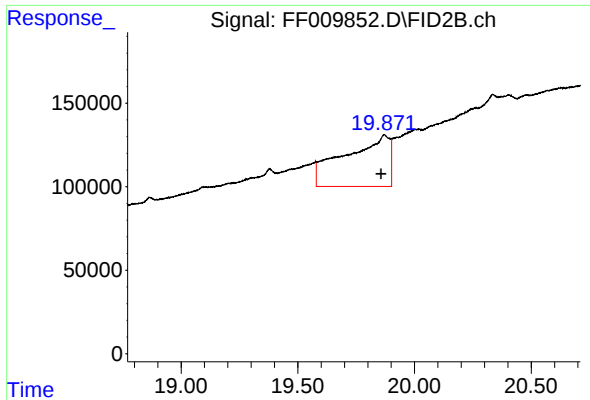

#16 N-HEXATRIACONTANE

R.T.: 19.870 min
Delta R.T.: 0.013 min
Response: 4080766
Conc: 39.58 ug/ml

Instrument :
FID_F
ClientSampleId :

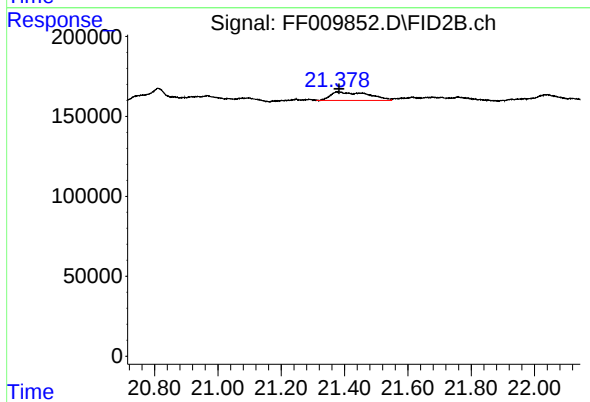

#18 N-TETRACONTANE

R.T.: 21.374 min
Delta R.T.: -0.009 min
Response: 442316
Conc: 4.87 ug/ml