

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
 Data File : FF009856.D
 Signal(s) : FID2B.ch
 Acq On : 04 Feb 2022 00:40
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 04 01:48:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.474	96993	0.742 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.596	81394	0.561 ug/ml
13) N-TRIACONTANE	17.479	241988	1.691 ug/ml
14) N-DOTRIACONTANE	18.310	475729	3.496 ug/ml
15) N-TETRATRIACONTANE	19.144	460835	3.880 ug/ml
16) N-HEXATRIACONTANE	19.868	812955	7.885 ug/ml
18) N-TETRACONTANE	21.378	152736	1.681 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
Data File : FF009856.D
Signal(s) : FID2B.ch
Acq On : 04 Feb 2022 00:40
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 04 01:48:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

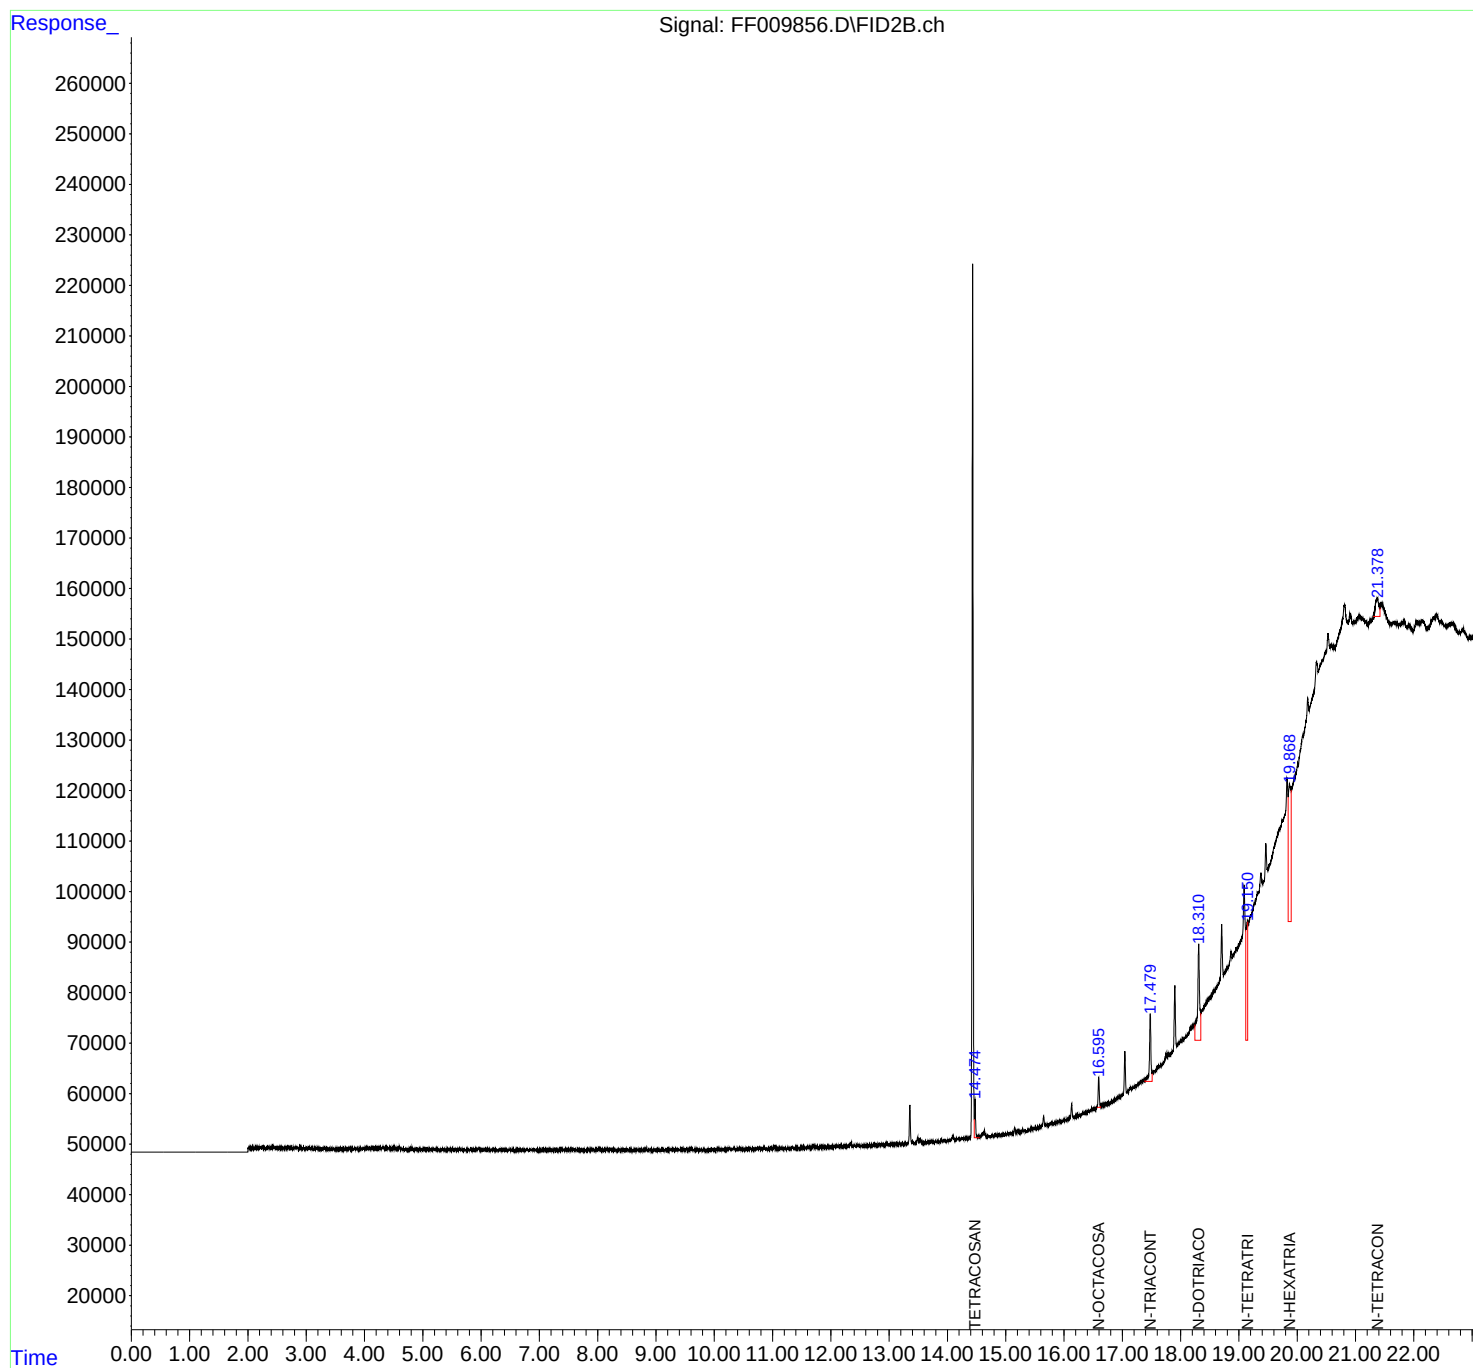


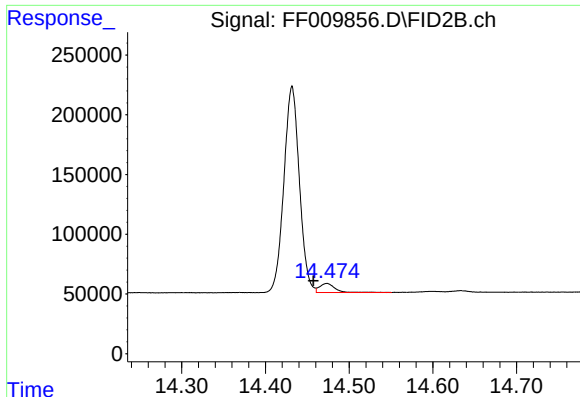

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.474 min
Delta R.T.: 0.017 min
Response: 96993
Conc: 0.74 ug/ml

Instrument :
FID_F
ClientSampleId :

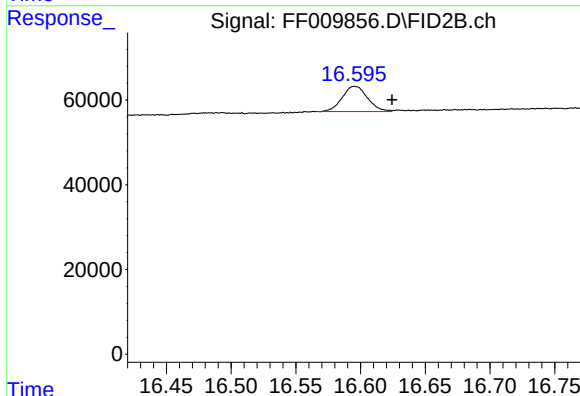


#12 N-OCTACOSANE

R.T.: 16.596 min
Delta R.T.: -0.029 min
Response: 81394
Conc: 0.56 ug/ml

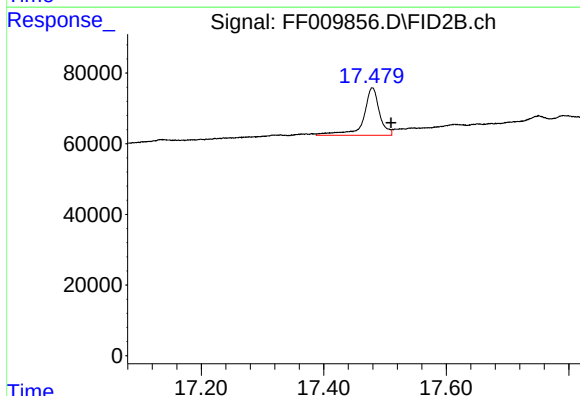


#13 N-TRIACONTANE

R.T.: 17.479 min
Delta R.T.: -0.031 min
Response: 241988
Conc: 1.69 ug/ml

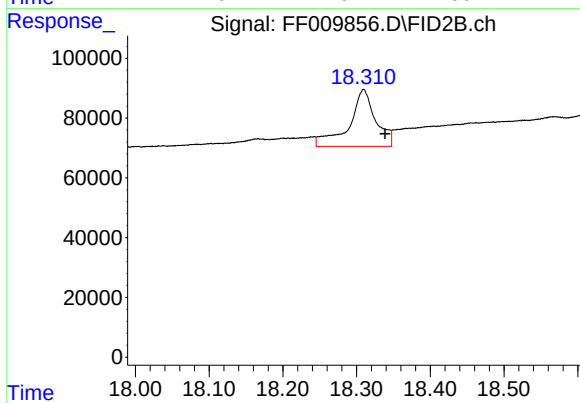

#14 N-DOTRIACONTANE


R.T.: 18.310 min
Delta R.T.: -0.029 min
Response: 475729
Conc: 3.50 ug/ml

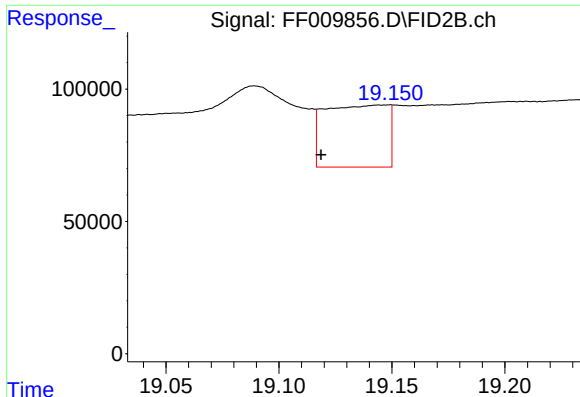

#15 N-TETRATRIACONTANE


R.T.: 19.144 min
Delta R.T.: 0.026 min
Response: 460835
Conc: 3.88 ug/ml

Instrument :
FID_F
ClientSampleId :

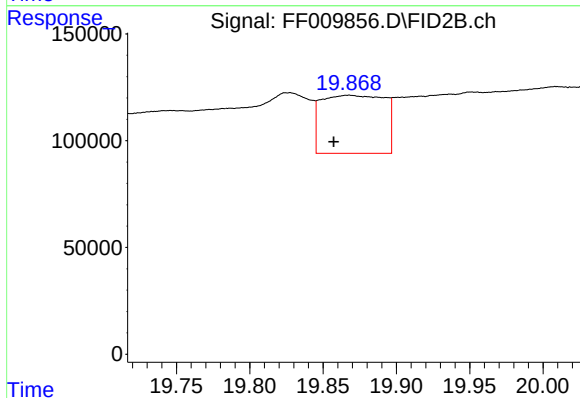

#16 N-HEXATRIACONTANE

R.T.: 19.868 min
Delta R.T.: 0.011 min
Response: 812955
Conc: 7.88 ug/ml

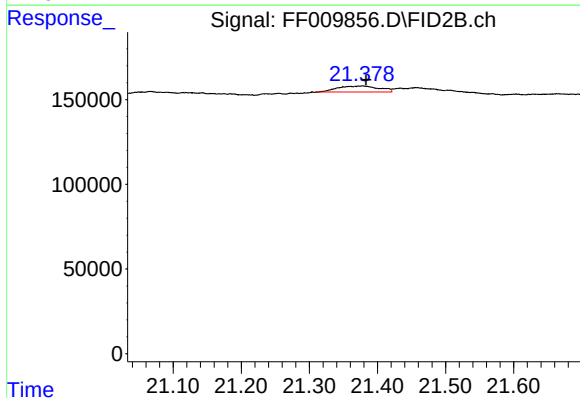

#18 N-TETRACONTANE

R.T.: 21.378 min
Delta R.T.: -0.005 min
Response: 152736
Conc: 1.68 ug/ml