

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
Data File : FF009840.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2022 16:48
Operator : AJ\MA
Sample : N1381-04
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
DB-06(38-40)-02-01-22

Integration File: calibration.e
Quant Time: Feb 03 22:36:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.434	1443520	11.046 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
Data File : FF009840.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2022 16:48
Operator : AJ\MA
Sample : N1381-04
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
DB-06(38-40)-02-01-22

Integration File: calibration.e
Quant Time: Feb 03 22:36:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

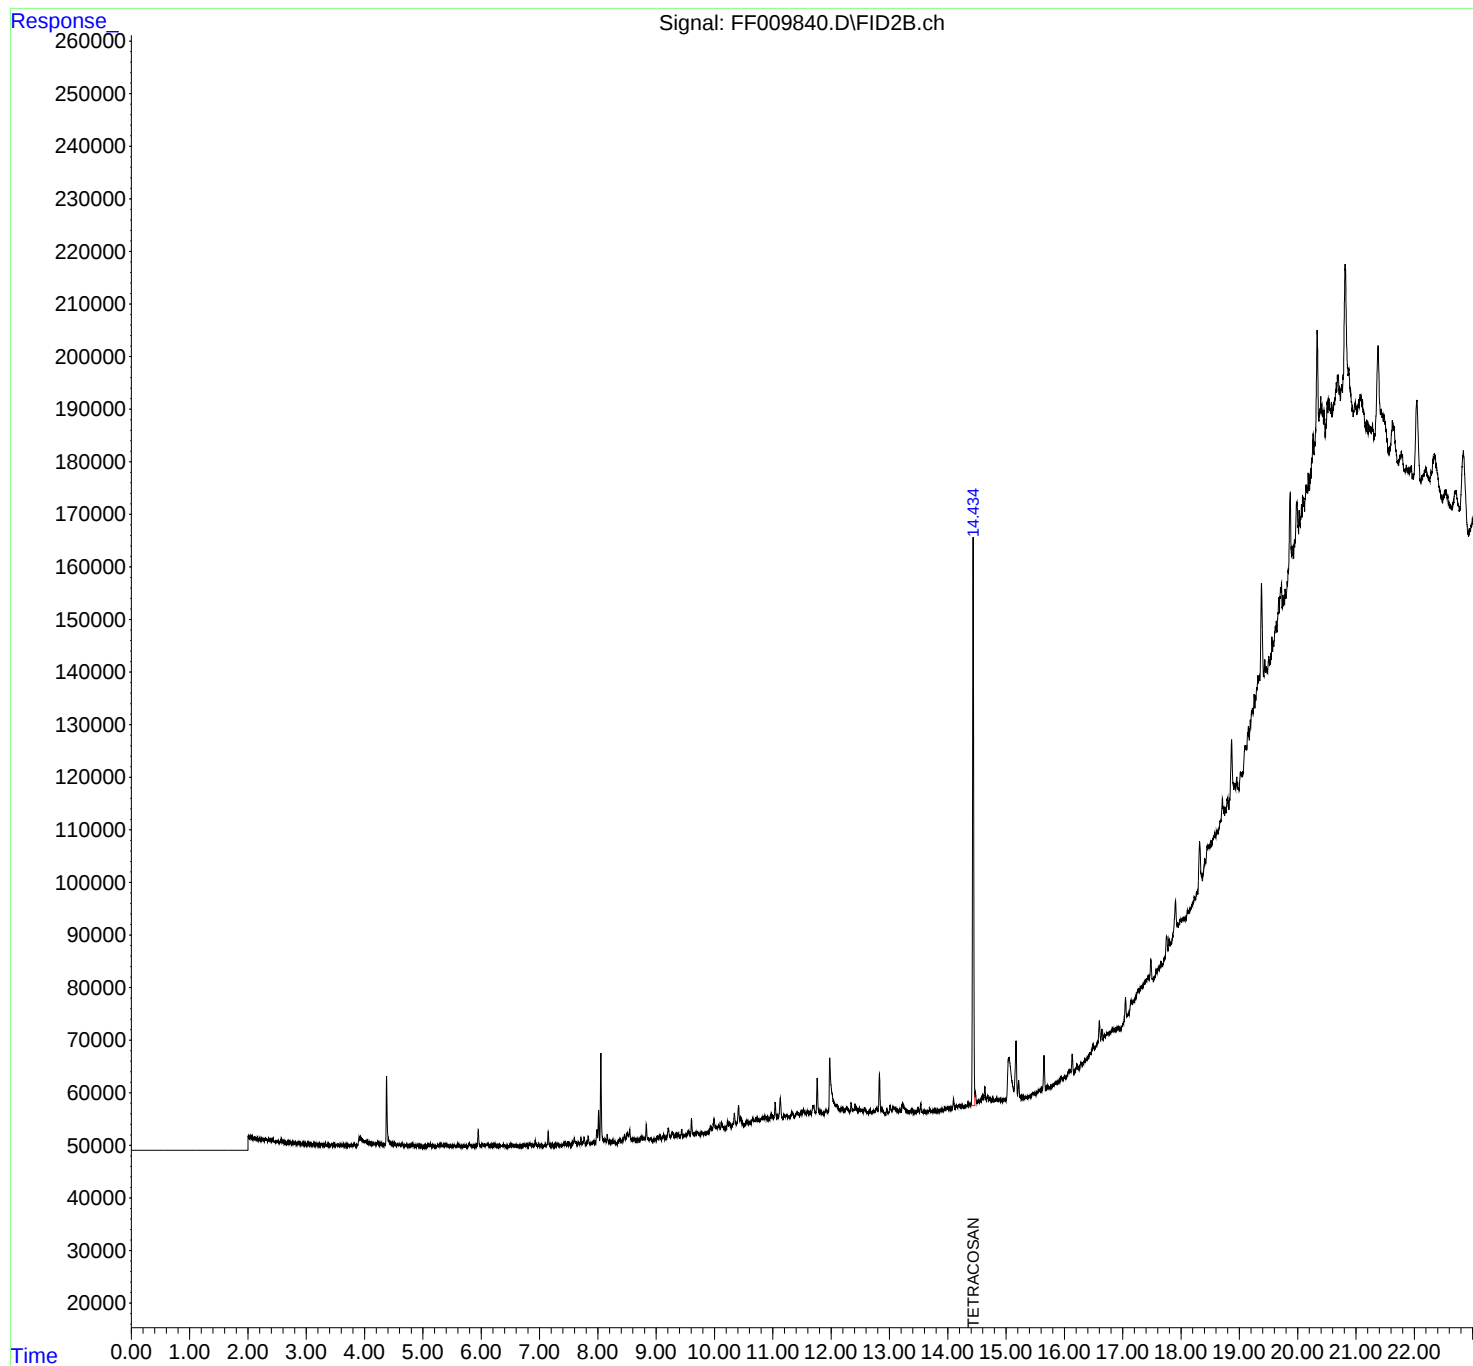

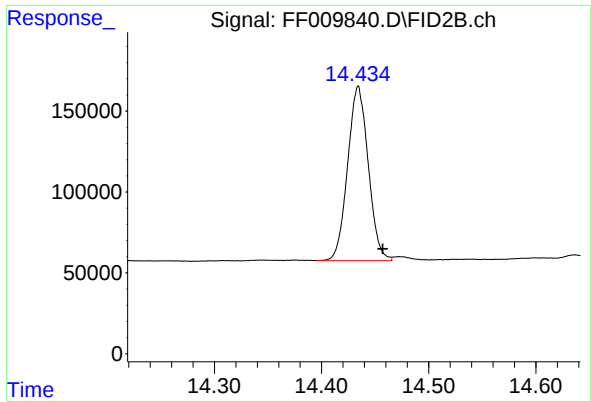

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.434 min
Delta R.T.: -0.023 min
Response: 1443520
Conc: 11.05 ug/ml

Instrument :
FID_F
ClientSampleId :
DB-06(38-40)-02-01-22