

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
 Data File : FF009843.D
 Signal(s) : FID2B.ch
 Acq On : 03 Feb 2022 18:17
 Operator : AJ\MA
 Sample : N1381-07
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 DB-07(13.5-15)-02-02-22

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/04/2022
 Supervised By :Ankita Jodhani 02/04/2022

Integration File: calibration.e
 Quant Time: Feb 03 22:37:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.449	2161887	16.544 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
Data File : FF009843.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2022 18:17
Operator : AJ\MA
Sample : N1381-07
Misc :
ALS Vial : 64 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
DB-07(13.5-15)-02-02-22


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/04/2022
Supervised By :Ankita Jodhani 02/04/2022

Integration File: calibration.e
Quant Time: Feb 03 22:37:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

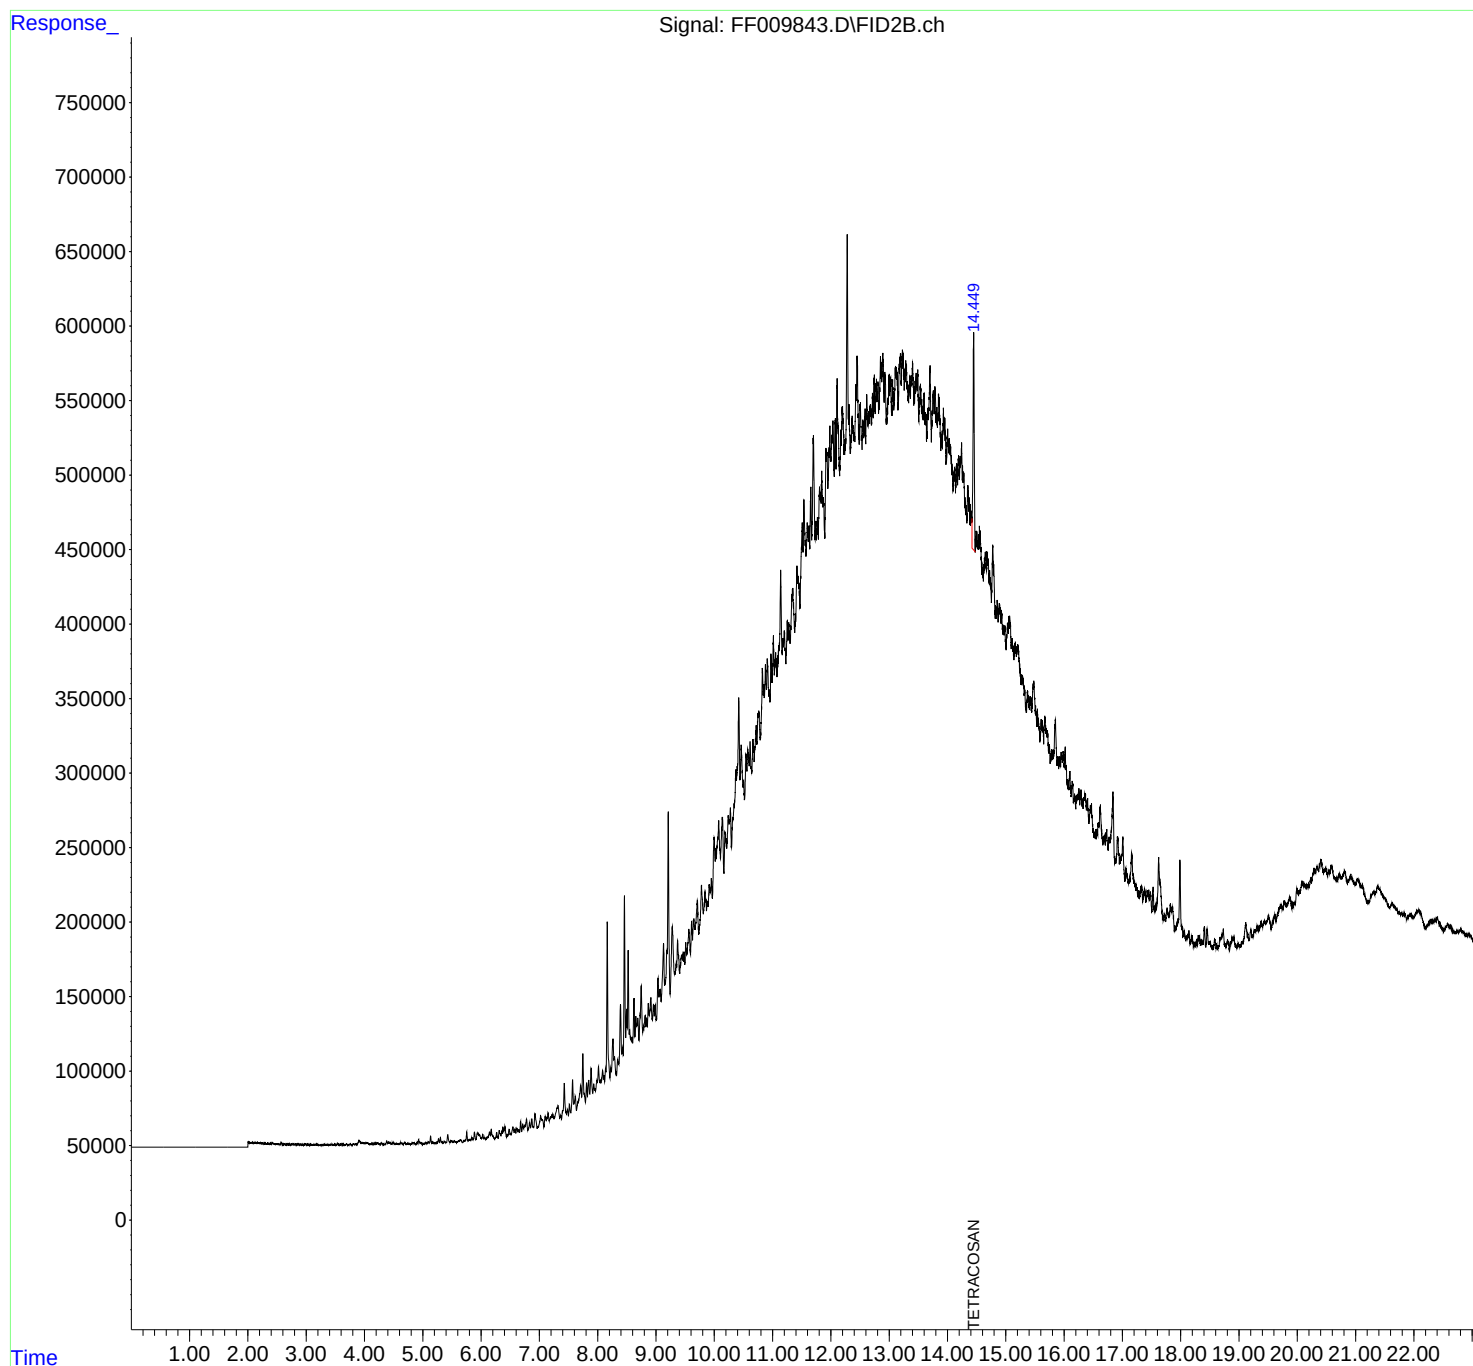

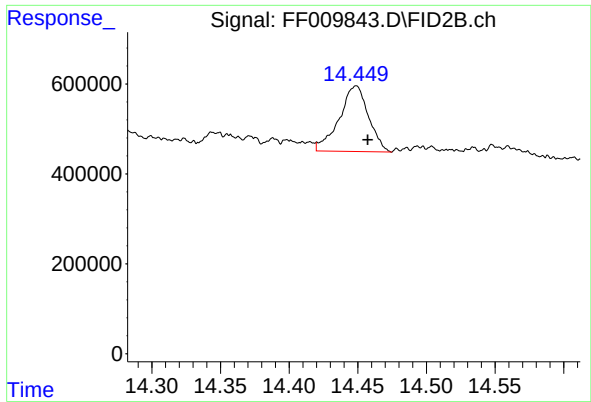

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.449 min
Delta R.T.: -0.008 min
Response: 2161887
Conc: 16.54 ug/ml

Instrument :

FID_F

ClientSampleId :

DB-07(13.5-15)-02-02-22

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 02/04/2022
Supervised By :Ankita Jodhani 02/04/2022