

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
Data File : FF009846.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2022 19:45
Operator : AJ\MA
Sample : N1381-08
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
DB-07(20-22)-02-02-22

Integration File: calibration.e
Quant Time: Feb 03 22:37:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.434	2341463	17.918 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020322\
Data File : FF009846.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2022 19:45
Operator : AJ\MA
Sample : N1381-08
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
DB-07(20-22)-02-02-22

Integration File: calibration.e
Quant Time: Feb 03 22:37:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

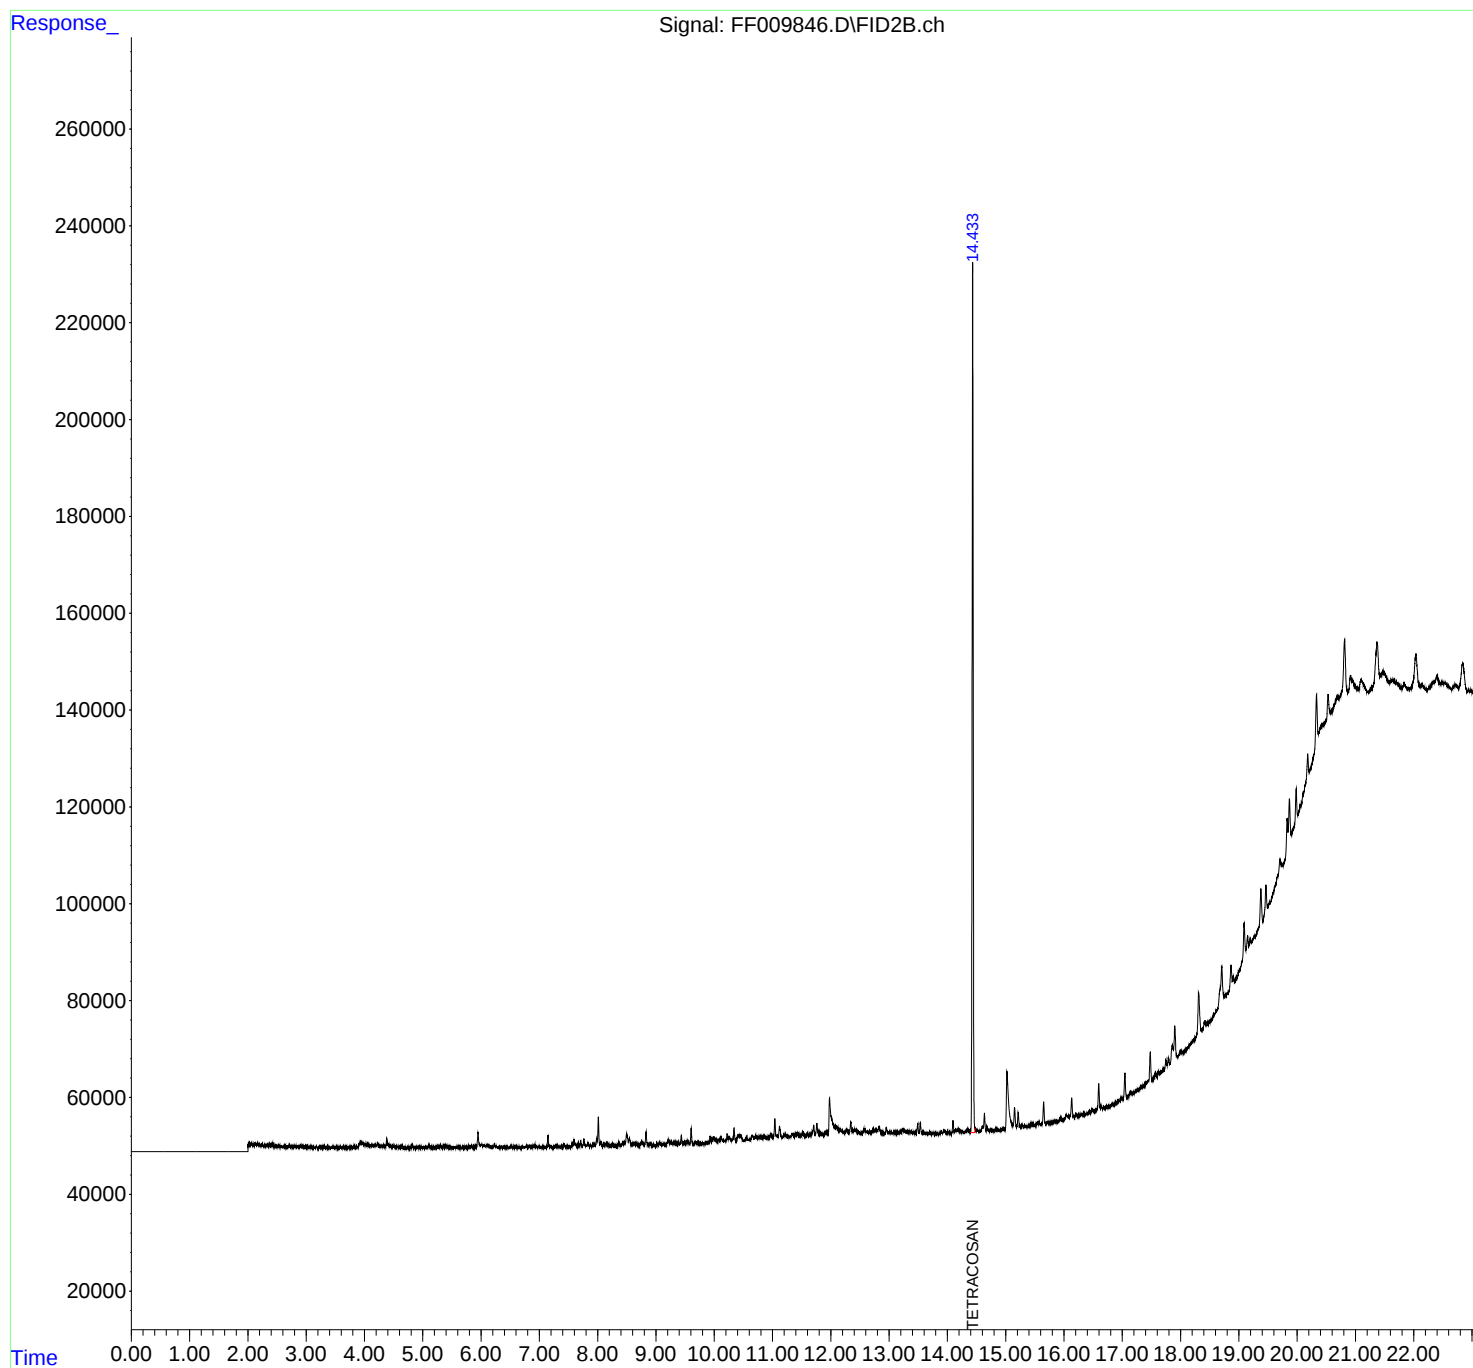

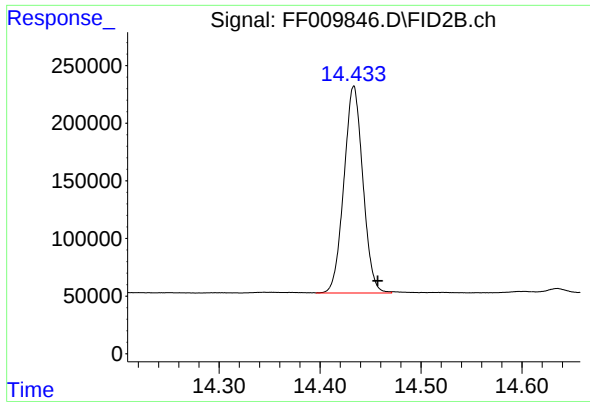

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.434 min
Delta R.T.: -0.023 min
Response: 2341463
Conc: 17.92 ug/ml

Instrument :
FID_F
ClientSampleId :
DB-07(20-22)-02-02-22