

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020323\
 Data File : FF011978.D
 Signal(s) : FID2B.ch
 Acq On : 03 Feb 2023 08:37
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 03 10:45:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
 Quant Title :
 QLast Update : Fri Jan 27 14:21:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.051	5741840	49.828 ug/ml
Target Compounds			
1) N-OCTANE	2.080	5794409	50.368 ug/ml
2) N-DECANE	4.604	6374500	54.066 ug/ml
3) N-DODECANE	6.768	6573121	54.872 ug/ml
4) N-TETRADECANE	8.595	6635762	55.103 ug/ml
5) N-HEXADECANE	10.201	6814477	54.631 ug/ml
6) N-OCTADECANE	11.643	6850873	53.879 ug/ml
7) N-EICOSANE	12.954	6793928	52.642 ug/ml
8) N-DOCOSANE	14.152	6516502	51.121 ug/ml
10) N-TETRACOSANE	15.255	6434753	49.450 ug/ml
11) N-HEXACOSANE	16.275	6249268	48.018 ug/ml
12) N-OCTACOSANE	17.225	6105076	46.949 ug/ml
13) N-TRIACONTANE	18.114	5961032	46.189 ug/ml
14) N-DOTRIACONTANE	18.946	5713298	43.899 ug/ml
15) N-TETRATRIACONTANE	19.728	5438401	48.848 ug/ml
16) N-HEXATRIACONTANE	20.468	5172049	50.350 ug/ml
17) N-OCTATRIACONTANE	21.210	6333214	64.293 ug/ml
18) N-TETRACONTANE	22.133	5650374	54.521 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020323\
Data File : FF011978.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2023 08:37
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 03 10:45:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

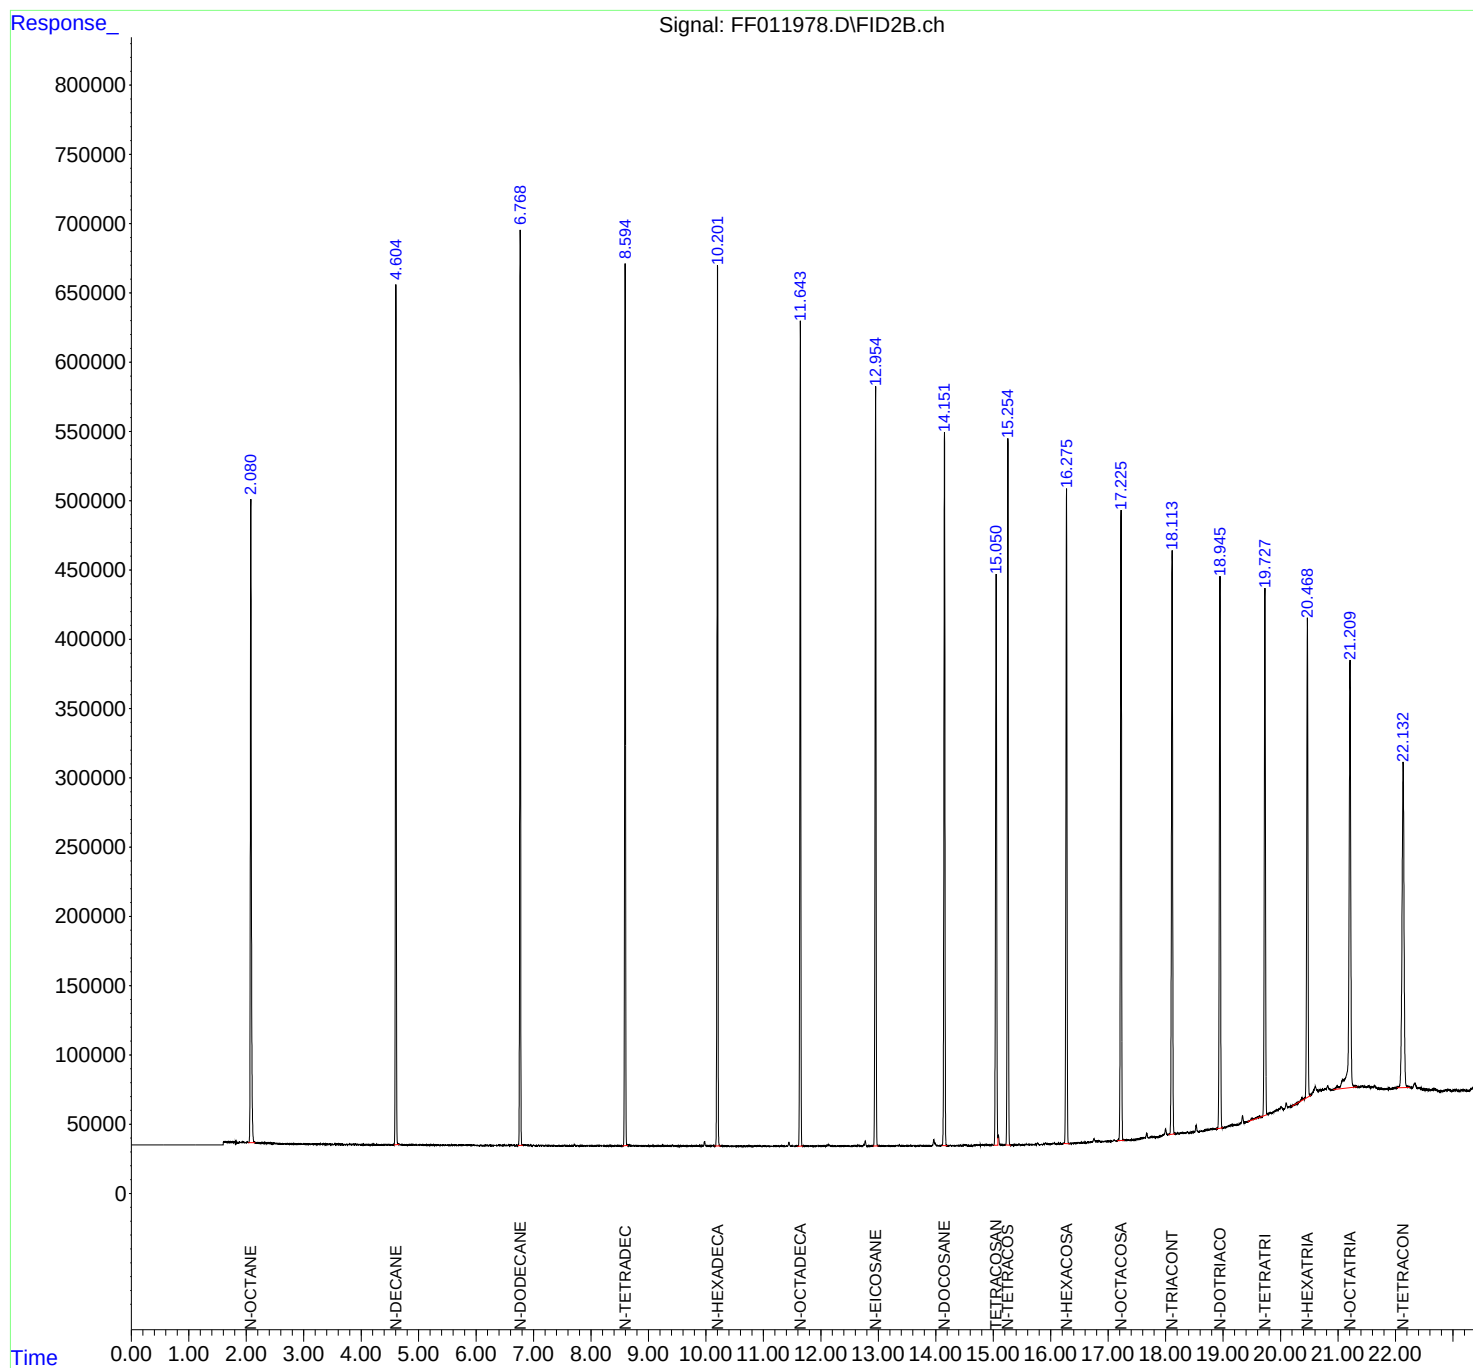


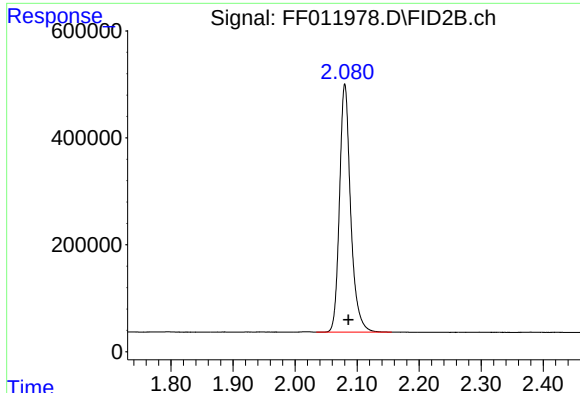

#1 N-OCTANE


R.T.: 2.080 min
Delta R.T.: -0.006 min
Response: 5794409
Conc: 50.37 ug/ml

Instrument :
FID_F
ClientSampleId :

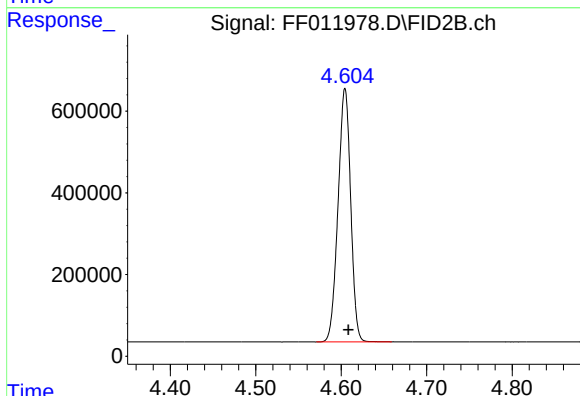


#2 N-DECANE

R.T.: 4.604 min
Delta R.T.: -0.004 min
Response: 6374500
Conc: 54.07 ug/ml

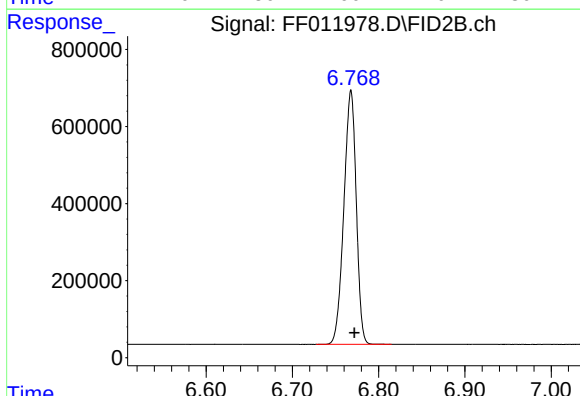


#3 N-DODECANE

R.T.: 6.768 min
Delta R.T.: -0.004 min
Response: 6573121
Conc: 54.87 ug/ml

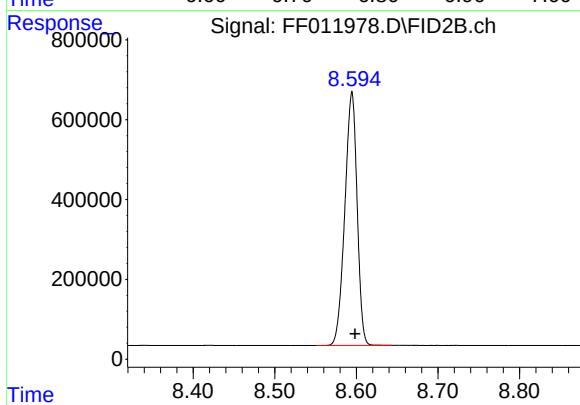

#4 N-TETRADECANE


R.T.: 8.595 min
Delta R.T.: -0.004 min
Response: 6635762
Conc: 55.10 ug/ml

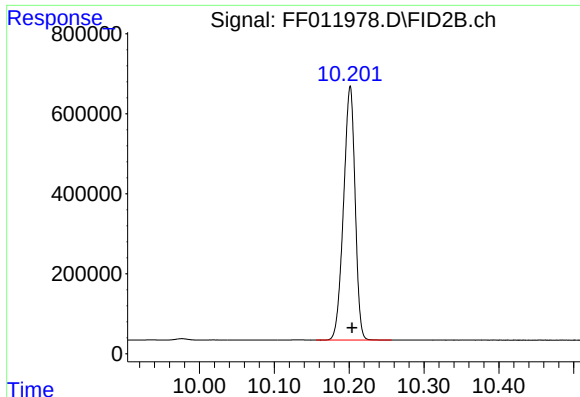

#5 N-HEXADECANE


R.T.: 10.201 min
Delta R.T.: -0.002 min
Response: 6814477
Conc: 54.63 ug/ml

Instrument :
FID_F
ClientSampleId :

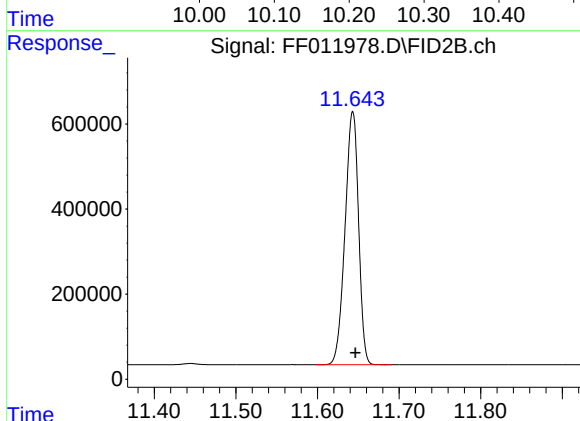


#6 N-OCTADECANE

R.T.: 11.643 min
Delta R.T.: -0.003 min
Response: 6850873
Conc: 53.88 ug/ml

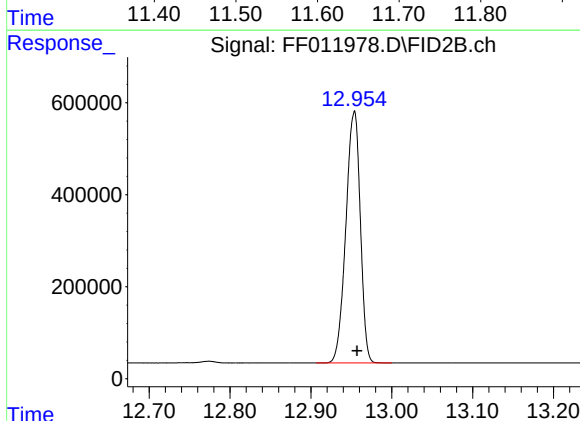


#7 N-EICOSANE

R.T.: 12.954 min
Delta R.T.: -0.003 min
Response: 6793928
Conc: 52.64 ug/ml

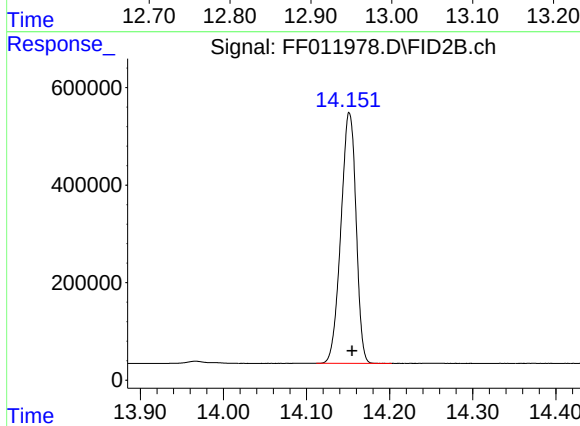

#8 N-DOCOSANE


R.T.: 14.152 min
Delta R.T.: -0.003 min
Response: 6516502
Conc: 51.12 ug/ml

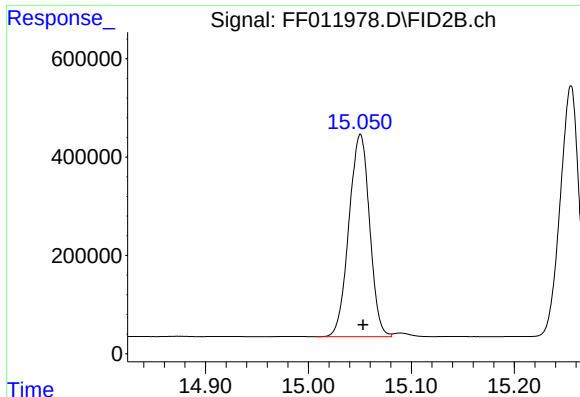

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.051 min
Delta R.T.: -0.002 min
Response: 5741840
Conc: 49.83 ug/ml

Instrument :
FID_F
ClientSampleId :

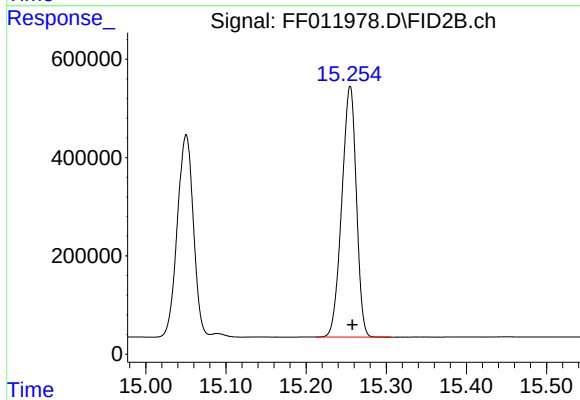


#10 N-TETRACOSANE

R.T.: 15.255 min
Delta R.T.: -0.003 min
Response: 6434753
Conc: 49.45 ug/ml

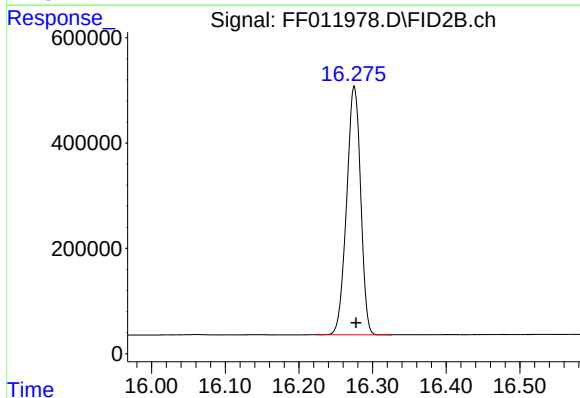


#11 N-HEXACOSANE

R.T.: 16.275 min
Delta R.T.: -0.003 min
Response: 6249268
Conc: 48.02 ug/ml

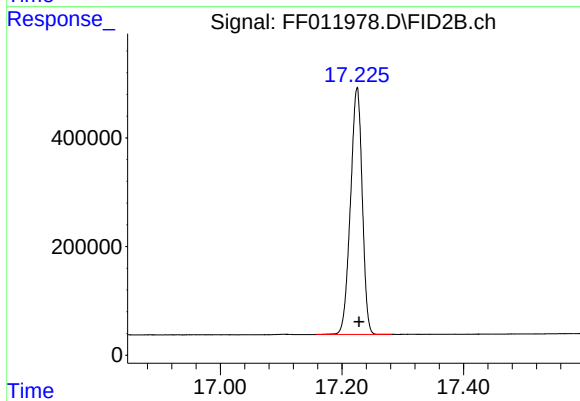

#12 N-OCTACOSANE


R.T.: 17.225 min
Delta R.T.: -0.003 min
Response: 6105076
Conc: 46.95 ug/ml

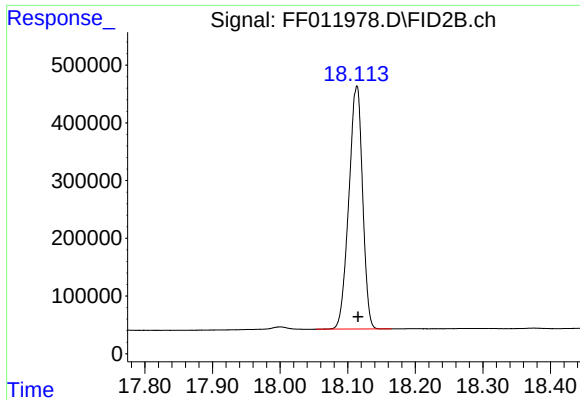

#13 N-TRIACONTANE


R.T.: 18.114 min
Delta R.T.: -0.002 min
Response: 5961032
Conc: 46.19 ug/ml

Instrument :
FID_F
ClientSampleId :

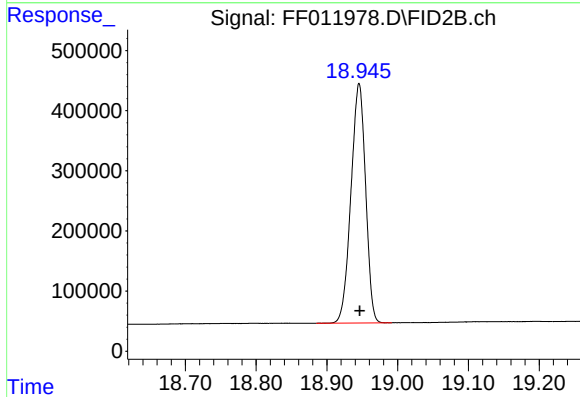


#14 N-DOTRIACONTANE

R.T.: 18.946 min
Delta R.T.: 0.000 min
Response: 5713298
Conc: 43.90 ug/ml

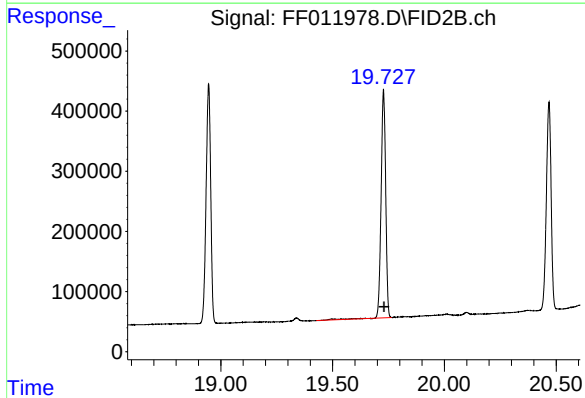


#15 N-TETRATRIACONTANE

R.T.: 19.728 min
Delta R.T.: -0.002 min
Response: 5438401
Conc: 48.85 ug/ml

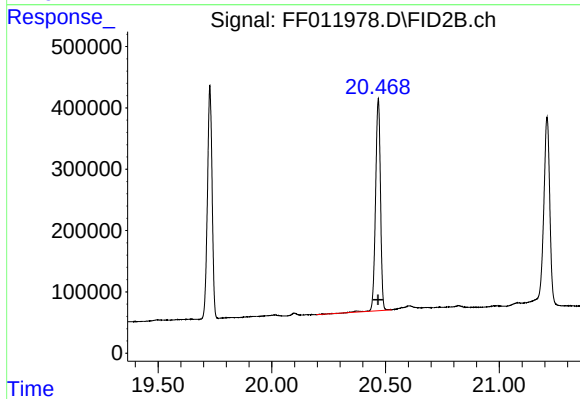

#16 N-HEXATRIACONTANE


R.T.: 20.468 min
Delta R.T.: 0.000 min
Response: 5172049
Conc: 50.35 ug/ml

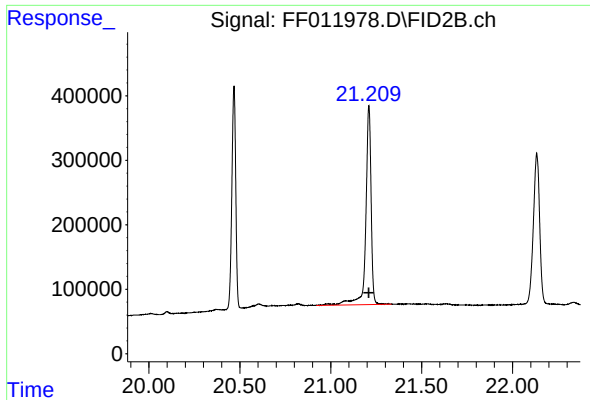

#17 N-OCTATRIACONTANE

R.T.: 21.210 min
Delta R.T.: 0.000 min
Response: 6333214
Conc: 64.29 ug/ml

Instrument :
FID_F
ClientSampleId :

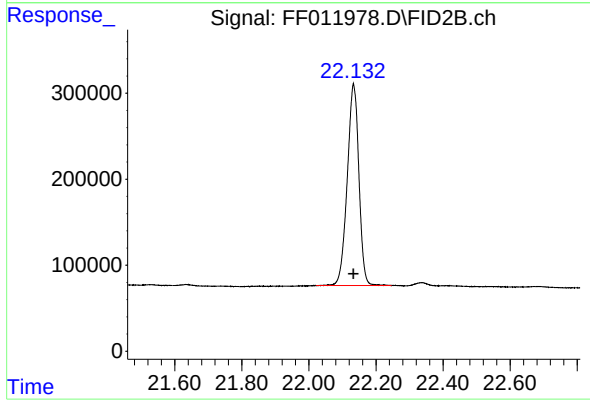

#18 N-TETRACONTANE

R.T.: 22.133 min
Delta R.T.: 0.000 min
Response: 5650374
Conc: 54.52 ug/ml