

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020323\
Data File : FF011979.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2023 09:06
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 03 10:45:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.767	3098253	25.864 ug/ml
12)	N-OCTACOSANE	17.223	2961120	22.772 ug/ml
13)	N-TRIACONTANE	18.108	46581	0.361 ug/ml
14)	N-DOTRIACONTANE	18.941	89063	0.684 ug/ml
15)	N-TETRATRIACONTANE	19.722	64005	0.575 ug/ml
16)	N-HEXATRIACONTANE	20.463	64317	0.626 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020323\
Data File : FF011979.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2023 09:06
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 03 10:45:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

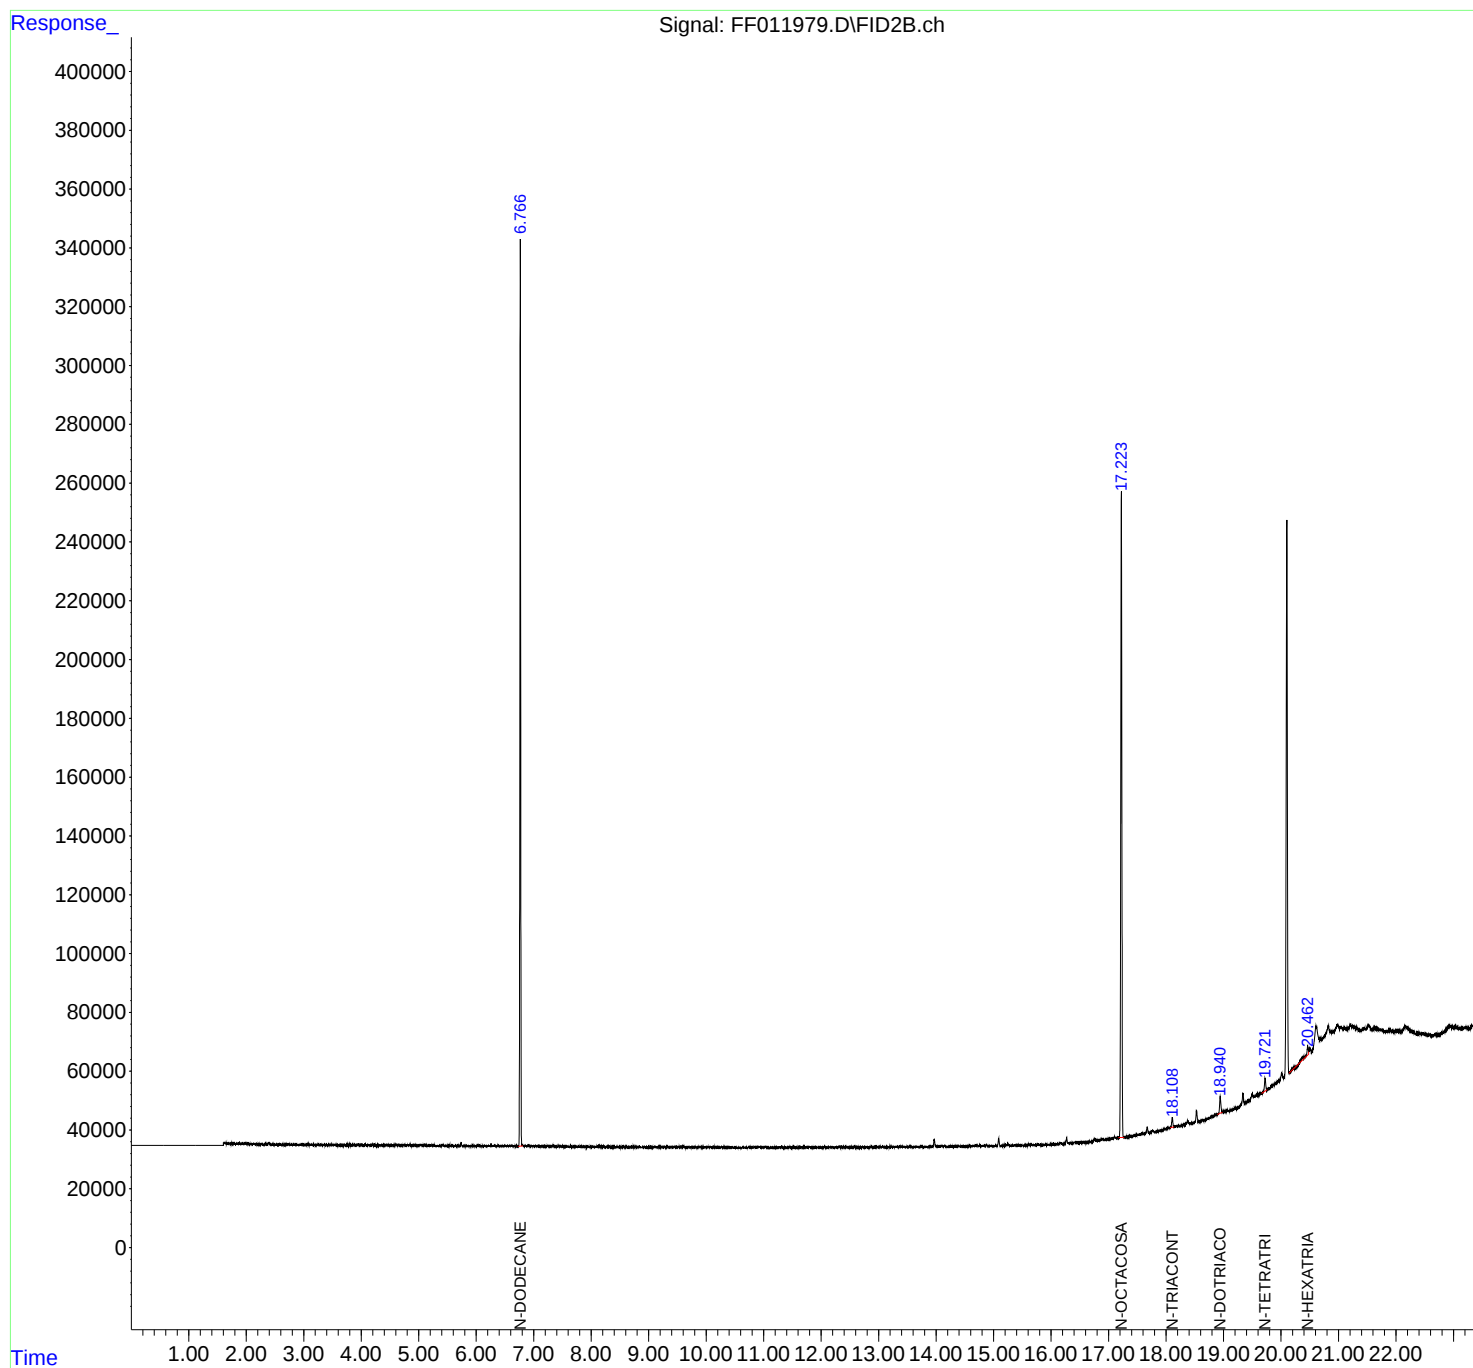


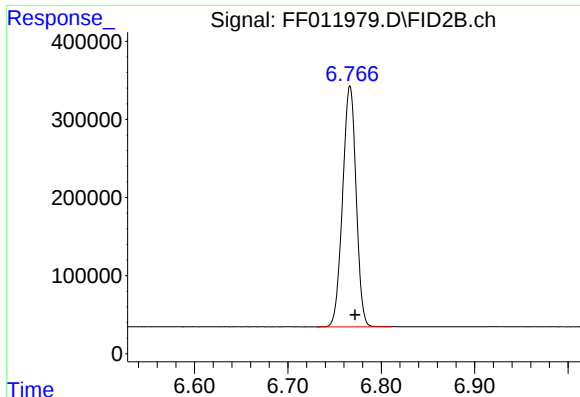

#3 N-DODECANE


R.T.: 6.767 min
Delta R.T.: -0.006 min
Response: 3098253
Conc: 25.86 ug/ml

Instrument :
FID_F
ClientSampleId :

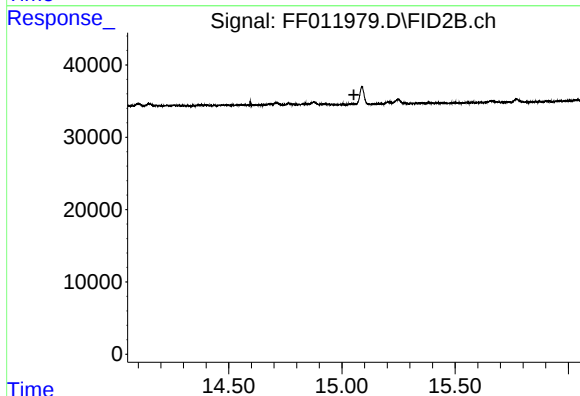


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.053 min
Response: 0
Conc: N.D.

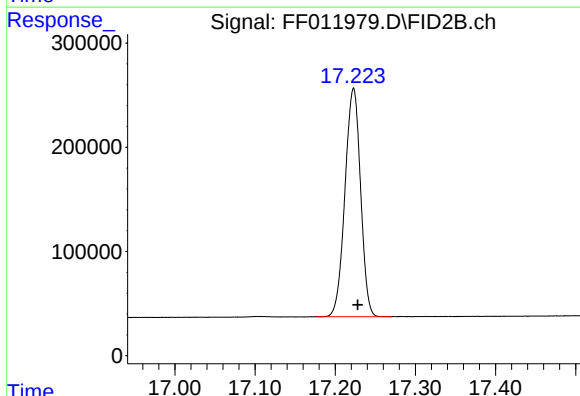


#12 N-OCTACOSANE

R.T.: 17.223 min
Delta R.T.: -0.005 min
Response: 2961120
Conc: 22.77 ug/ml

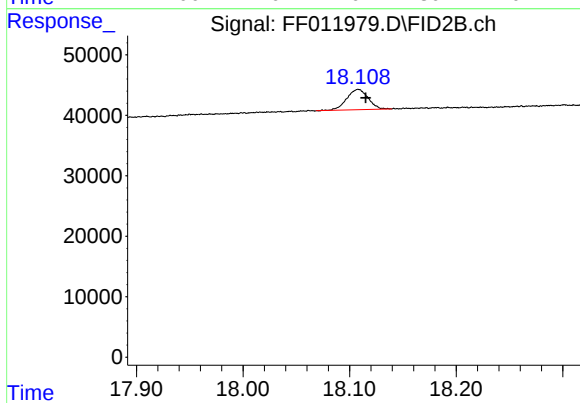

#13 N-TRIACONTANE


R.T.: 18.108 min
Delta R.T.: -0.007 min
Response: 46581
Conc: 0.36 ug/ml

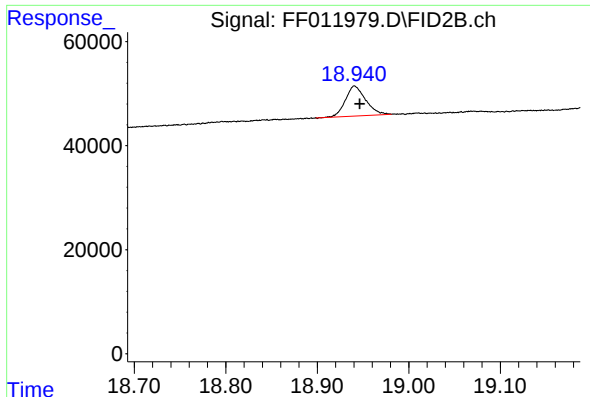

#14 N-DOTRIACONTANE


R.T.: 18.941 min
Delta R.T.: -0.006 min
Response: 89063
Conc: 0.68 ug/ml

Instrument :
FID_F
ClientSampleId :

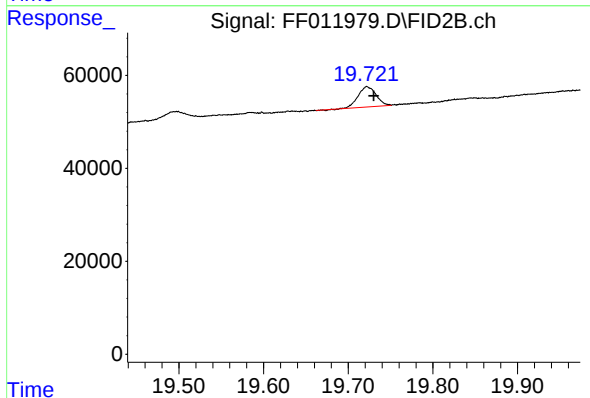

#15 N-TETRATRIACONTANE

R.T.: 19.722 min
Delta R.T.: -0.008 min
Response: 64005
Conc: 0.57 ug/ml

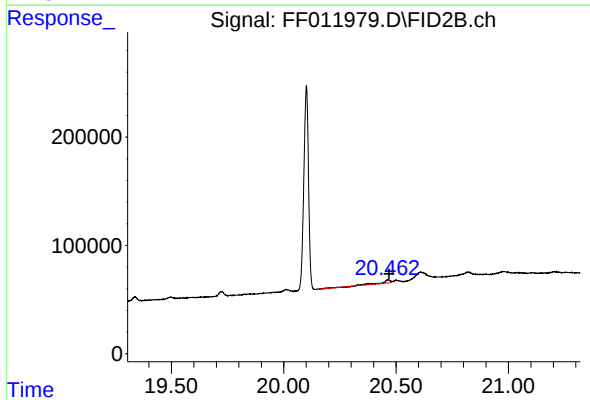

#16 N-HEXATRIACONTANE

R.T.: 20.463 min
Delta R.T.: -0.005 min
Response: 64317
Conc: 0.63 ug/ml