

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020323\
Data File : FF011979.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2023 09:06
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Feb 03 10:45:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.767	3098253	25.864 ug/ml
12)	N-OCTACOSANE	17.223	2961120	22.772 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020323\
Data File : FF011979.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2023 09:06
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Feb 03 10:45:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

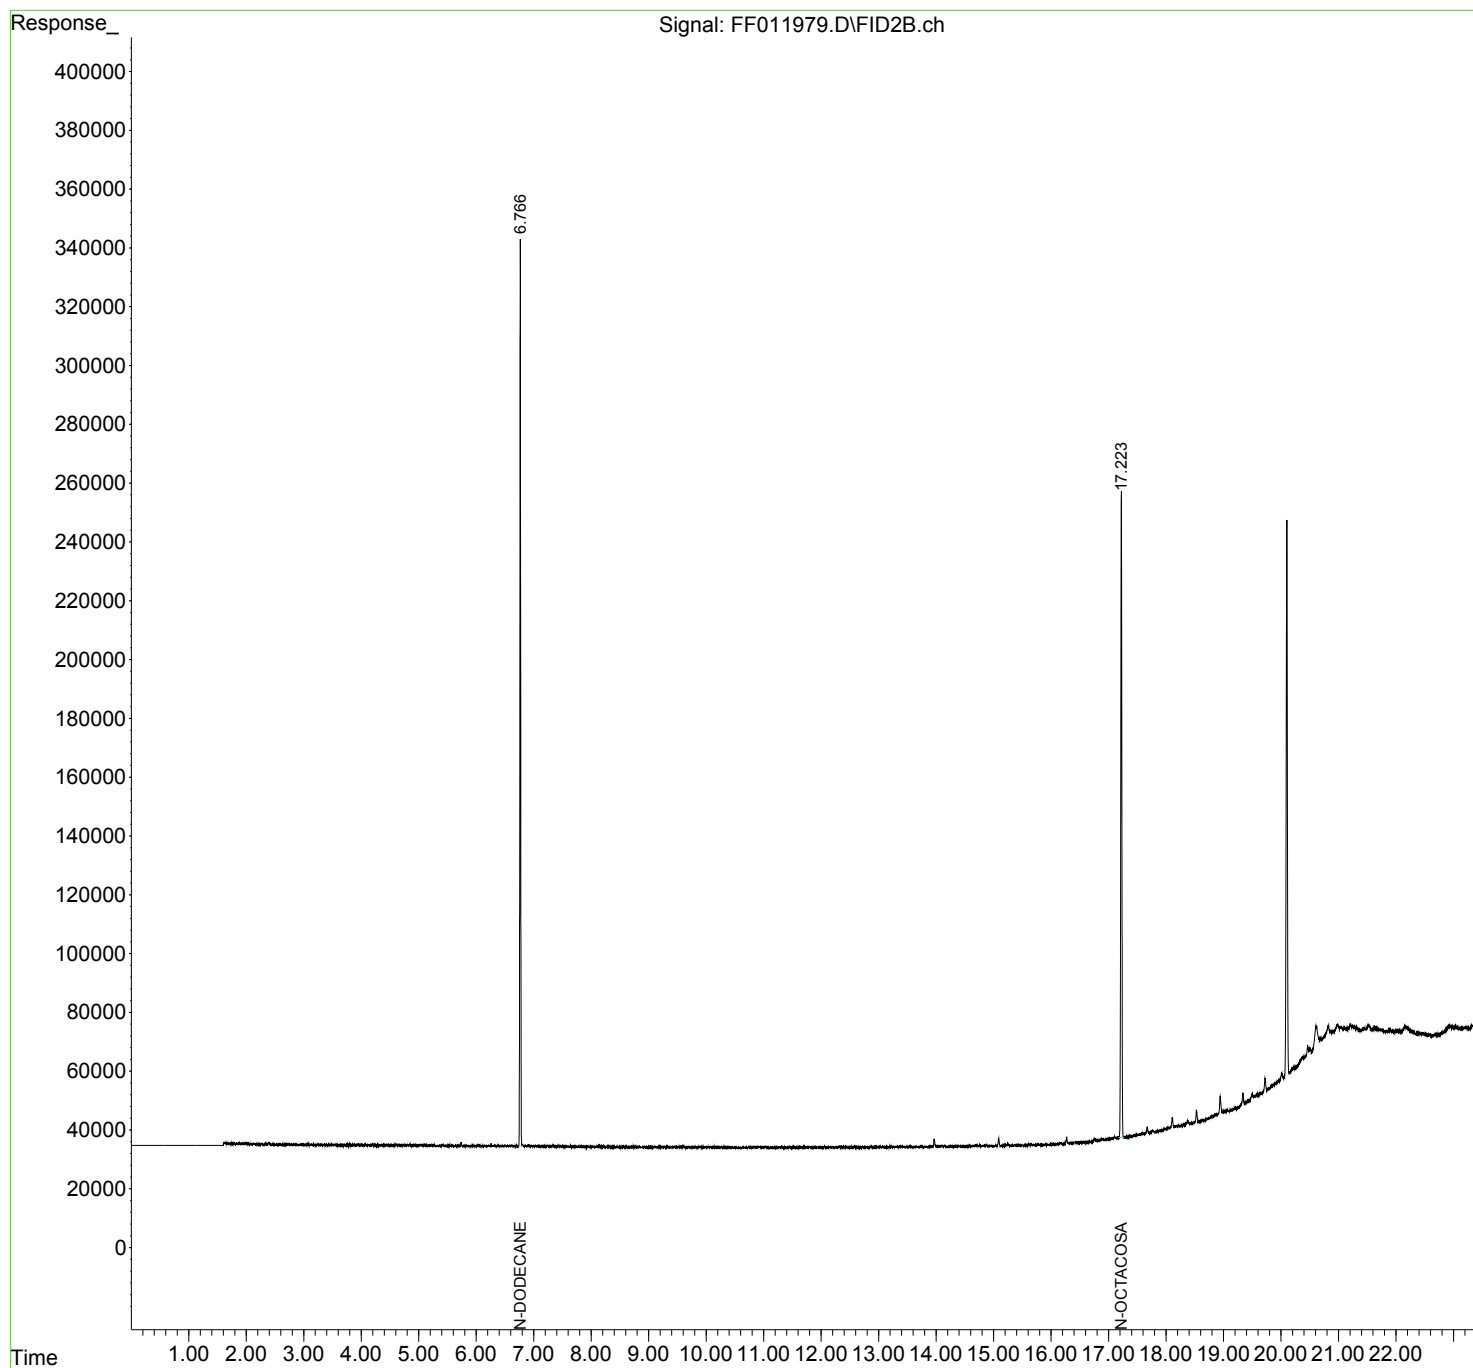


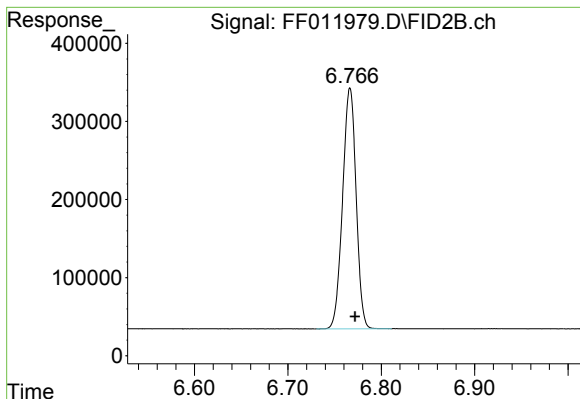

#3 N-DODECANE


R.T.: 6.767 min
Delta R.T.: -0.006 min
Response: 3098253
Conc: 25.86 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

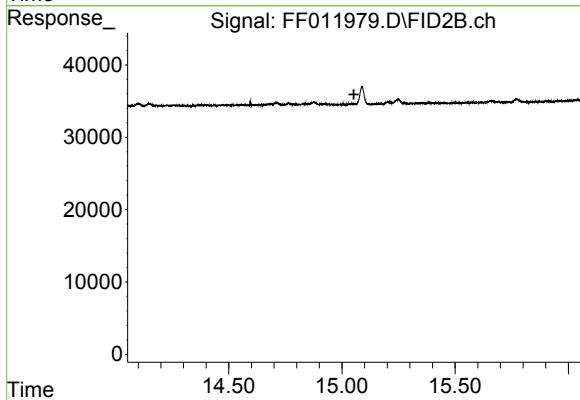

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.053 min
Response: 0
Conc: N.D.

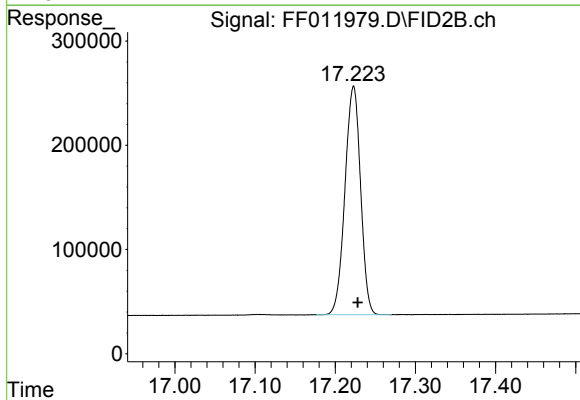

#12 N-OCTACOSANE

R.T.: 17.223 min
Delta R.T.: -0.005 min
Response: 2961120
Conc: 22.77 ug/ml