

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020323\
Data File : FF011984.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2023 16:23
Operator : YP\AJ
Sample : 01414-02
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SASP2-123-2(20-30)

Integration File: autoint1.e
Quant Time: Feb 03 23:50:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.046	3481463	30.213 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020323\
Data File : FF011984.D
Signal(s) : FID2B.ch
Acq On : 03 Feb 2023 16:23
Operator : YP\AJ
Sample : 01414-02
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SASP2-123-2(20-30)

Integration File: autoint1.e
Quant Time: Feb 03 23:50:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

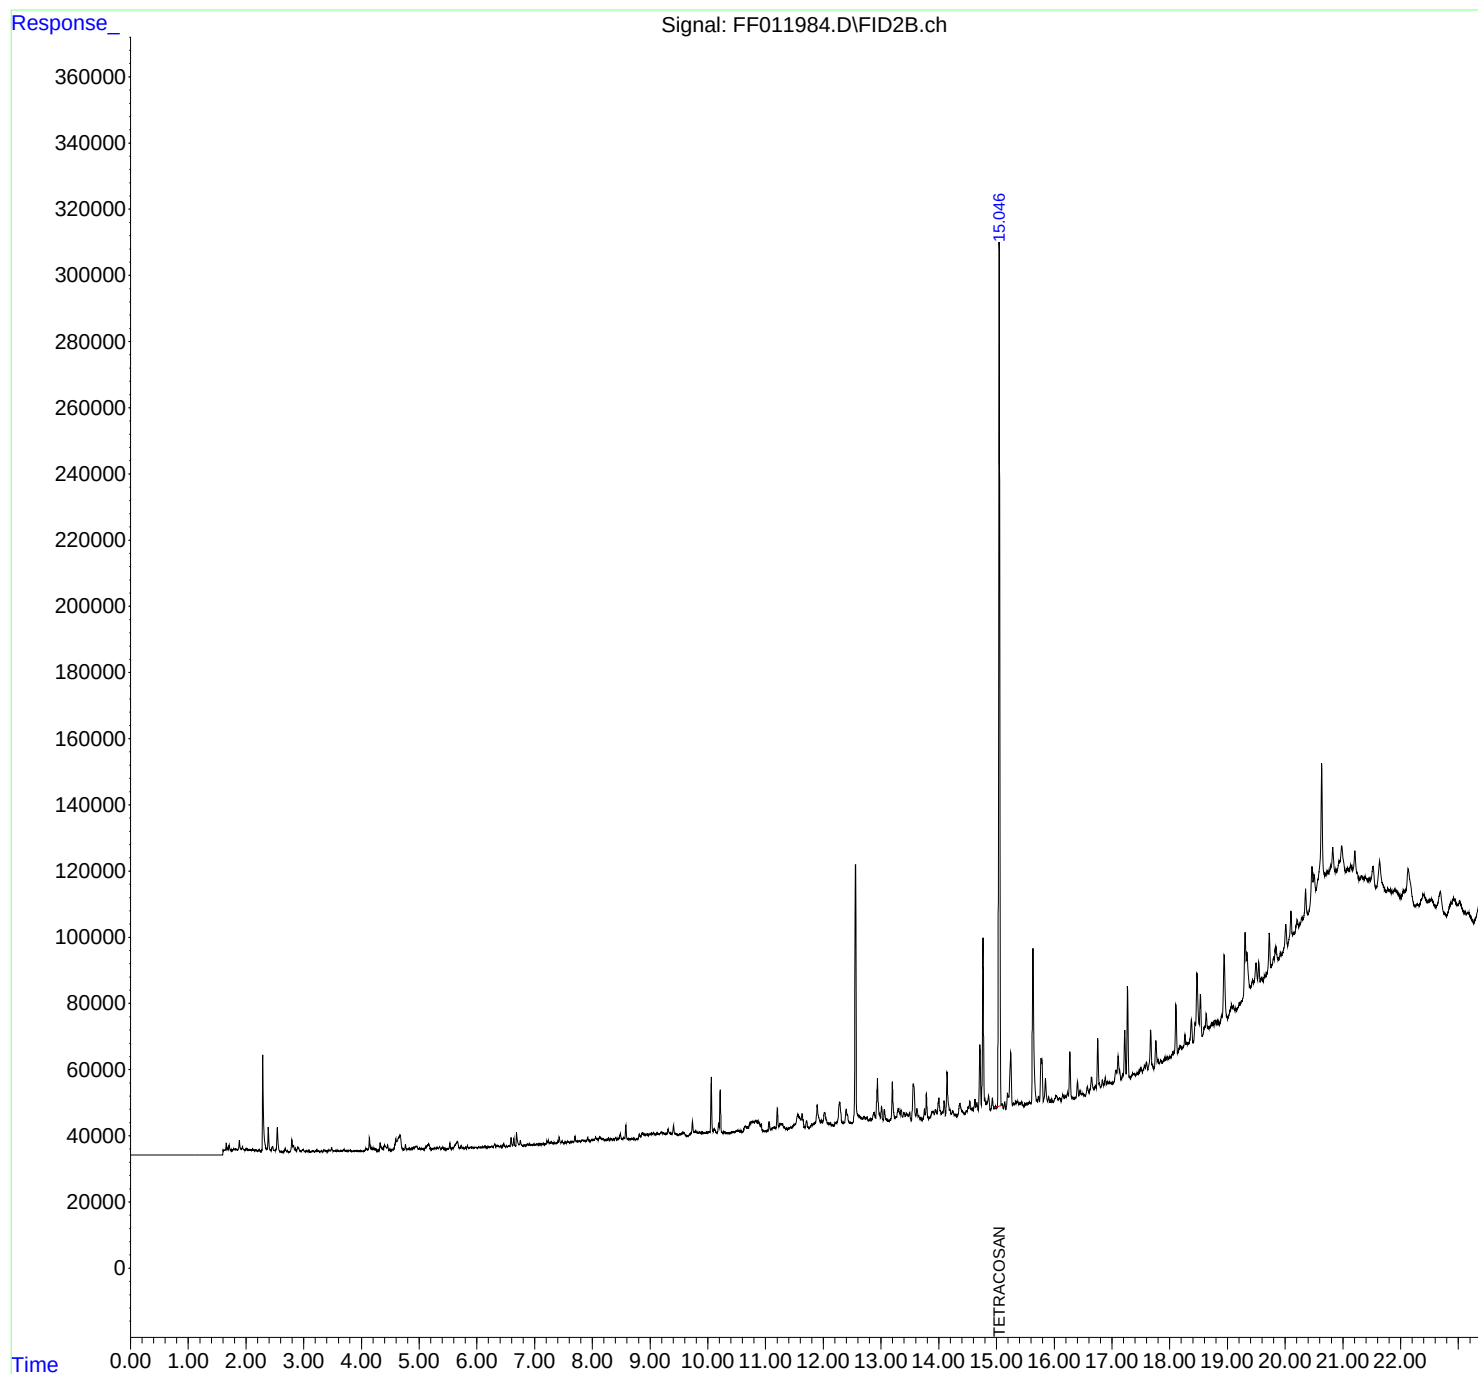

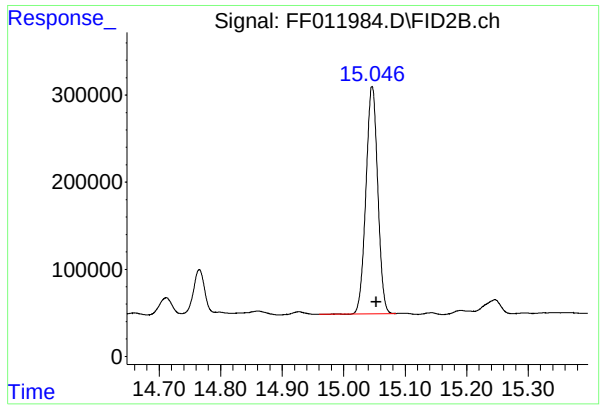

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.046 min
Delta R.T.: -0.007 min
Response: 3481463
Conc: 30.21 ug/ml

Instrument :
FID_F
ClientSampleId :
SASP2-123-2(20-30)