

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020419\
 Data File : FF003368.D
 Signal(s) : FID2B.ch
 Acq On : 04 Feb 2019 20:04
 Operator : AJ\SJ
 Sample : K1312-01MSD
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 05 00:01:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
 Quant Title :
 QLast Update : Fri Feb 01 22:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.617	2961240	24.528 ug/ml
Target Compounds			
2) N-DECANE	4.343	2891416	21.605 ug/ml
3) N-DODECANE	6.363	3070788	22.775 ug/ml
4) N-TETRADECANE	8.155	3207724	23.698 ug/ml
5) N-HEXADECANE	9.756	3318029	24.348 ug/ml
6) N-OCTADECANE	11.200	3344688	24.307 ug/ml
7) N-EICOSANE	12.512	3278286	23.839 ug/ml
8) N-DOCOSANE	13.714	3284323	24.005 ug/ml
10) N-TETRACOSANE	14.822	3369120	24.774 ug/ml
11) N-HEXACOSANE	15.846	3457941	25.494 ug/ml
12) N-OCTACOSANE	16.800	3787999	27.667 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020419\
Data File : FF003368.D
Signal(s) : FID2B.ch
Acq On : 04 Feb 2019 20:04
Operator : AJ\SJ
Sample : K1312-01MSD
Misc :
ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 05 00:01:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

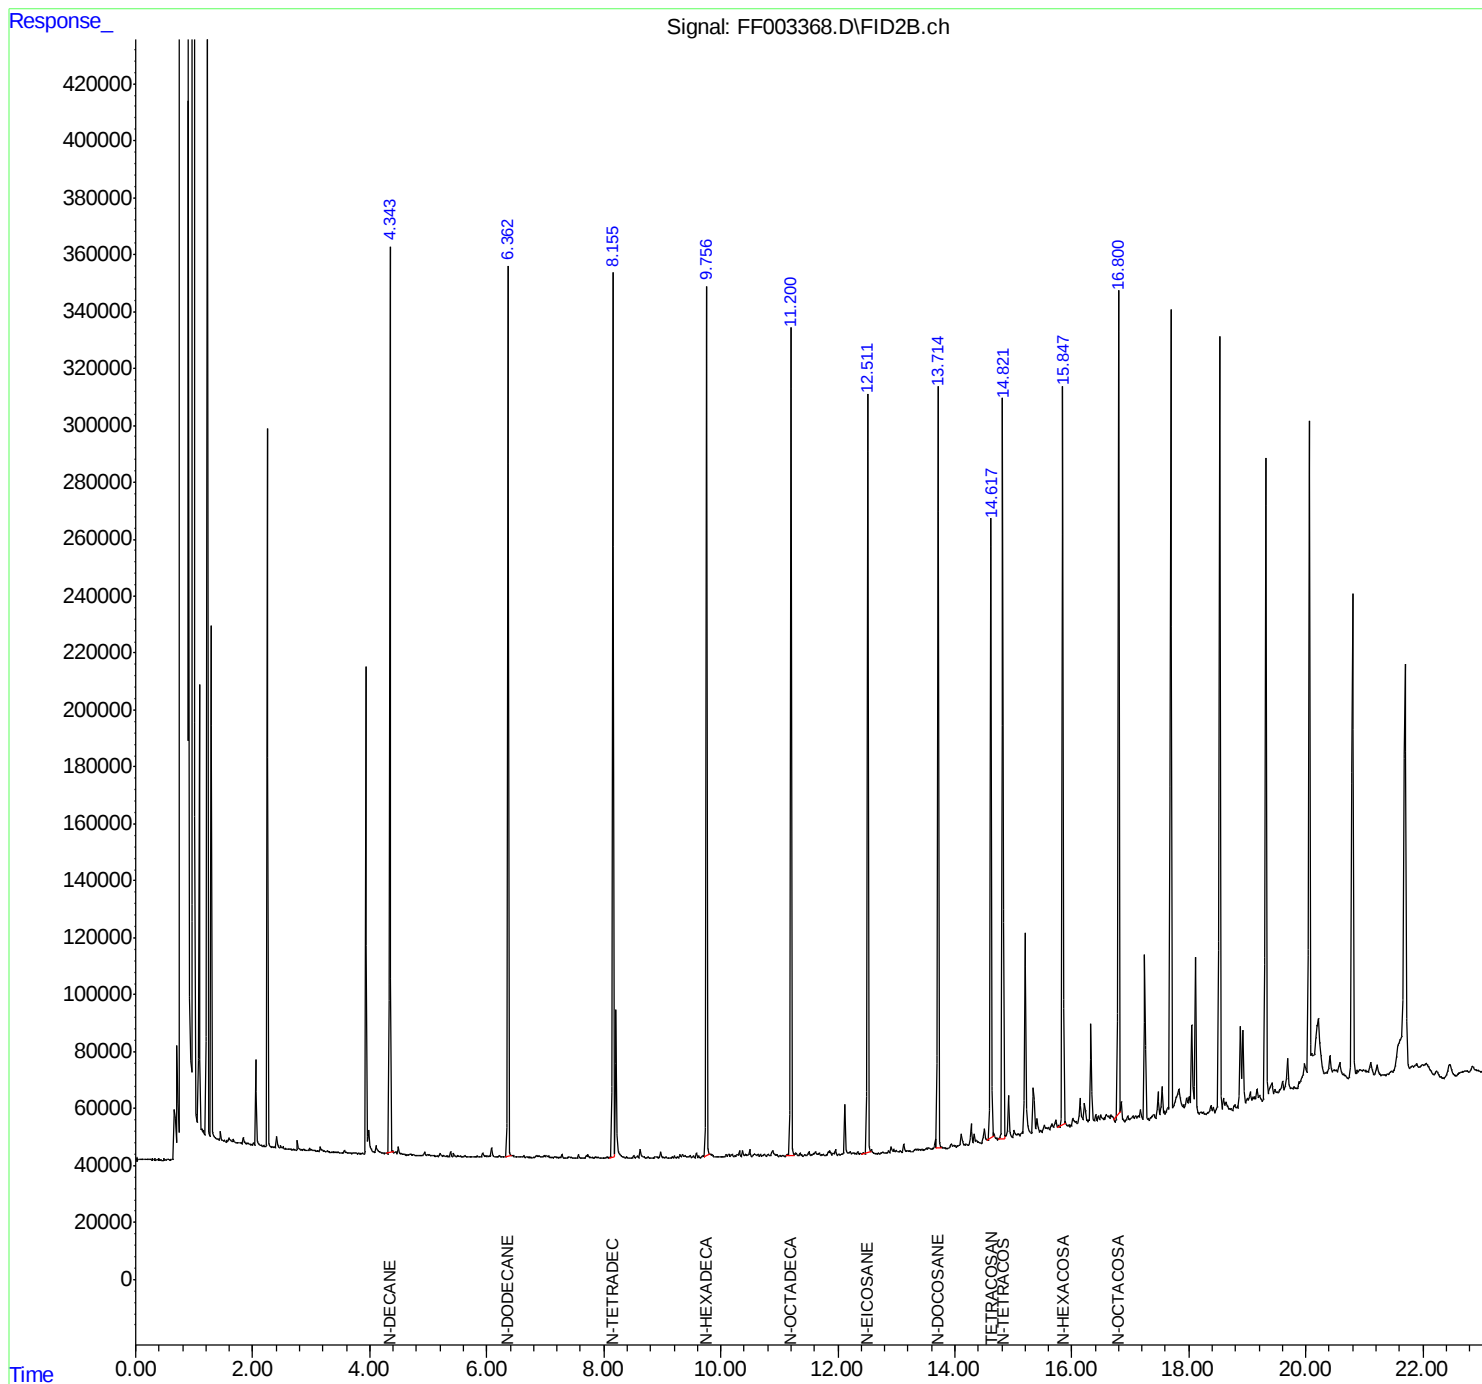

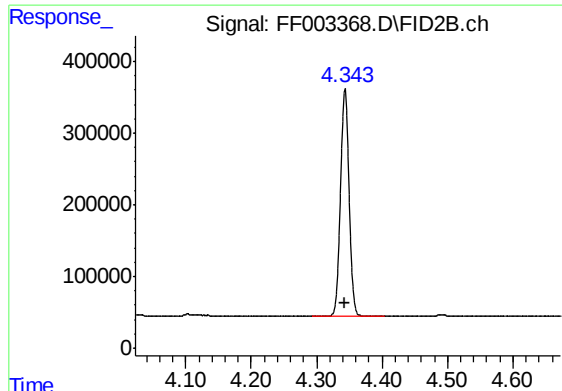


#2 N-DECANE

R.T.: 4.343 min
Delta R.T.: 0.001 min
Response: 2891416
Conc: 21.61 ug/ml

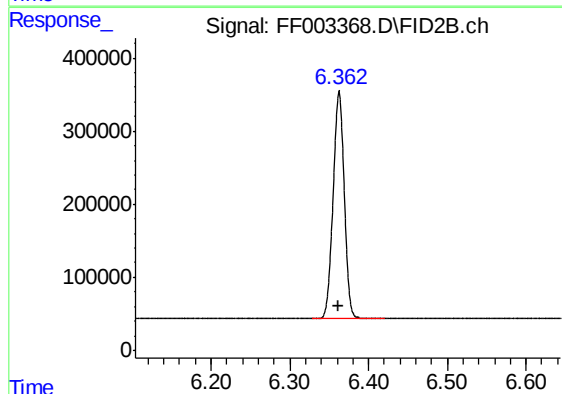


#3 N-DODECANE

R.T.: 6.363 min
Delta R.T.: 0.002 min
Response: 3070788
Conc: 22.78 ug/ml

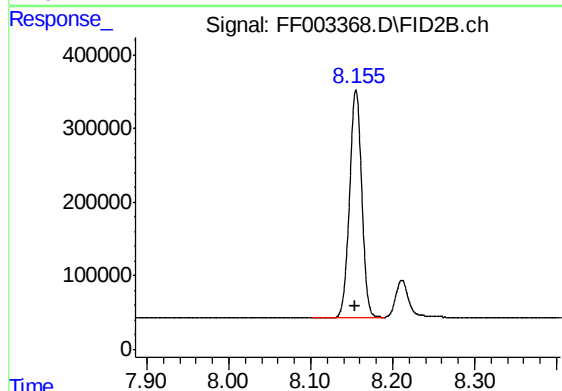


#4 N-TETRADECANE

R.T.: 8.155 min
Delta R.T.: 0.002 min
Response: 3207724
Conc: 23.70 ug/ml

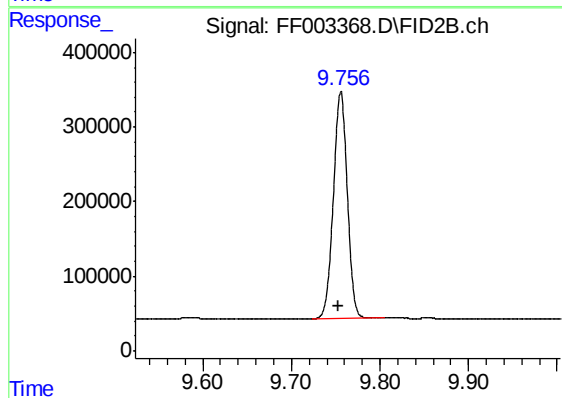


#5 N-HEXADECANE

R.T.: 9.756 min
Delta R.T.: 0.003 min
Response: 3318029
Conc: 24.35 ug/ml

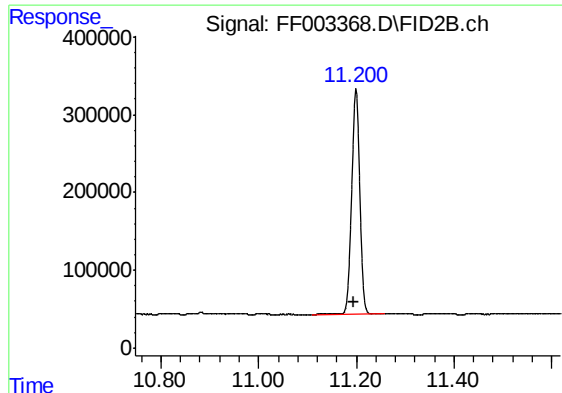


#6 N-OCTADECANE

R.T.: 11.200 min
Delta R.T.: 0.004 min
Response: 3344688
Conc: 24.31 ug/ml

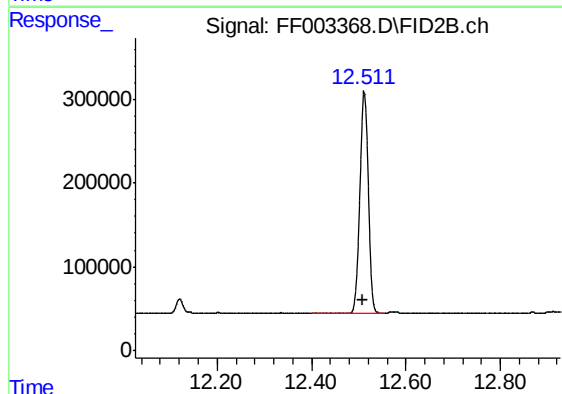


#7 N-EICOSANE

R.T.: 12.512 min
Delta R.T.: 0.004 min
Response: 3278286
Conc: 23.84 ug/ml

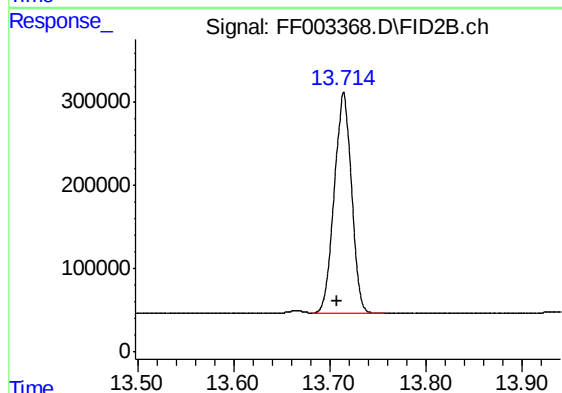


#8 N-DOCOSANE

R.T.: 13.714 min
Delta R.T.: 0.006 min
Response: 3284323
Conc: 24.00 ug/ml

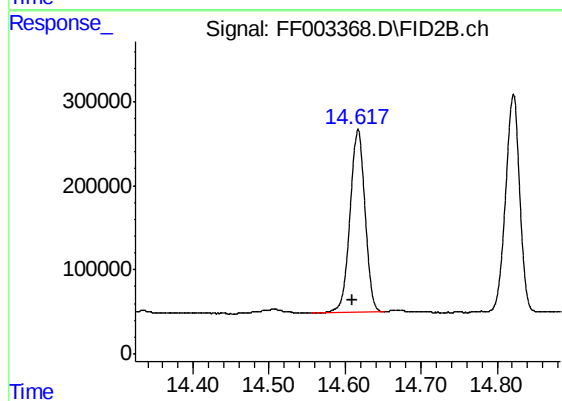


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.617 min
Delta R.T.: 0.007 min
Response: 2961240
Conc: 24.53 ug/ml

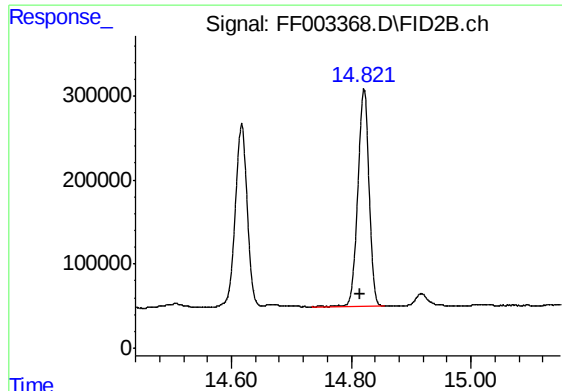


#10 N-TETRACOSANE

R.T.: 14.822 min
Delta R.T.: 0.008 min
Response: 3369120
Conc: 24.77 ug/ml

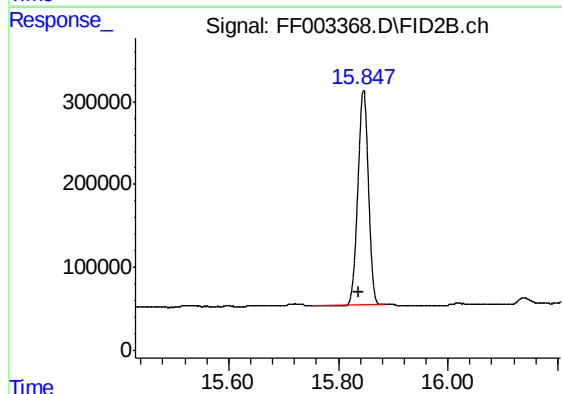

#11 N-HEXACOSANE

R.T.: 15.846 min
Delta R.T.: 0.008 min
Response: 3457941
Conc: 25.49 ug/ml

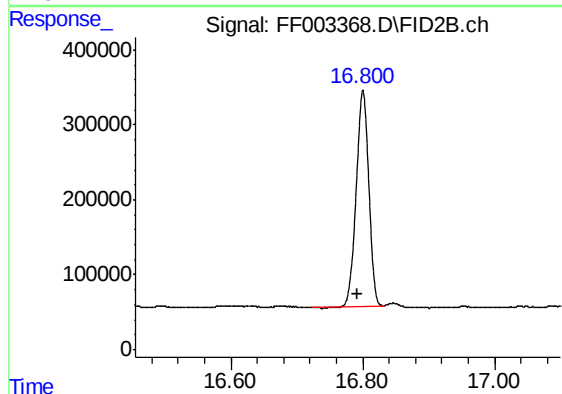

#12 N-OCTACOSANE

R.T.: 16.800 min
Delta R.T.: 0.009 min
Response: 3787999
Conc: 27.67 ug/ml