

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020419\
 Data File : FF003370.D
 Signal(s) : FID2B.ch
 Acq On : 04 Feb 2019 21:04
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 05 00:02:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
 Quant Title :
 QLast Update : Fri Feb 01 22:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.629	5662092	46.900 ug/ml
Target Compounds			
2) N-DECANE	4.355	6579066	49.160 ug/ml
3) N-DODECANE	6.376	6609863	49.024 ug/ml
4) N-TETRADECANE	8.168	6597965	48.745 ug/ml
5) N-HEXADECANE	9.768	6605797	48.473 ug/ml
6) N-OCTADECANE	11.213	6591236	47.901 ug/ml
7) N-EICOSANE	12.525	6497040	47.246 ug/ml
8) N-DOCOSANE	13.727	6412194	46.866 ug/ml
10) N-TETRACOSANE	14.833	6325465	46.513 ug/ml
11) N-HEXACOSANE	15.858	6285578	46.342 ug/ml
12) N-OCTACOSANE	16.812	6300241	46.016 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020419\
Data File : FF003370.D
Signal(s) : FID2B.ch
Acq On : 04 Feb 2019 21:04
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 05 00:02:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

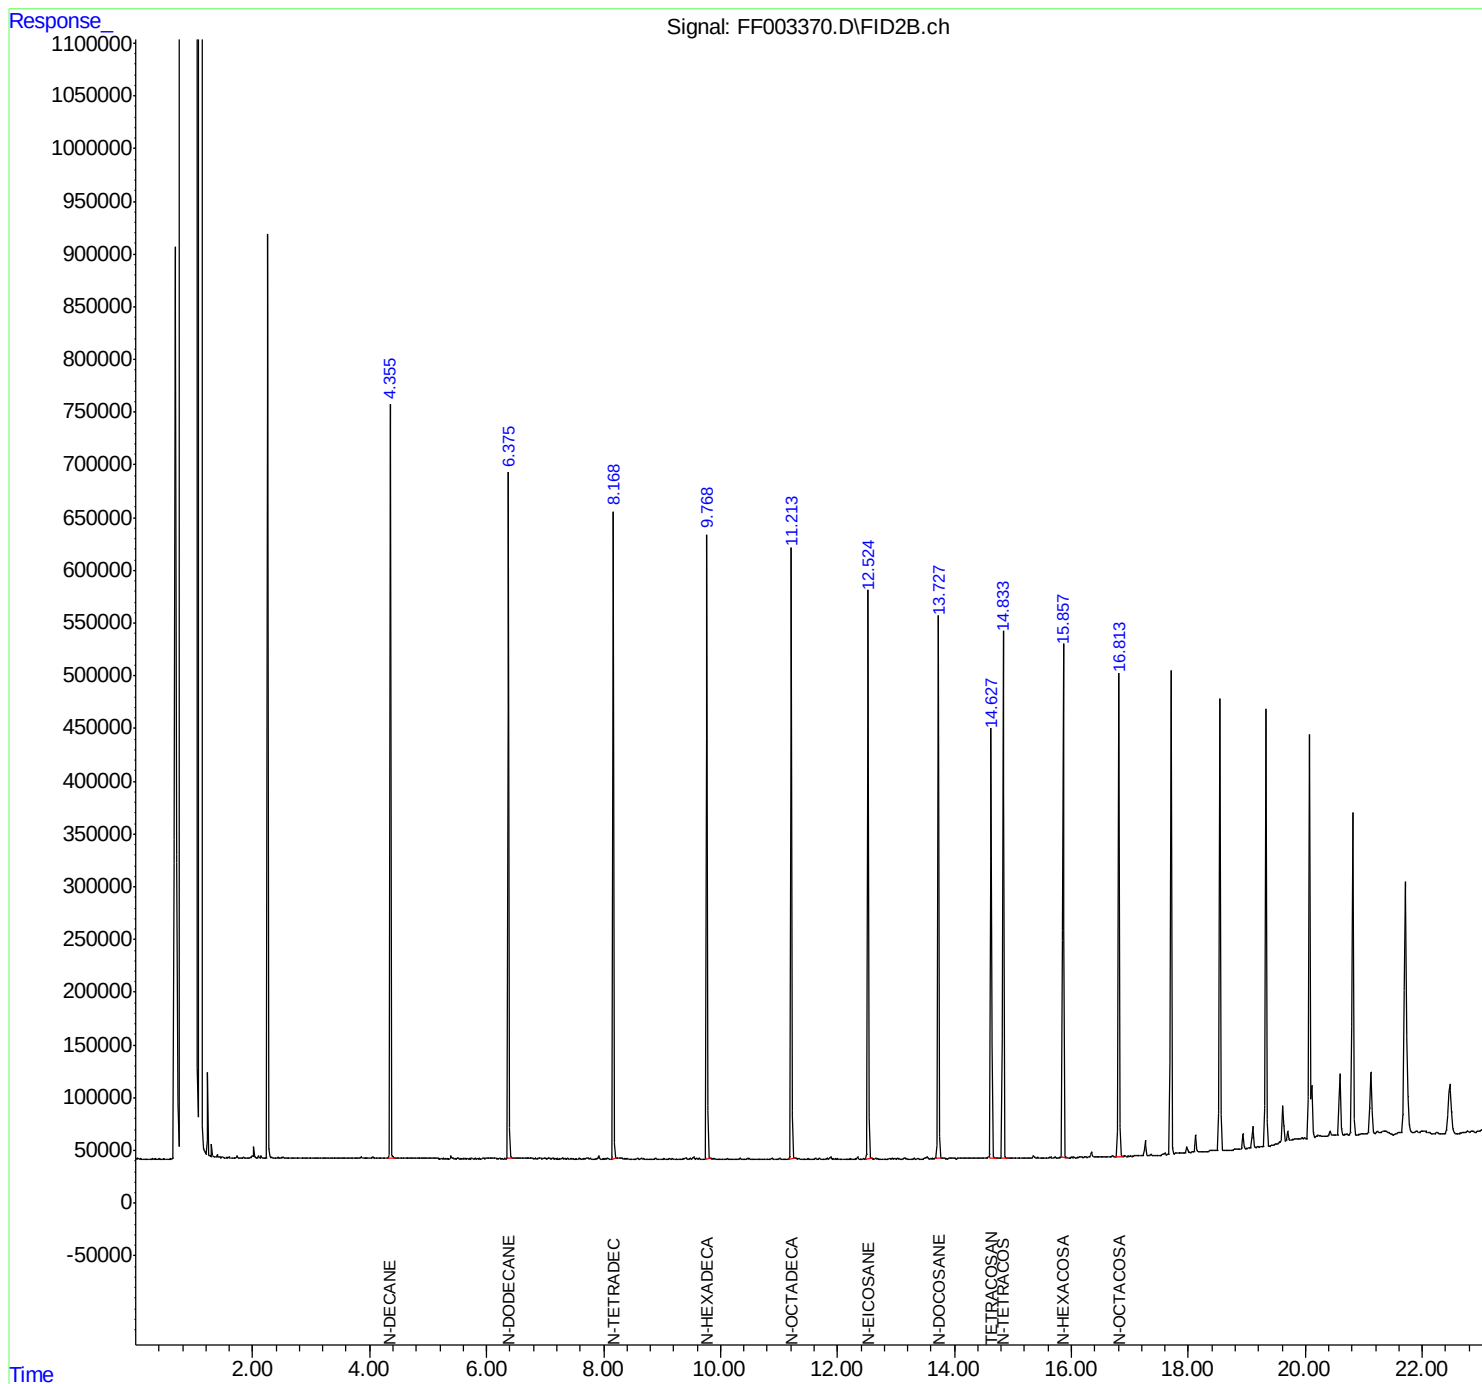

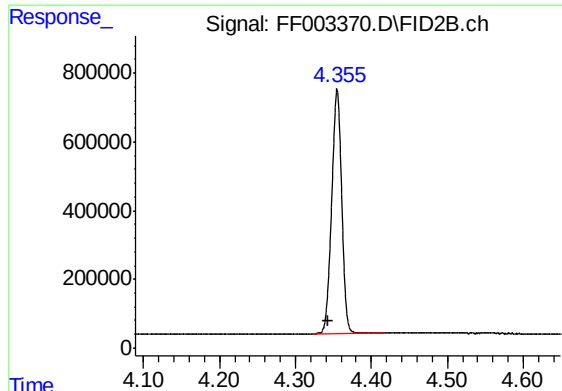


#2 N-DECANE

R.T.: 4.355 min
Delta R.T.: 0.013 min
Response: 6579066
Conc: 49.16 ug/ml

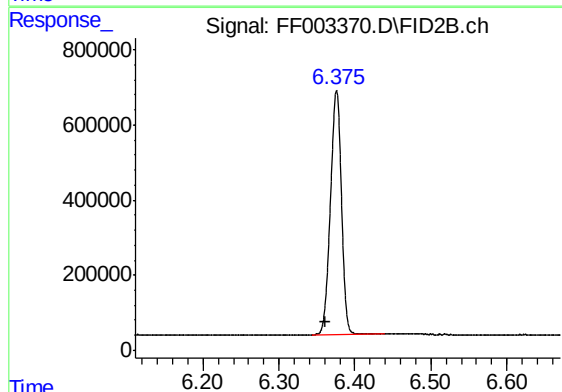


#3 N-DODECANE

R.T.: 6.376 min
Delta R.T.: 0.015 min
Response: 6609863
Conc: 49.02 ug/ml

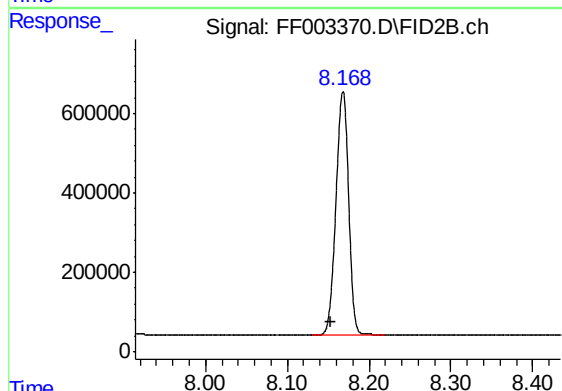


#4 N-TETRADECANE

R.T.: 8.168 min
Delta R.T.: 0.015 min
Response: 6597965
Conc: 48.75 ug/ml

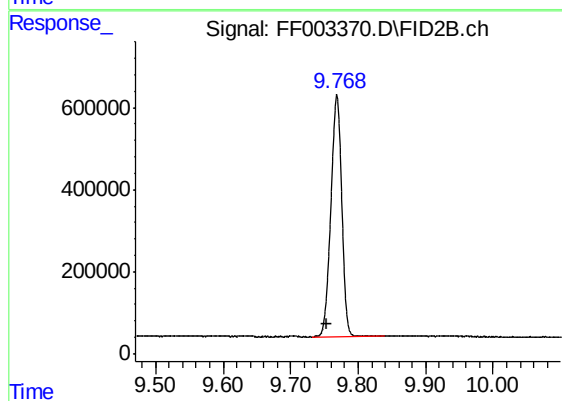


#5 N-HEXADECANE

R.T.: 9.768 min
Delta R.T.: 0.016 min
Response: 6605797
Conc: 48.47 ug/ml

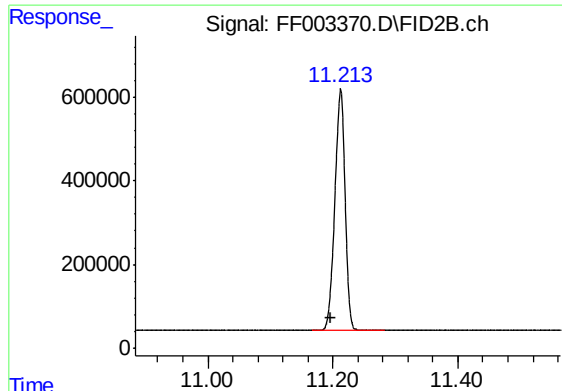


#6 N-OCTADECANE

R.T.: 11.213 min
Delta R.T.: 0.017 min
Response: 6591236
Conc: 47.90 ug/ml

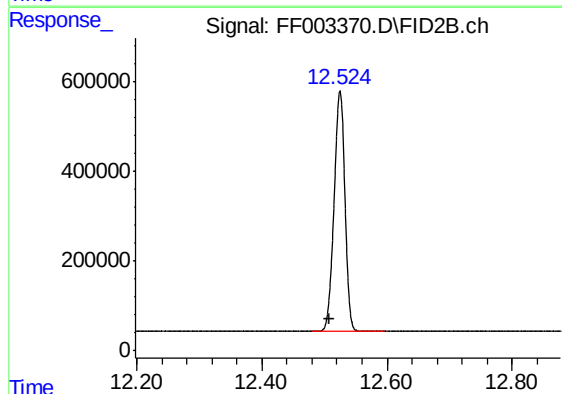


#7 N-EICOSANE

R.T.: 12.525 min
Delta R.T.: 0.017 min
Response: 6497040
Conc: 47.25 ug/ml

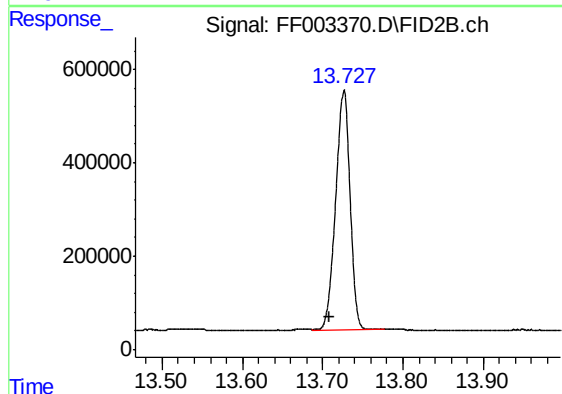


#8 N-DOCOSANE

R.T.: 13.727 min
Delta R.T.: 0.019 min
Response: 6412194
Conc: 46.87 ug/ml

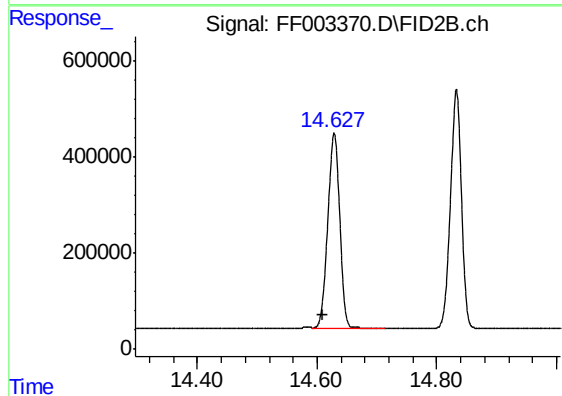


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.629 min
Delta R.T.: 0.019 min
Response: 5662092
Conc: 46.90 ug/ml

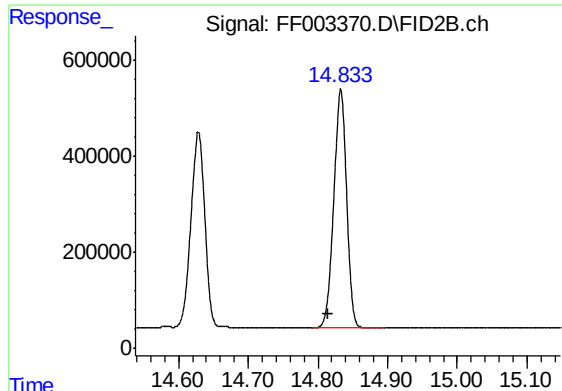


#10 N-TETRACOSANE

R.T.: 14.833 min
Delta R.T.: 0.019 min
Response: 6325465
Conc: 46.51 ug/ml

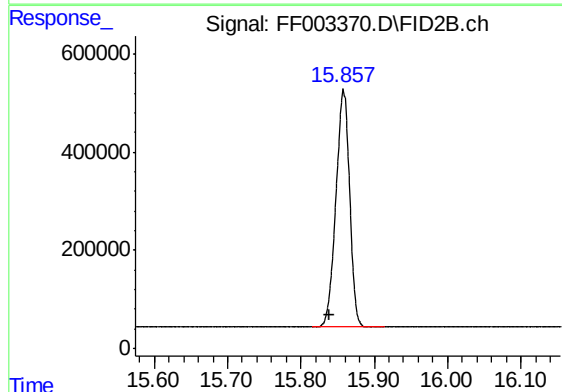

#11 N-HEXACOSANE

R.T.: 15.858 min
Delta R.T.: 0.020 min
Response: 6285578
Conc: 46.34 ug/ml

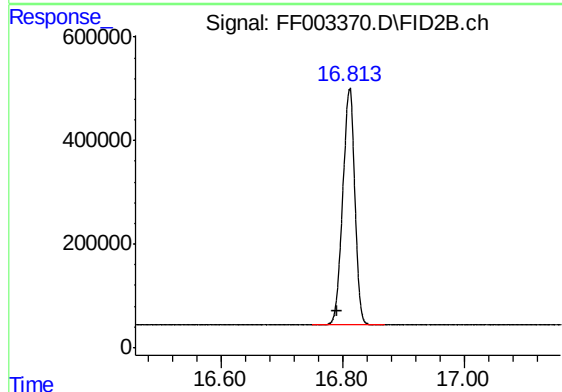

#12 N-OCTACOSANE

R.T.: 16.812 min
Delta R.T.: 0.021 min
Response: 6300241
Conc: 46.02 ug/ml