

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020422\
 Data File : FF009858.D
 Signal(s) : FID2B.ch
 Acq On : 04 Feb 2022 08:57
 Operator : AJ\MA
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 04 22:02:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
8) N-DOCOSANE	13.526	148450	0.998 ug/ml
10) N-TETRACOSANE	14.627	110034	0.742 ug/ml
11) N-HEXACOSANE	15.645	130128	0.890 ug/ml
12) N-OCTACOSANE	16.592	267791	1.845 ug/ml
13) N-TRIACONTANE	17.476	258013	1.803 ug/ml
14) N-DOTRIACONTANE	18.308	835955	6.143 ug/ml
15) N-TETRATRIACONTANE	19.124	535976	4.513 ug/ml
16) N-HEXATRIACONTANE	19.866	684857	6.642 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020422\
Data File : FF009858.D
Signal(s) : FID2B.ch
Acq On : 04 Feb 2022 08:57
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 04 22:02:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

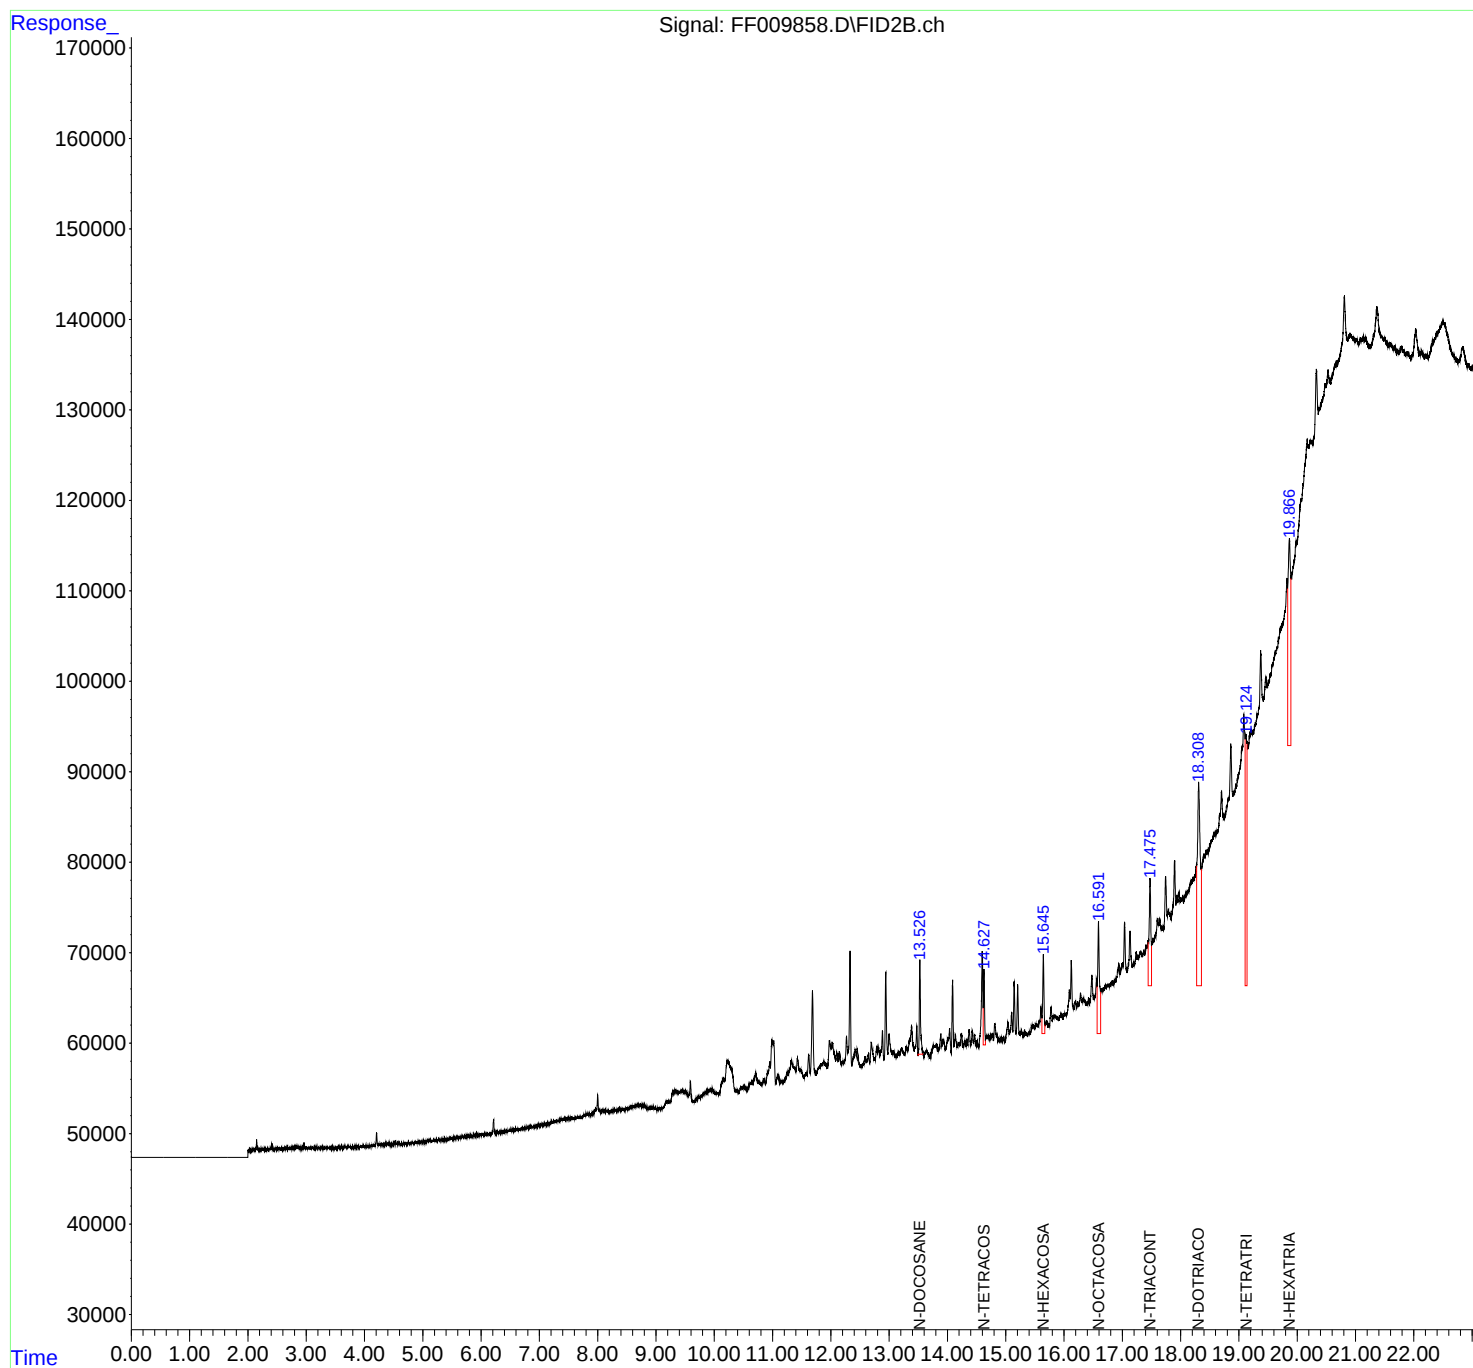


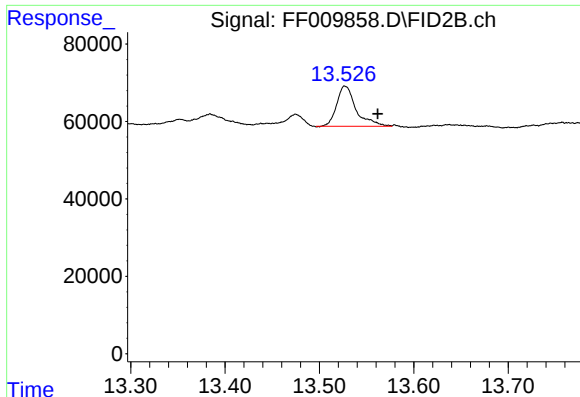

#8 N-DOCOSANE


R.T.: 13.526 min
Delta R.T.: -0.035 min
Response: 148450
Conc: 1.00 ug/ml

Instrument :
FID_F
ClientSampleId :

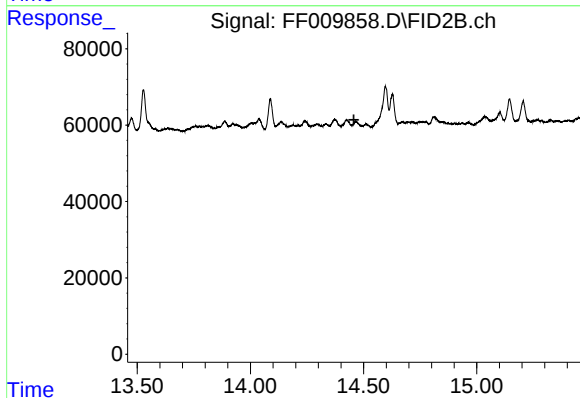


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.457 min
Response: 0
Conc: N.D.

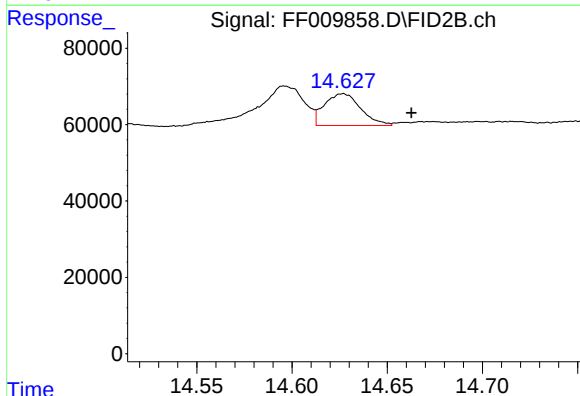


#10 N-TETRACOSANE

R.T.: 14.627 min
Delta R.T.: -0.036 min
Response: 110034
Conc: 0.74 ug/ml

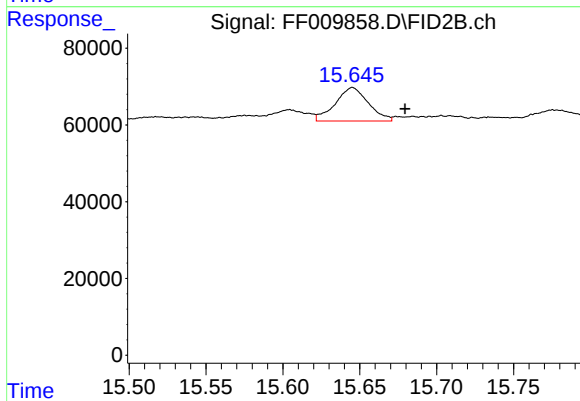

#11 N-HEXACOSANE


R.T.: 15.645 min
Delta R.T.: -0.034 min
Response: 130128
Conc: 0.89 ug/ml

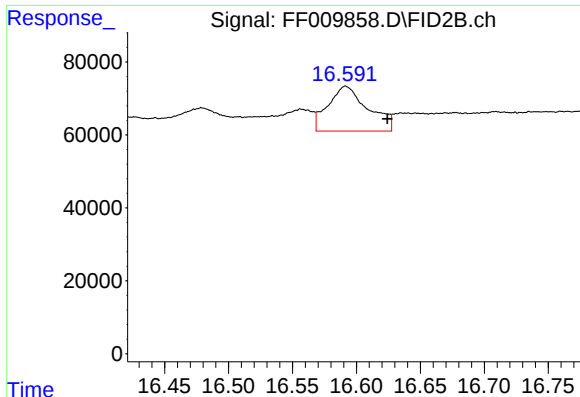

#12 N-OCTACOSANE


R.T.: 16.592 min
Delta R.T.: -0.033 min
Response: 267791
Conc: 1.84 ug/ml

Instrument :
FID_F
ClientSampleId :

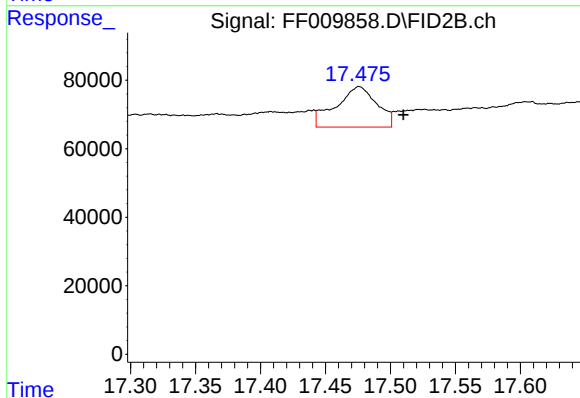


#13 N-TRIACONTANE

R.T.: 17.476 min
Delta R.T.: -0.034 min
Response: 258013
Conc: 1.80 ug/ml

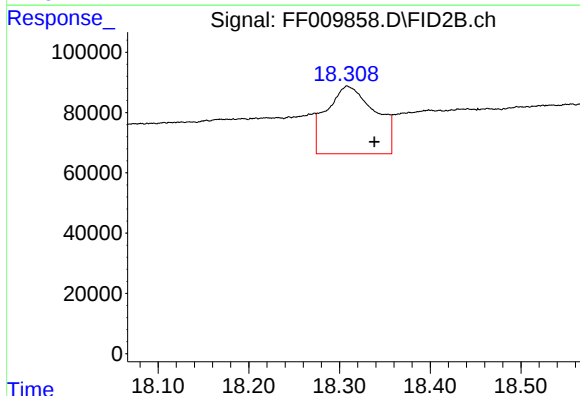


#14 N-DOTRIACONTANE

R.T.: 18.308 min
Delta R.T.: -0.030 min
Response: 835955
Conc: 6.14 ug/ml

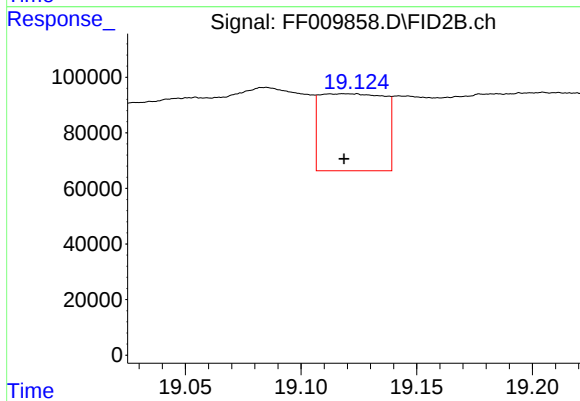

#15 N-TETRATRIACONTANE

R.T.: 19.124 min
Delta R.T.: 0.006 min
Response: 535976
Conc: 4.51 ug/ml

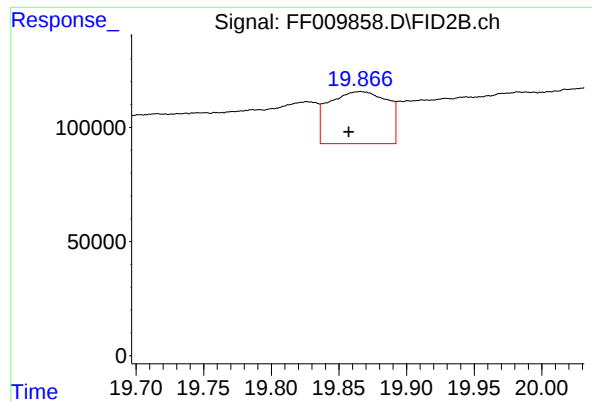

#16 N-HEXATRIACONTANE

R.T.: 19.866 min
Delta R.T.: 0.009 min
Response: 684857
Conc: 6.64 ug/ml

Instrument :

FID_F

ClientSampleId :