

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020422\
 Data File : FF009862.D
 Signal(s) : FID2B.ch
 Acq On : 04 Feb 2022 10:59
 Operator : AJ\MA
 Sample : N1381-05 100X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 04 22:02:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
2) N-DECANE	4.281	70933	0.502 ug/ml
3) N-DODECANE	6.238	400562	2.799 ug/ml
4) N-TETRADECANE	8.054	310026	2.110 ug/ml
6) N-OCTADECANE	11.124f	78538	0.509 ug/ml
14) N-DOTRIACONTANE	18.315	138731	1.019 ug/ml
15) N-TETRATRIACONTANE	19.092	1602883	13.495 ug/ml
16) N-HEXATRIACONTANE	19.864	3318603	32.187 ug/ml
18) N-TETRACONTANE	21.370	206411	2.272 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020422\
Data File : FF009862.D
Signal(s) : FID2B.ch
Acq On : 04 Feb 2022 10:59
Operator : AJ\MA
Sample : N1381-05 100X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 04 22:02:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

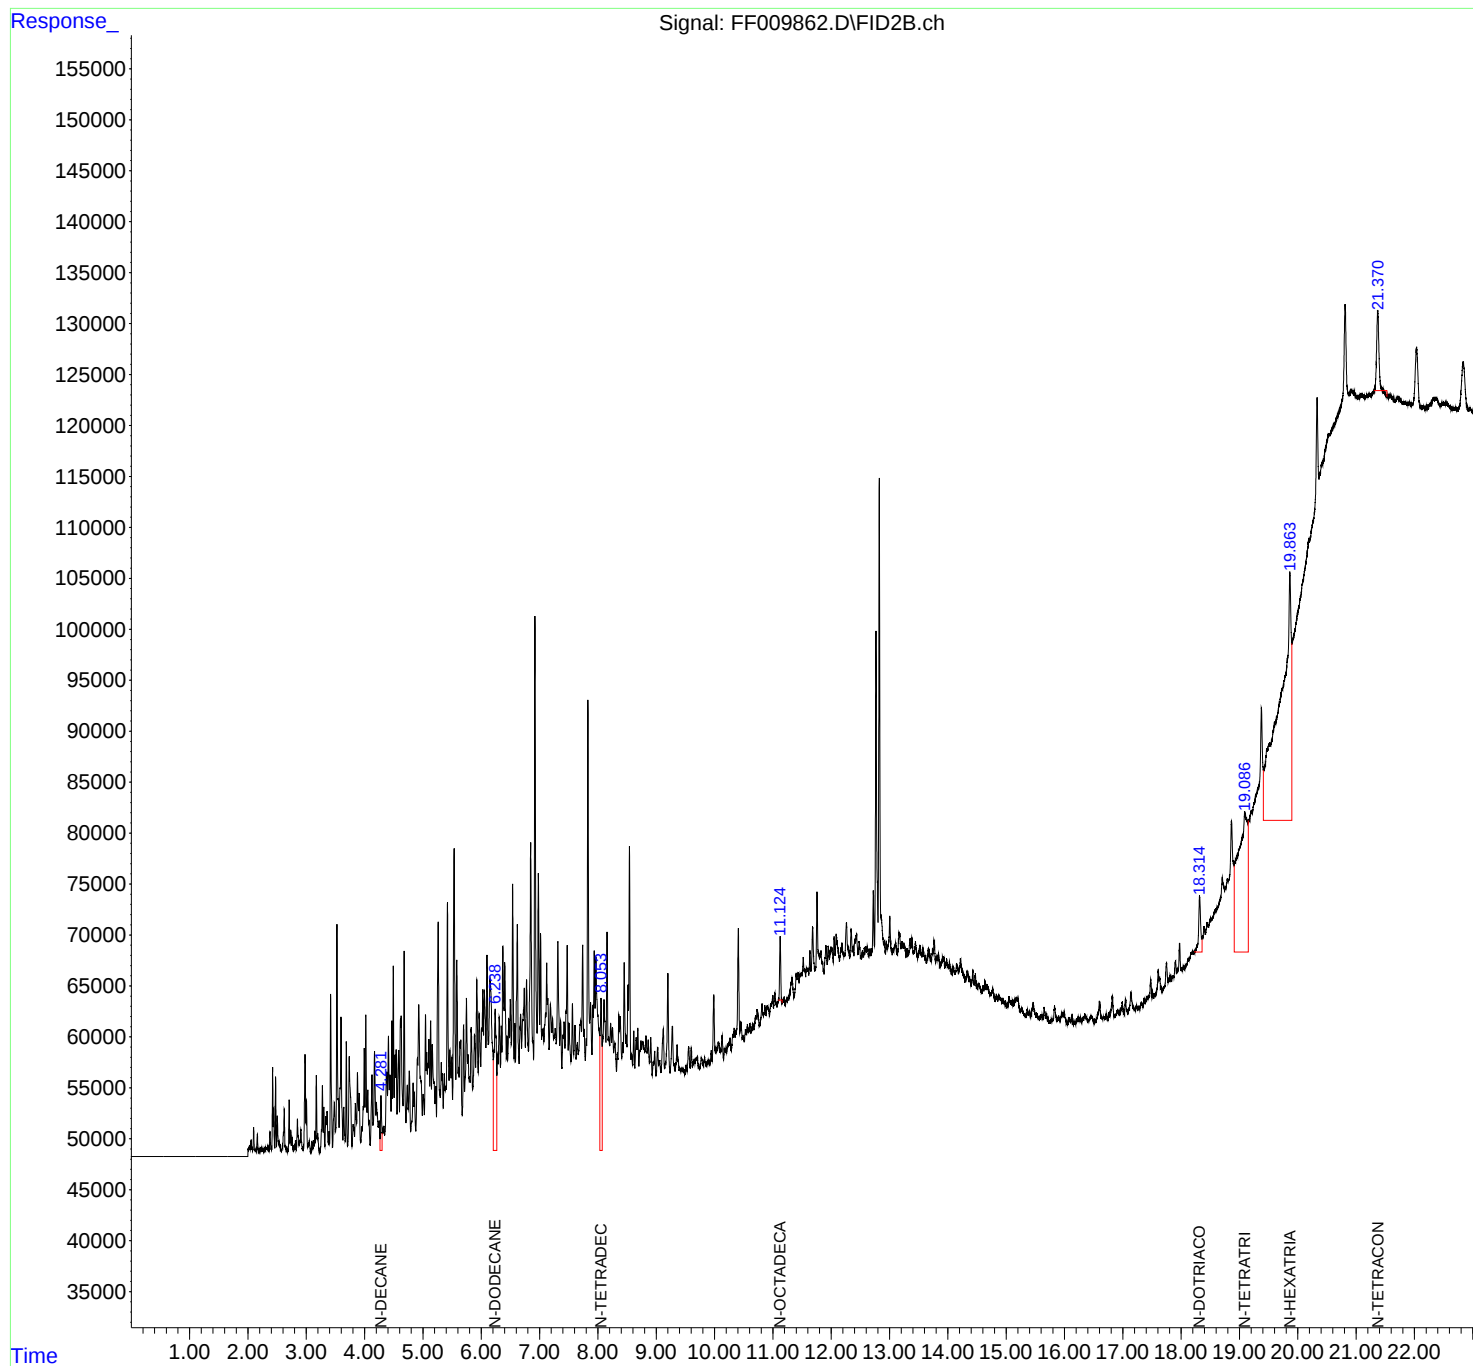


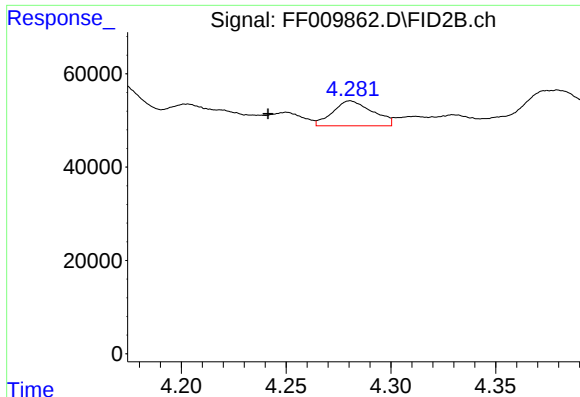

#2 N-DECANE


R.T.: 4.281 min
Delta R.T.: 0.039 min
Response: 70933
Conc: 0.50 ug/ml

Instrument :
FID_F
ClientSampleId :

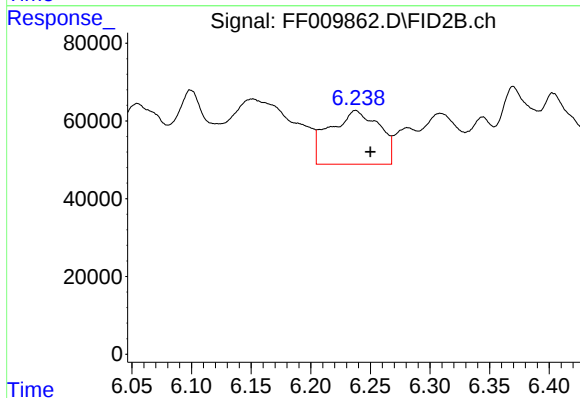


#3 N-DODECANE

R.T.: 6.238 min
Delta R.T.: -0.012 min
Response: 400562
Conc: 2.80 ug/ml

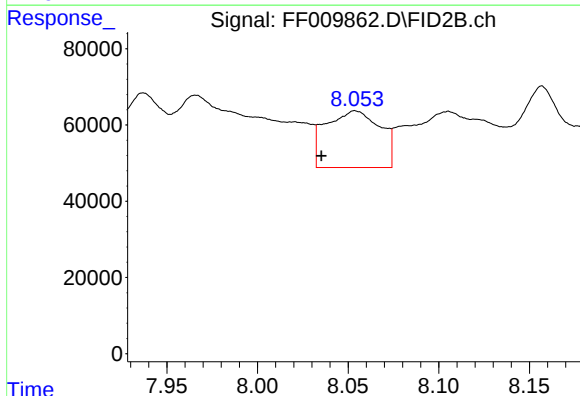


#4 N-TETRADECANE

R.T.: 8.054 min
Delta R.T.: 0.019 min
Response: 310026
Conc: 2.11 ug/ml

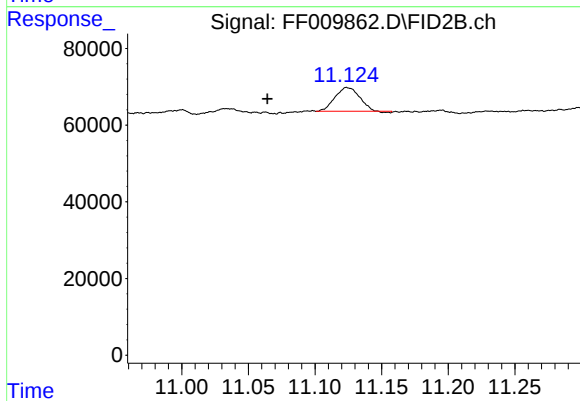

#6 N-OCTADECANE


R.T.: 11.124 min
Delta R.T.: 0.060 min
Response: 78538
Conc: 0.51 ug/ml

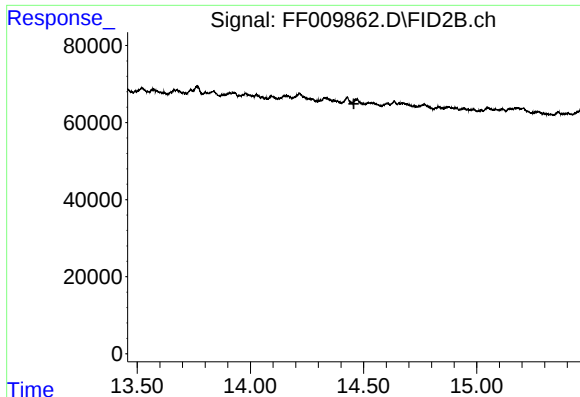

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.457 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

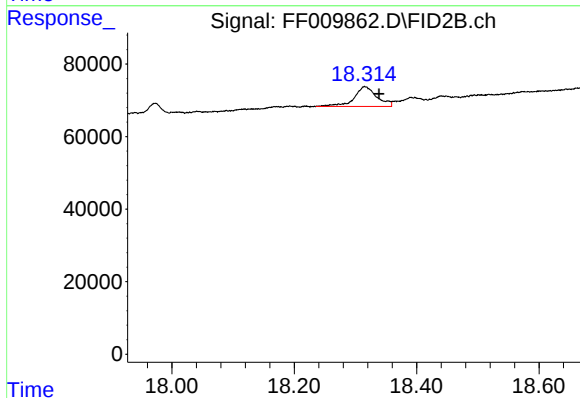


#14 N-DOTRIACONTANE

R.T.: 18.315 min
Delta R.T.: -0.023 min
Response: 138731
Conc: 1.02 ug/ml

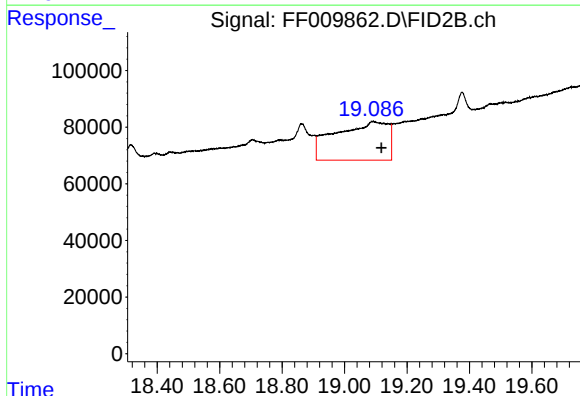


#15 N-TETRATRIACONTANE

R.T.: 19.092 min
Delta R.T.: -0.027 min
Response: 1602883
Conc: 13.50 ug/ml

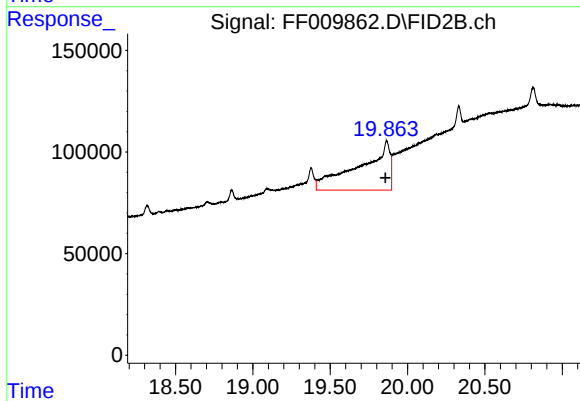

#16 N-HEXATRIACONTANE

R.T.: 19.864 min
Delta R.T.: 0.007 min
Response: 3318603
Conc: 32.19 ug/ml

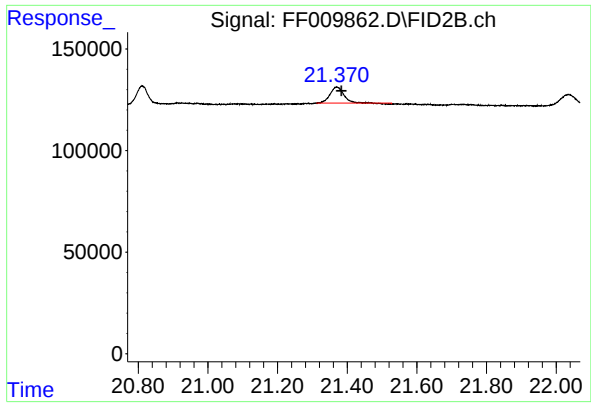

#18 N-TETRACONTANE

R.T.: 21.370 min
Delta R.T.: -0.013 min
Response: 206411
Conc: 2.27 ug/ml

Instrument :

FID_F

ClientSampleId :