

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020422\
Data File : FF009863.D
Signal(s) : FID2B.ch
Acq On : 04 Feb 2022 11:29
Operator : AJ\MA
Sample : N1381-07 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 04 22:02:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

5)	N-HEXADECANE	9.604	415276	2.776 ug/ml
6)	N-OCTADECANE	11.126f	88706	0.575 ug/ml
7)	N-EICOSANE	12.343	17934	0.119 ug/ml
16)	N-HEXATRIACONTANE	19.864	732950	7.109 ug/ml
18)	N-TETRACONTANE	21.372	239892	2.641 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020422\
Data File : FF009863.D
Signal(s) : FID2B.ch
Acq On : 04 Feb 2022 11:29
Operator : AJ\MA
Sample : N1381-07 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 04 22:02:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

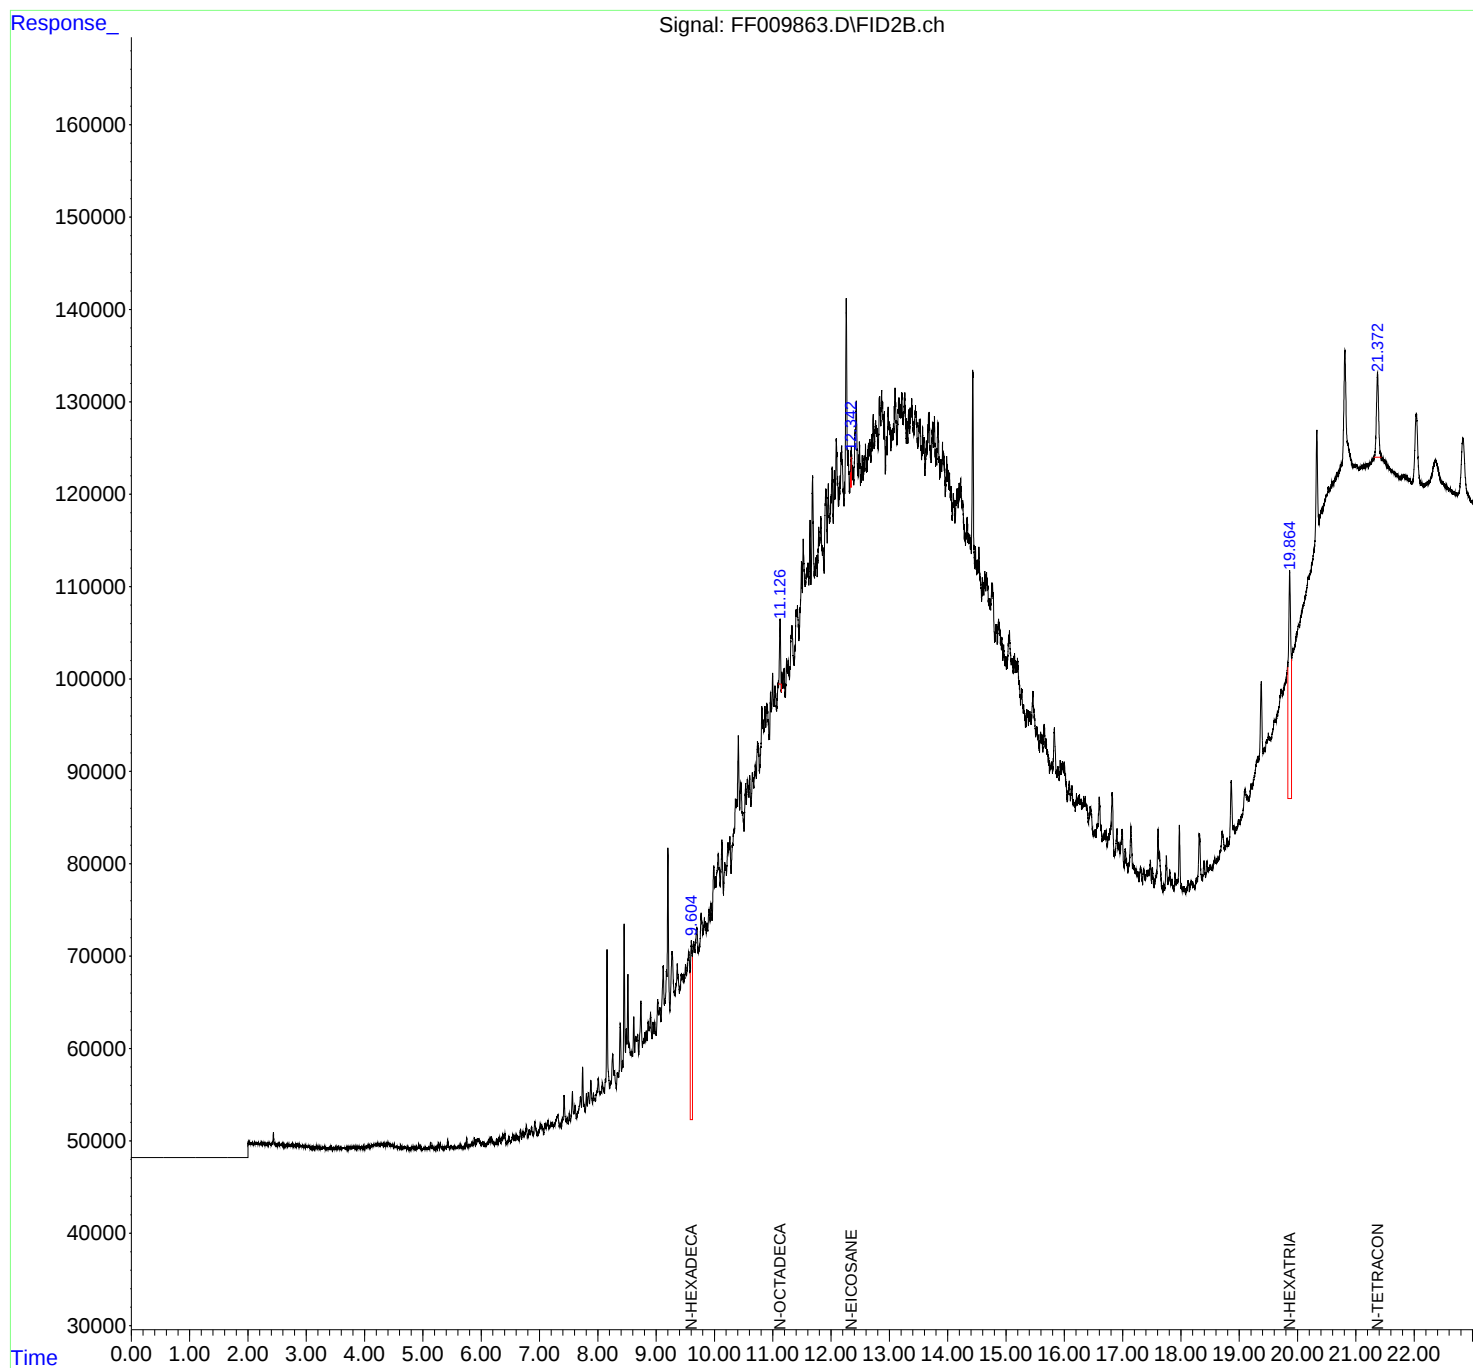


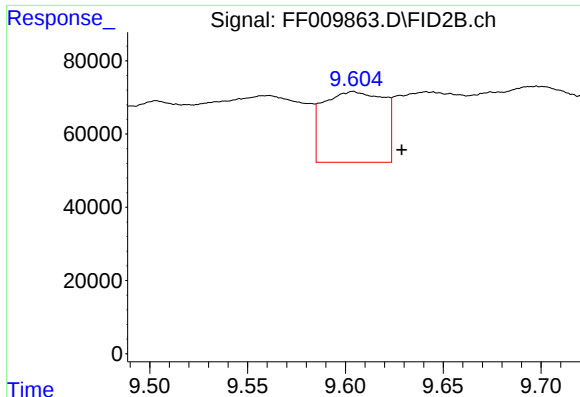

#5 N-HEXADECANE


R.T.: 9.604 min
Delta R.T.: -0.025 min
Response: 415276
Conc: 2.78 ug/ml

Instrument :
FID_F
ClientSampleId :

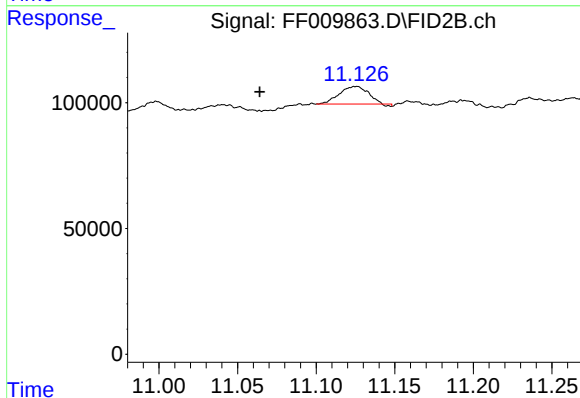


#6 N-OCTADECANE

R.T.: 11.126 min
Delta R.T.: 0.062 min
Response: 88706
Conc: 0.58 ug/ml

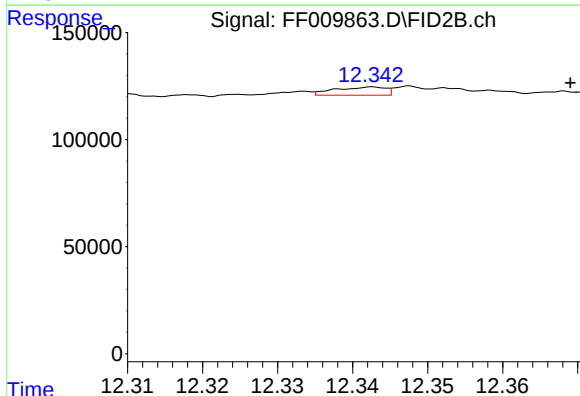


#7 N-EICOSANE

R.T.: 12.343 min
Delta R.T.: -0.026 min
Response: 17934
Conc: 0.12 ug/ml

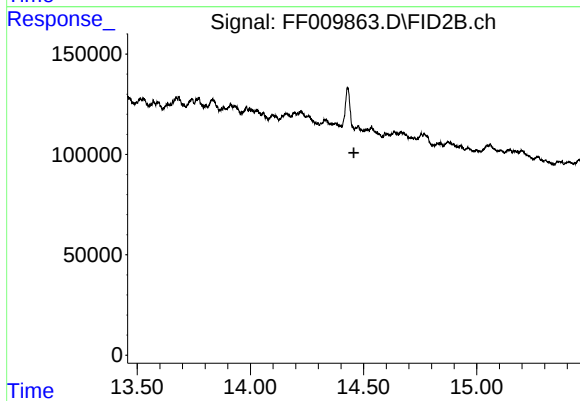

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.431 min
Delta R.T.: -0.026 min
Response: -115016
Conc: N.D.

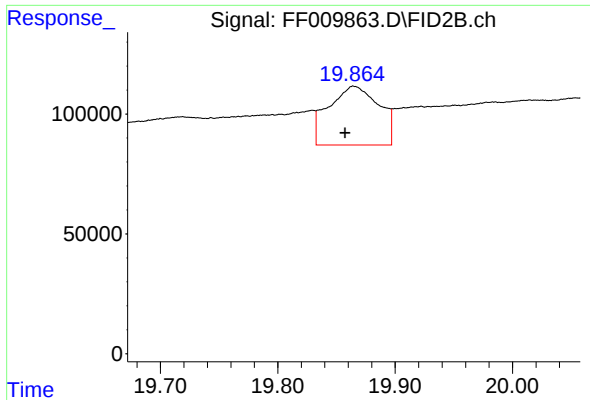

#16 N-HEXATRIACONTANE

R.T.: 19.864 min
Delta R.T.: 0.007 min
Response: 732950
Conc: 7.11 ug/ml

Instrument :
FID_F
ClientSampleId :

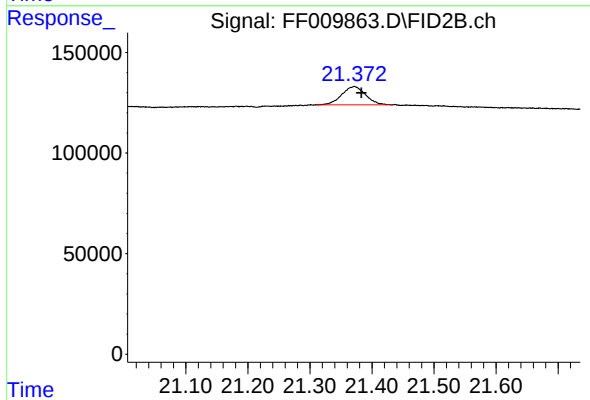

#18 N-TETRACONTANE

R.T.: 21.372 min
Delta R.T.: -0.012 min
Response: 239892
Conc: 2.64 ug/ml