

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020422\
Data File : FF009864.D
Signal(s) : FID2B.ch
Acq On : 04 Feb 2022 11:58
Operator : AJ\MA
Sample : N1381-09 50X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 04 22:02:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

2)	N-DECANE	4.175f	85639	0.606 ug/ml
3)	N-DODECANE	6.239	208729	1.459 ug/ml
6)	N-OCTADECANE	11.125f	51735	0.336 ug/ml
14)	N-DOTRIACONTANE	18.307	816027	5.997 ug/ml
15)	N-TETRATRIACONTANE	19.092	1205174	10.147 ug/ml
16)	N-HEXATRIACONTANE	19.864	196820	1.909 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020422\
Data File : FF009864.D
Signal(s) : FID2B.ch
Acq On : 04 Feb 2022 11:58
Operator : AJ\MA
Sample : N1381-09 50X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 04 22:02:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

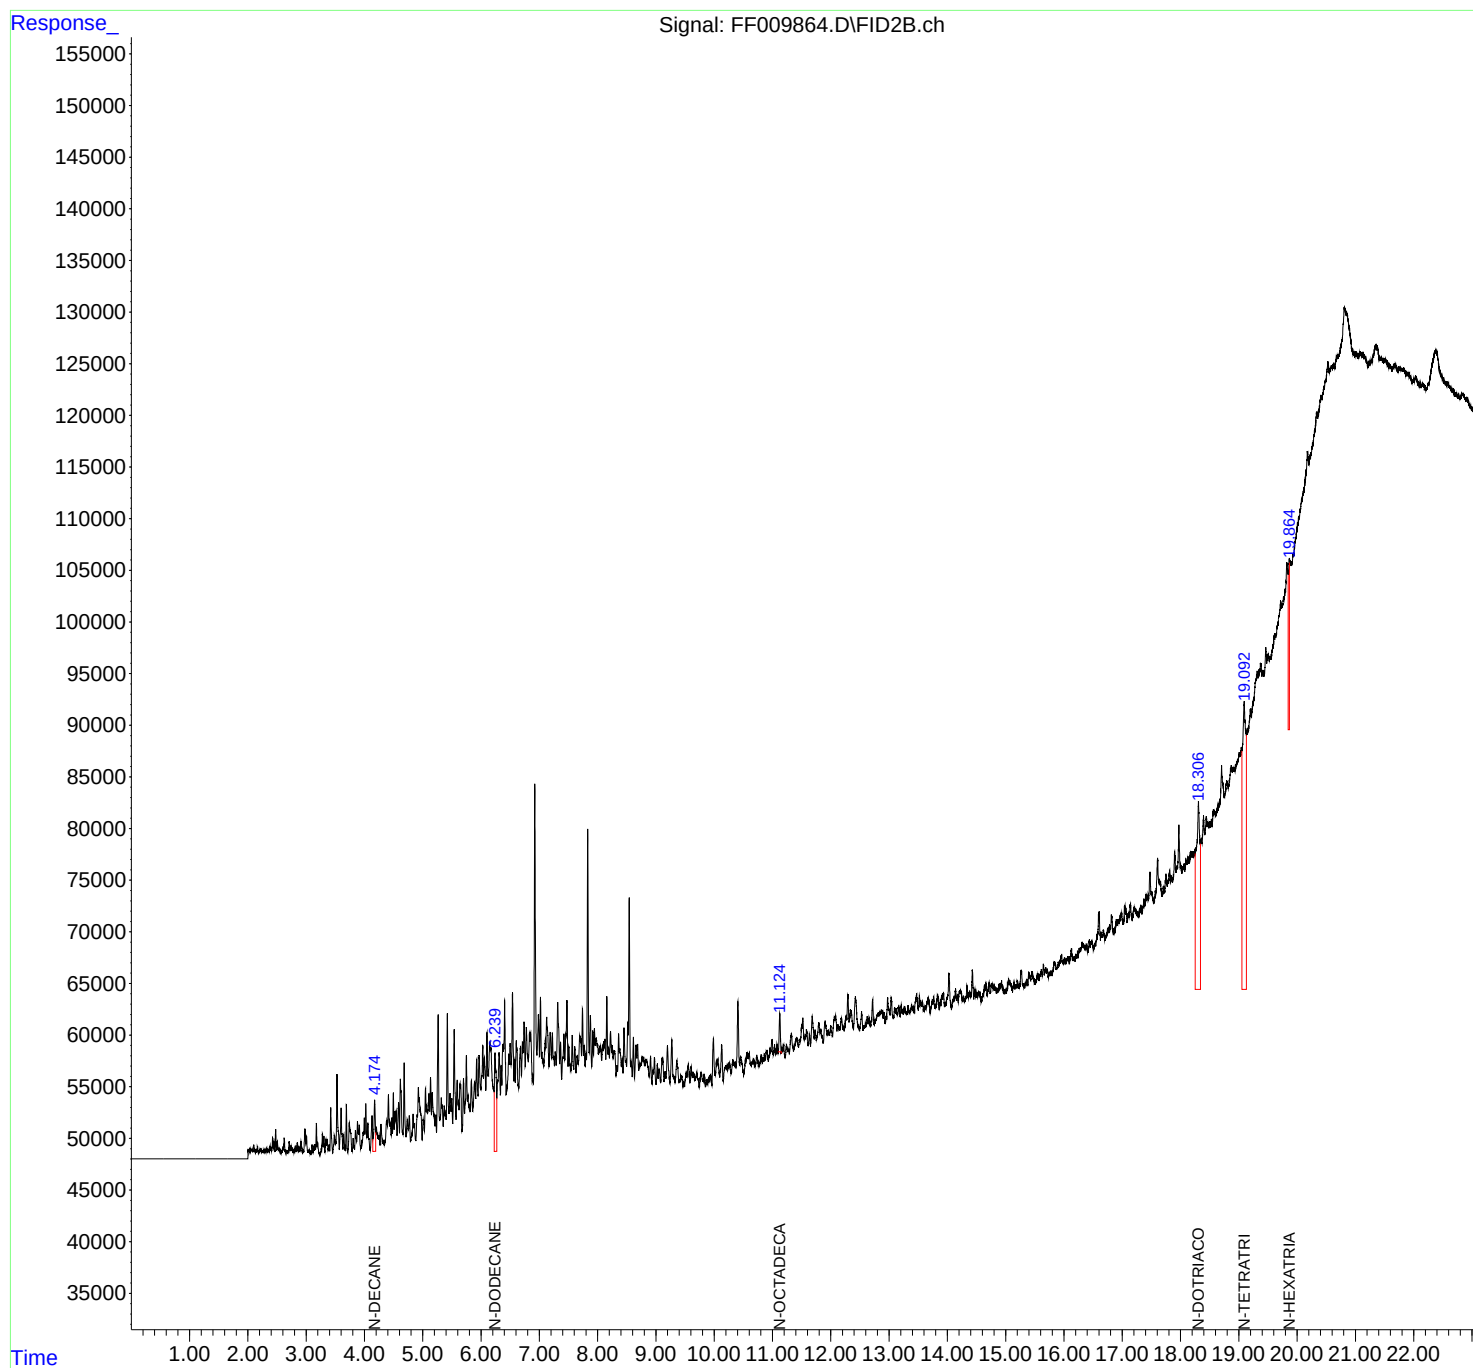


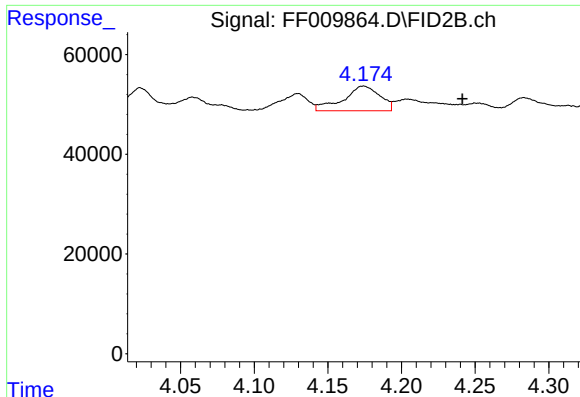

#2 N-DECANE


R.T.: 4.175 min
Delta R.T.: -0.067 min
Response: 85639
Conc: 0.61 ug/ml

Instrument :
FID_F
ClientSampleId :

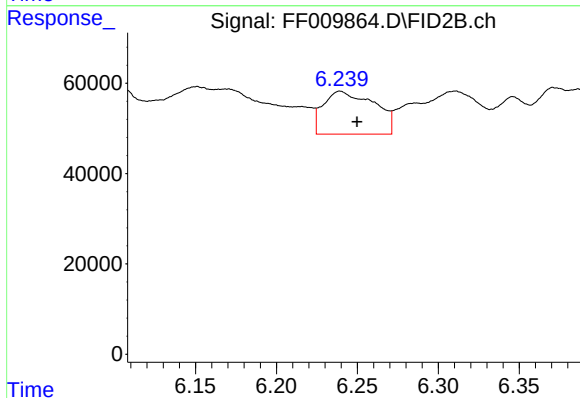


#3 N-DODECANE

R.T.: 6.239 min
Delta R.T.: -0.011 min
Response: 208729
Conc: 1.46 ug/ml

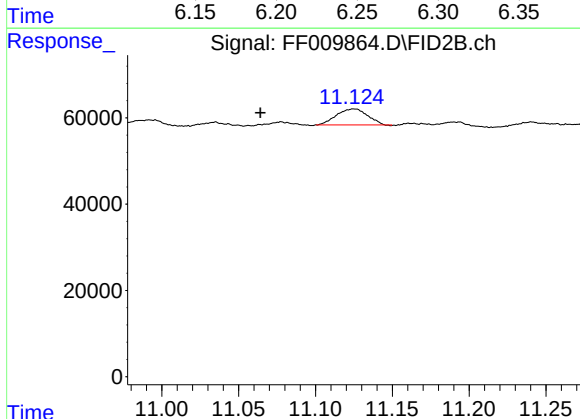


#6 N-OCTADECANE

R.T.: 11.125 min
Delta R.T.: 0.060 min
Response: 51735
Conc: 0.34 ug/ml

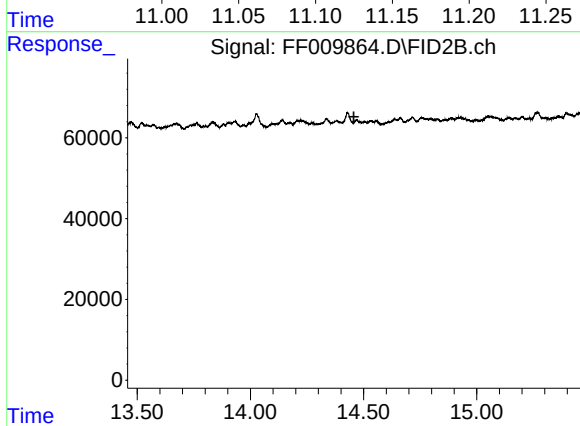

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T. : 14.457 min
Response: 0
Conc: N.D.

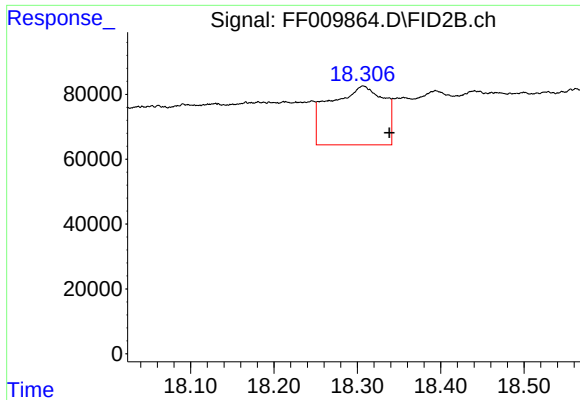

#14 N-DOTRIACONTANE


R.T.: 18.307 min
Delta R.T.: -0.032 min
Response: 816027
Conc: 6.00 ug/ml

Instrument :
FID_F
ClientSampleId :

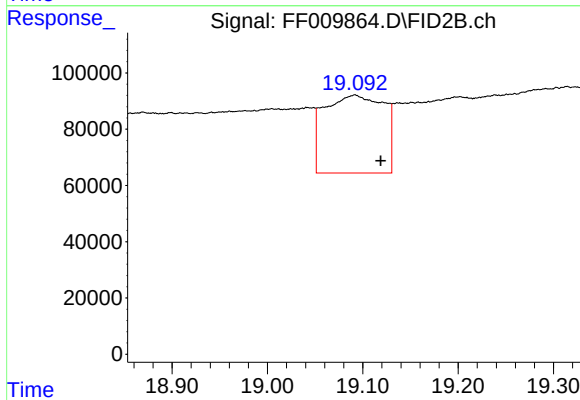

#15 N-TETRATRIACONTANE

R.T.: 19.092 min
Delta R.T.: -0.027 min
Response: 1205174
Conc: 10.15 ug/ml

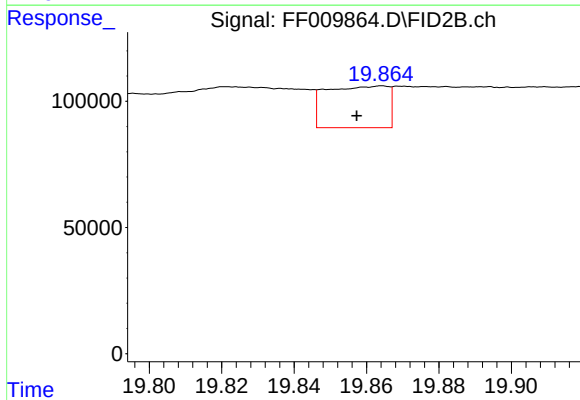

#16 N-HEXATRIACONTANE

R.T.: 19.864 min
Delta R.T.: 0.007 min
Response: 196820
Conc: 1.91 ug/ml