

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF020422\  
Data File : FF009874.D  
Signal(s) : FID2B.ch  
Acq On : 04 Feb 2022 19:56  
Operator : AJ\MA  
Sample : PB142490BL  
Misc :  
ALS Vial : 62 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Feb 04 22:04:04 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF011722.M  
Quant Title :  
QLast Update : Tue Jan 18 02:53:40 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.427 | 1976165  | 15.122 ug/ml |
| Target Compounds              |        |          |              |
| 13) N-TRIACONTANE             | 17.474 | 168678   | 1.179 ug/ml  |
| 14) N-DOTRIACONTANE           | 18.304 | 186481   | 1.370 ug/ml  |
| 15) N-TETRATRIACONTANE        | 19.125 | 140102   | 1.180 ug/ml  |
| 16) N-HEXATRIACONTANE         | 19.865 | 358895   | 3.481 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF020422\  
Data File : FF009874.D  
Signal(s) : FID2B.ch  
Acq On : 04 Feb 2022 19:56  
Operator : AJ\MA  
Sample : PB142490BL  
Misc :  
ALS Vial : 62 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Feb 04 22:04:04 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF011722.M  
Quant Title :  
QLast Update : Tue Jan 18 02:53:40 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

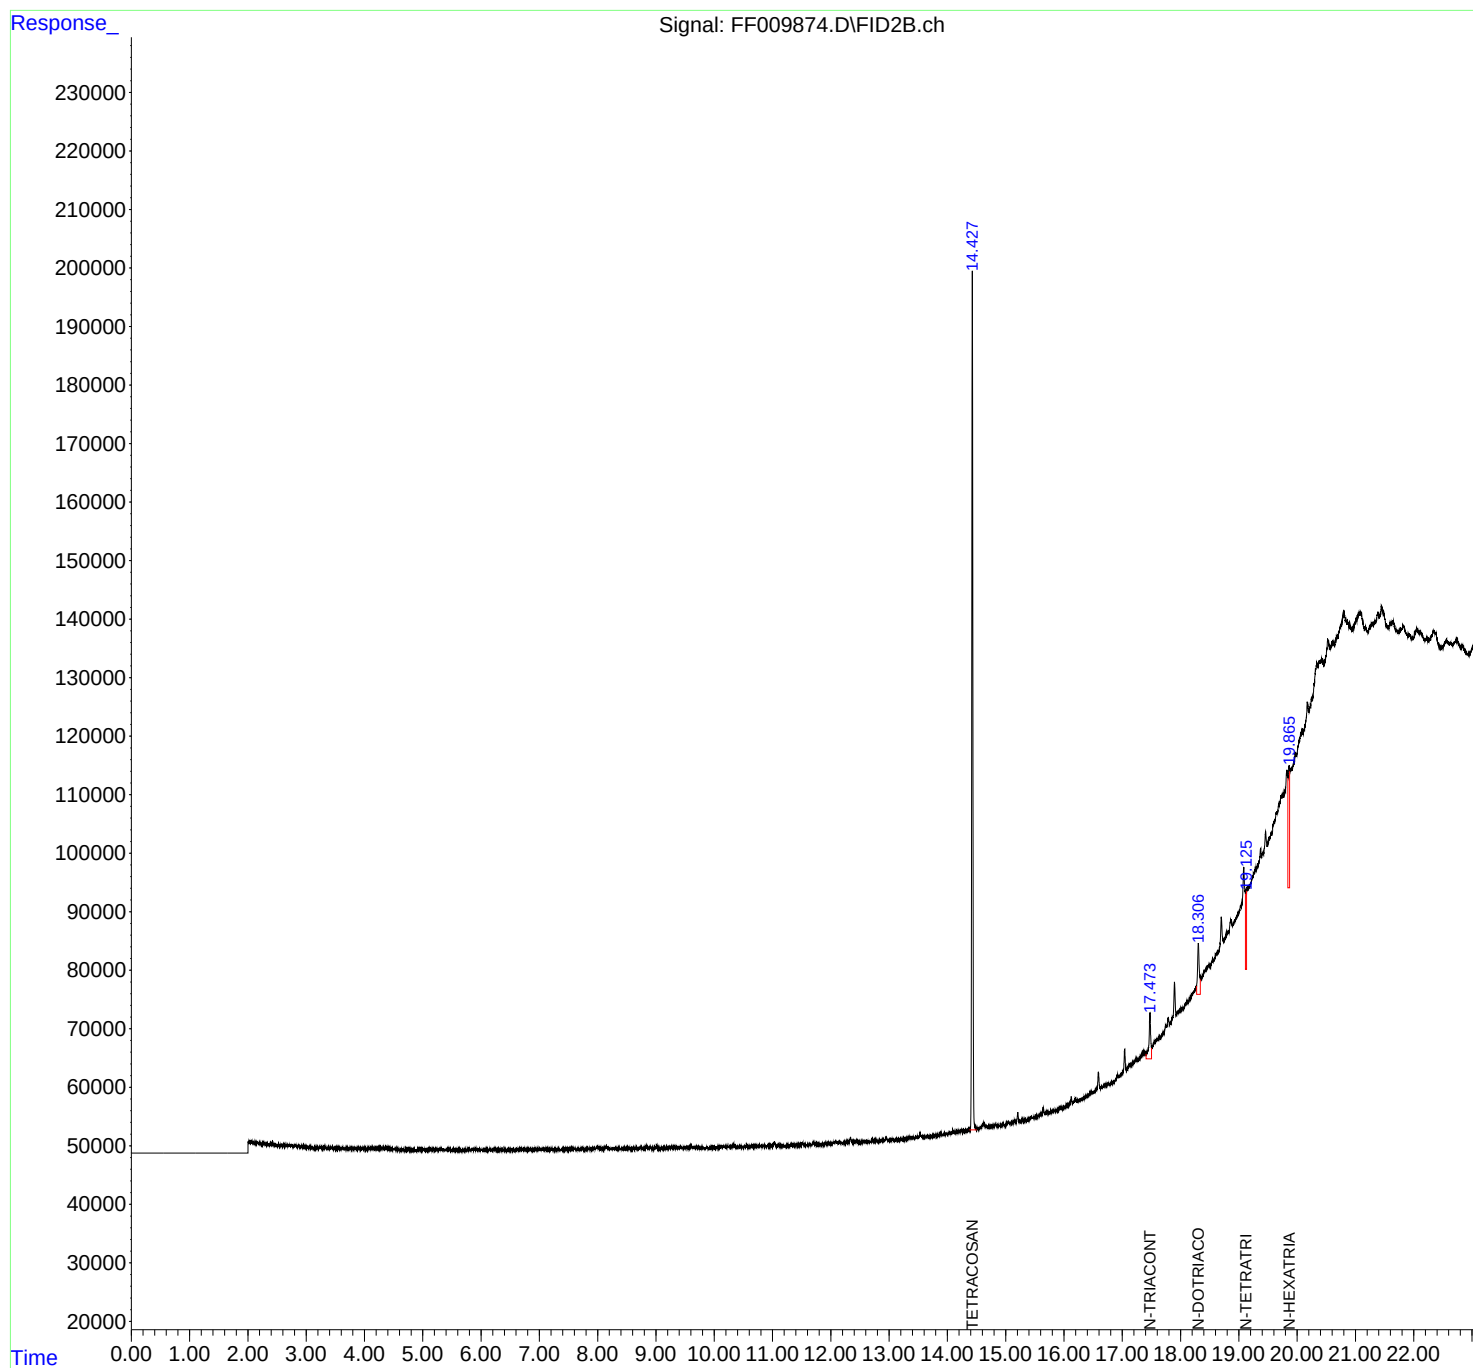


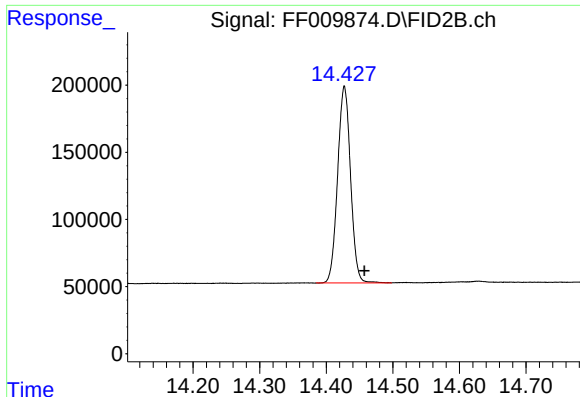

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.427 min  
Delta R.T.: -0.030 min  
Response: 1976165  
Conc: 15.12 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

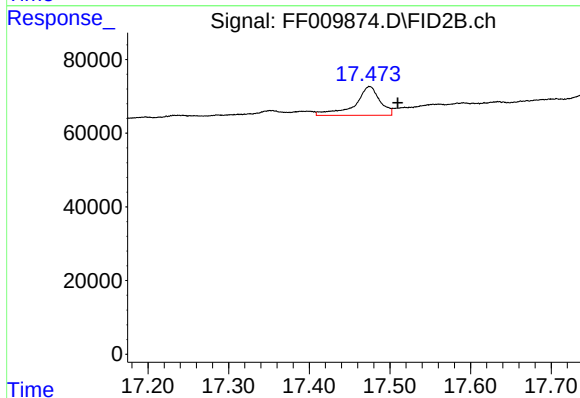


#13 N-TRIACONTANE

R.T.: 17.474 min  
Delta R.T.: -0.036 min  
Response: 168678  
Conc: 1.18 ug/ml

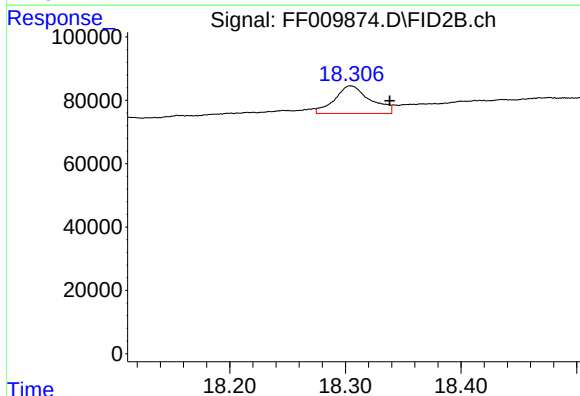


#14 N-DOTRIACONTANE

R.T.: 18.304 min  
Delta R.T.: -0.034 min  
Response: 186481  
Conc: 1.37 ug/ml

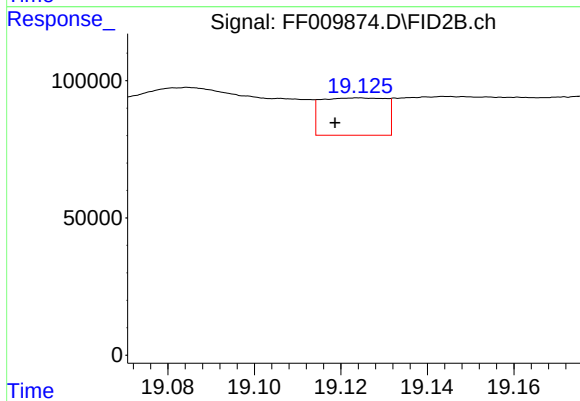

#15 N-TETRATRIACONTANE

R.T.: 19.125 min  
Delta R.T.: 0.006 min  
Response: 140102  
Conc: 1.18 ug/ml

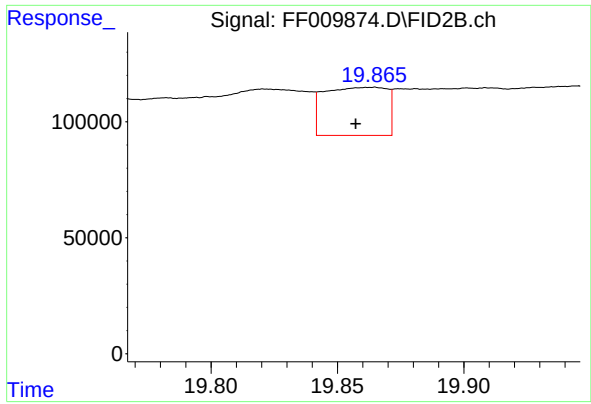

#16 N-HEXATRIACONTANE

R.T.: 19.865 min  
Delta R.T.: 0.008 min  
Response: 358895  
Conc: 3.48 ug/ml

Instrument :  
FID\_F  
ClientSampleId :