

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020422\
Data File : FF009881.D
Signal(s) : FID2B.ch
Acq On : 04 Feb 2022 23:50
Operator : AJ\MA
Sample : N1393-04
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 05 00:56:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.204	630841	4.408 ug/ml
4)	N-TETRADECANE	8.024	522122	3.553 ug/ml
5)	N-HEXADECANE	9.641	634683	4.243 ug/ml
6)	N-OCTADECANE	11.054	2416440	15.674 ug/ml
7)	N-EICOSANE	12.397	392762	2.598 ug/ml
14)	N-DOTRIACONTANE	18.300	231124	1.698 ug/ml
15)	N-TETRATRIACONTANE	19.139	265259	2.233 ug/ml
16)	N-HEXATRIACONTANE	19.860	2574359	24.969 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020422\
Data File : FF009881.D
Signal(s) : FID2B.ch
Acq On : 04 Feb 2022 23:50
Operator : AJ\MA
Sample : N1393-04
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 05 00:56:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

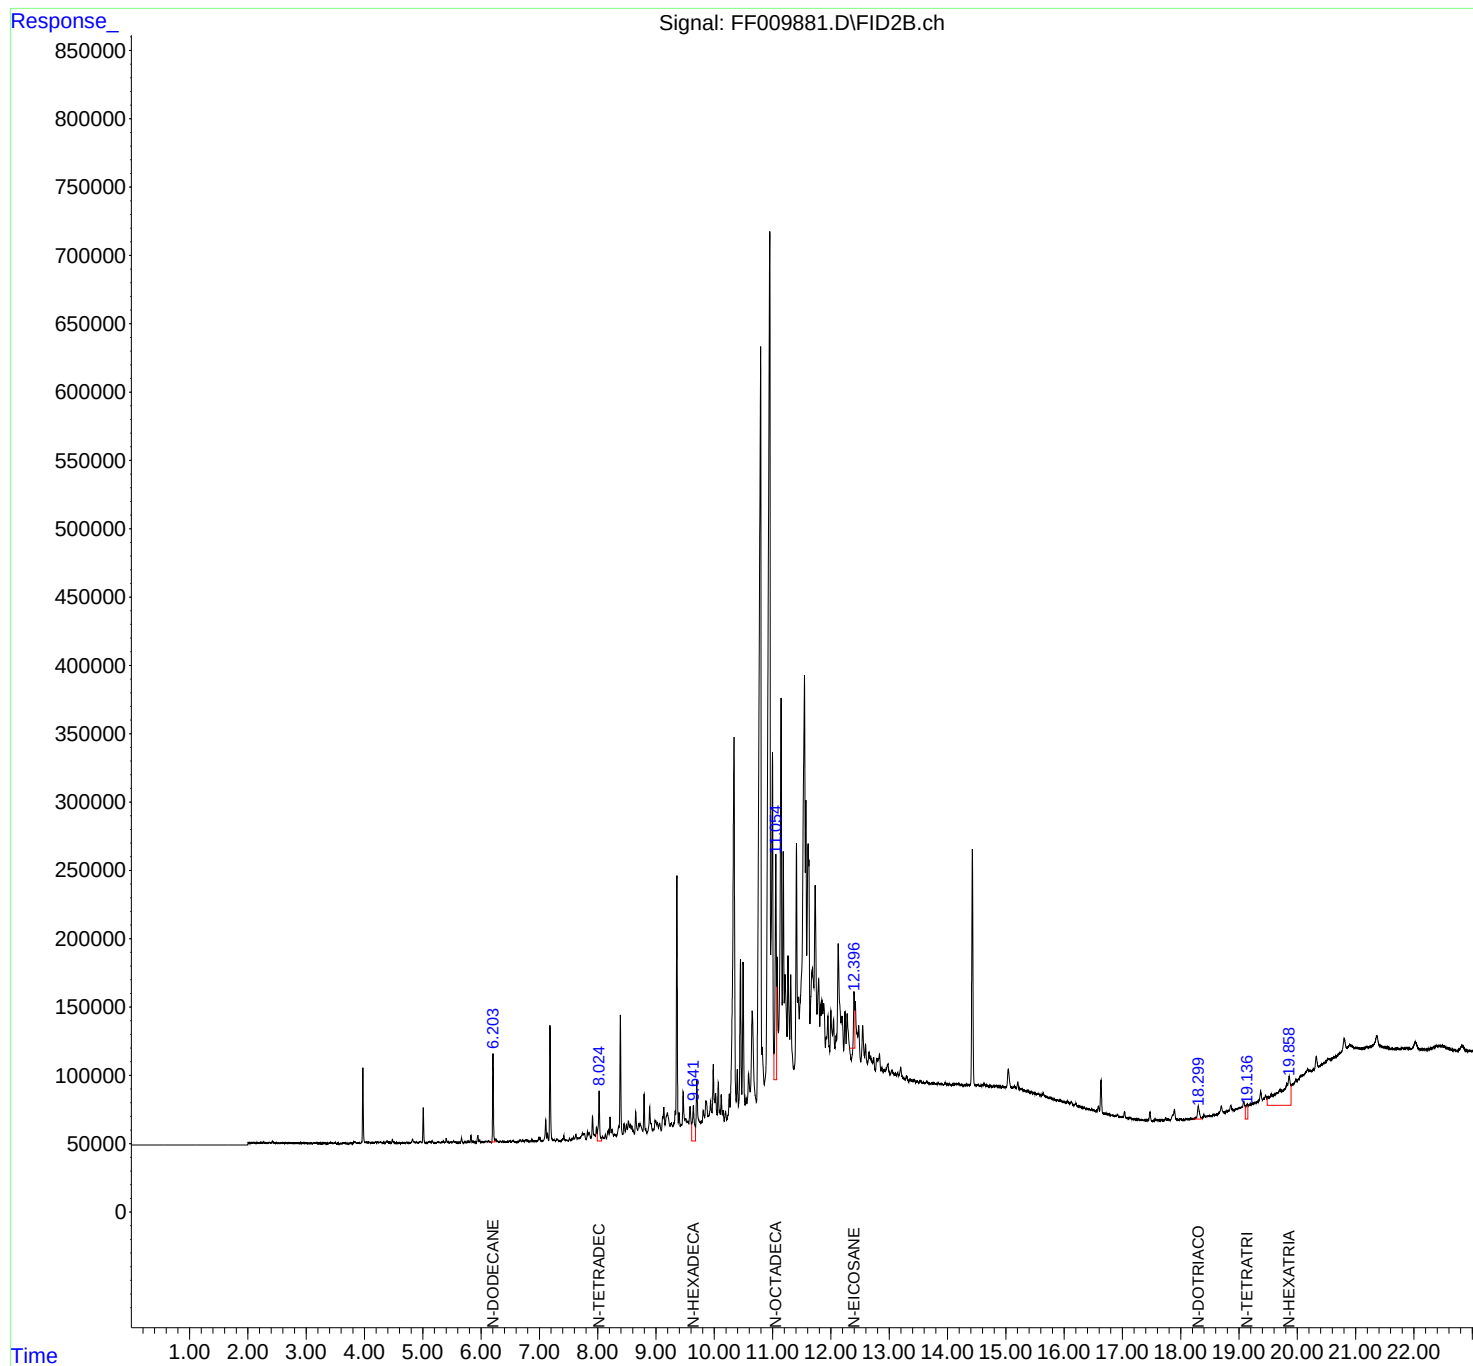


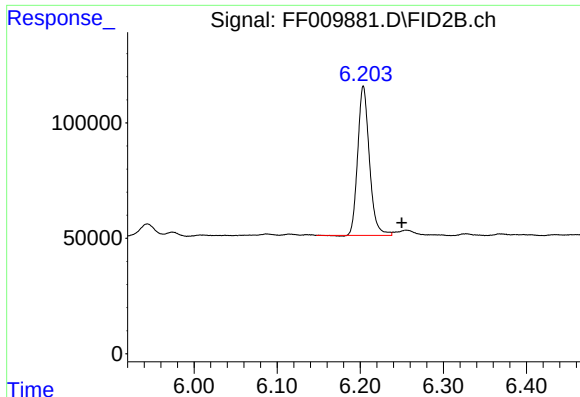

#3 N-DODECANE


R.T.: 6.204 min
Delta R.T.: -0.046 min
Response: 630841
Conc: 4.41 ug/ml

Instrument :
FID_F
ClientSampleId :

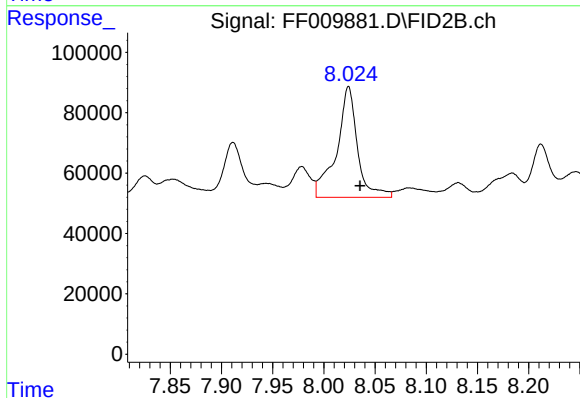


#4 N-TETRADECANE

R.T.: 8.024 min
Delta R.T.: -0.011 min
Response: 522122
Conc: 3.55 ug/ml

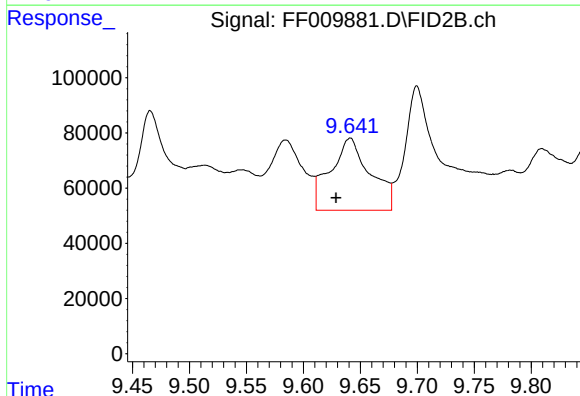


#5 N-HEXADECANE

R.T.: 9.641 min
Delta R.T.: 0.012 min
Response: 634683
Conc: 4.24 ug/ml

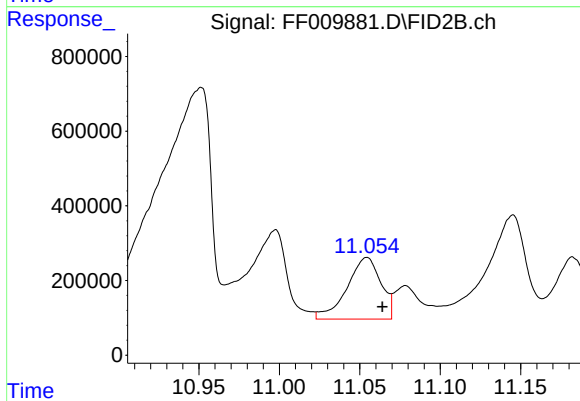

#6 N-OCTADECANE


R.T.: 11.054 min
Delta R.T.: -0.010 min
Response: 2416440
Conc: 15.67 ug/ml

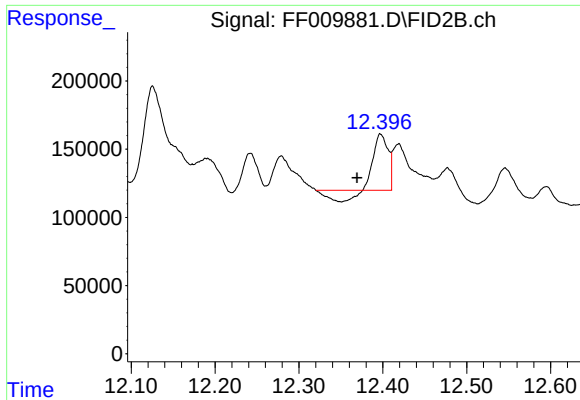

#7 N-EICOSANE


R.T.: 12.397 min
Delta R.T.: 0.028 min
Response: 392762
Conc: 2.60 ug/ml

Instrument :
FID_F
ClientSampleId :

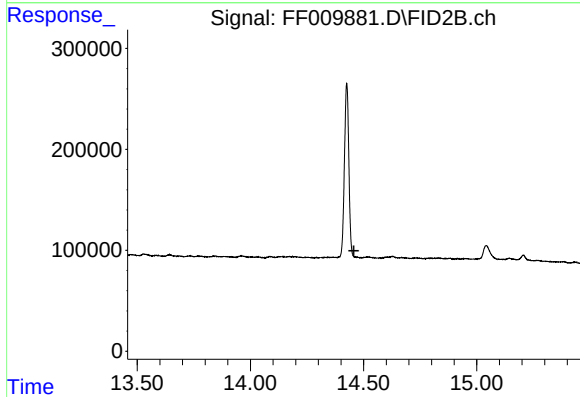


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.426 min
Delta R.T.: -0.032 min
Response: -5218043
Conc: N.D.

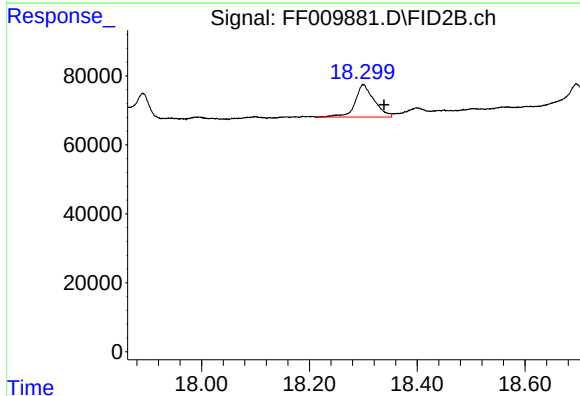


#14 N-DOTRIACONTANE

R.T.: 18.300 min
Delta R.T.: -0.038 min
Response: 231124
Conc: 1.70 ug/ml

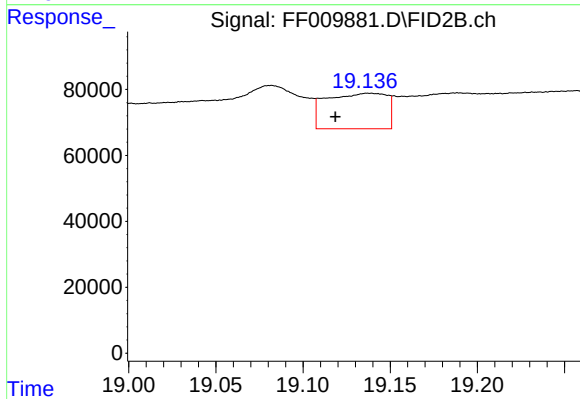

#15 N-TETRATRIACONTANE

R.T.: 19.139 min
Delta R.T.: 0.020 min
Response: 265259
Conc: 2.23 ug/ml

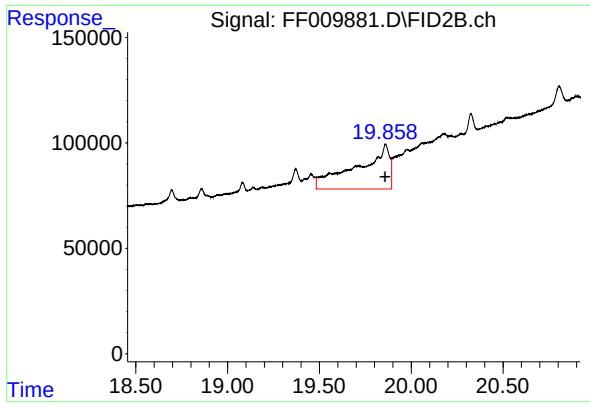

#16 N-HEXATRIACONTANE

R.T.: 19.860 min
Delta R.T.: 0.003 min
Response: 2574359
Conc: 24.97 ug/ml

Instrument :

FID_F

ClientSampleId :