

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020422\
 Data File : FF009883.D
 Signal(s) : FID2B.ch
 Acq On : 05 Feb 2022 00:49
 Operator : AJ\MA
 Sample : N1393-06
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 05 03:52:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
 Quant Title :
 QLast Update : Tue Jan 18 02:53:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.425	2817344	21.559 ug/ml
Target Compounds			
4) N-TETRADECANE	8.005	61076	0.416 ug/ml
6) N-OCTADECANE	11.032	35442	0.230 ug/ml
12) N-OCTACOSANE	16.632	187839	1.294 ug/ml
13) N-TRIACONTANE	17.471	138168	0.966 ug/ml
14) N-DOTRIACONTANE	18.298	186352	1.369 ug/ml
15) N-TETRATRIACONTANE	19.081	99276	0.836 ug/ml
16) N-HEXATRIACONTANE	19.861	387996	3.763 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020422\
Data File : FF009883.D
Signal(s) : FID2B.ch
Acq On : 05 Feb 2022 00:49
Operator : AJ\MA
Sample : N1393-06
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 05 03:52:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

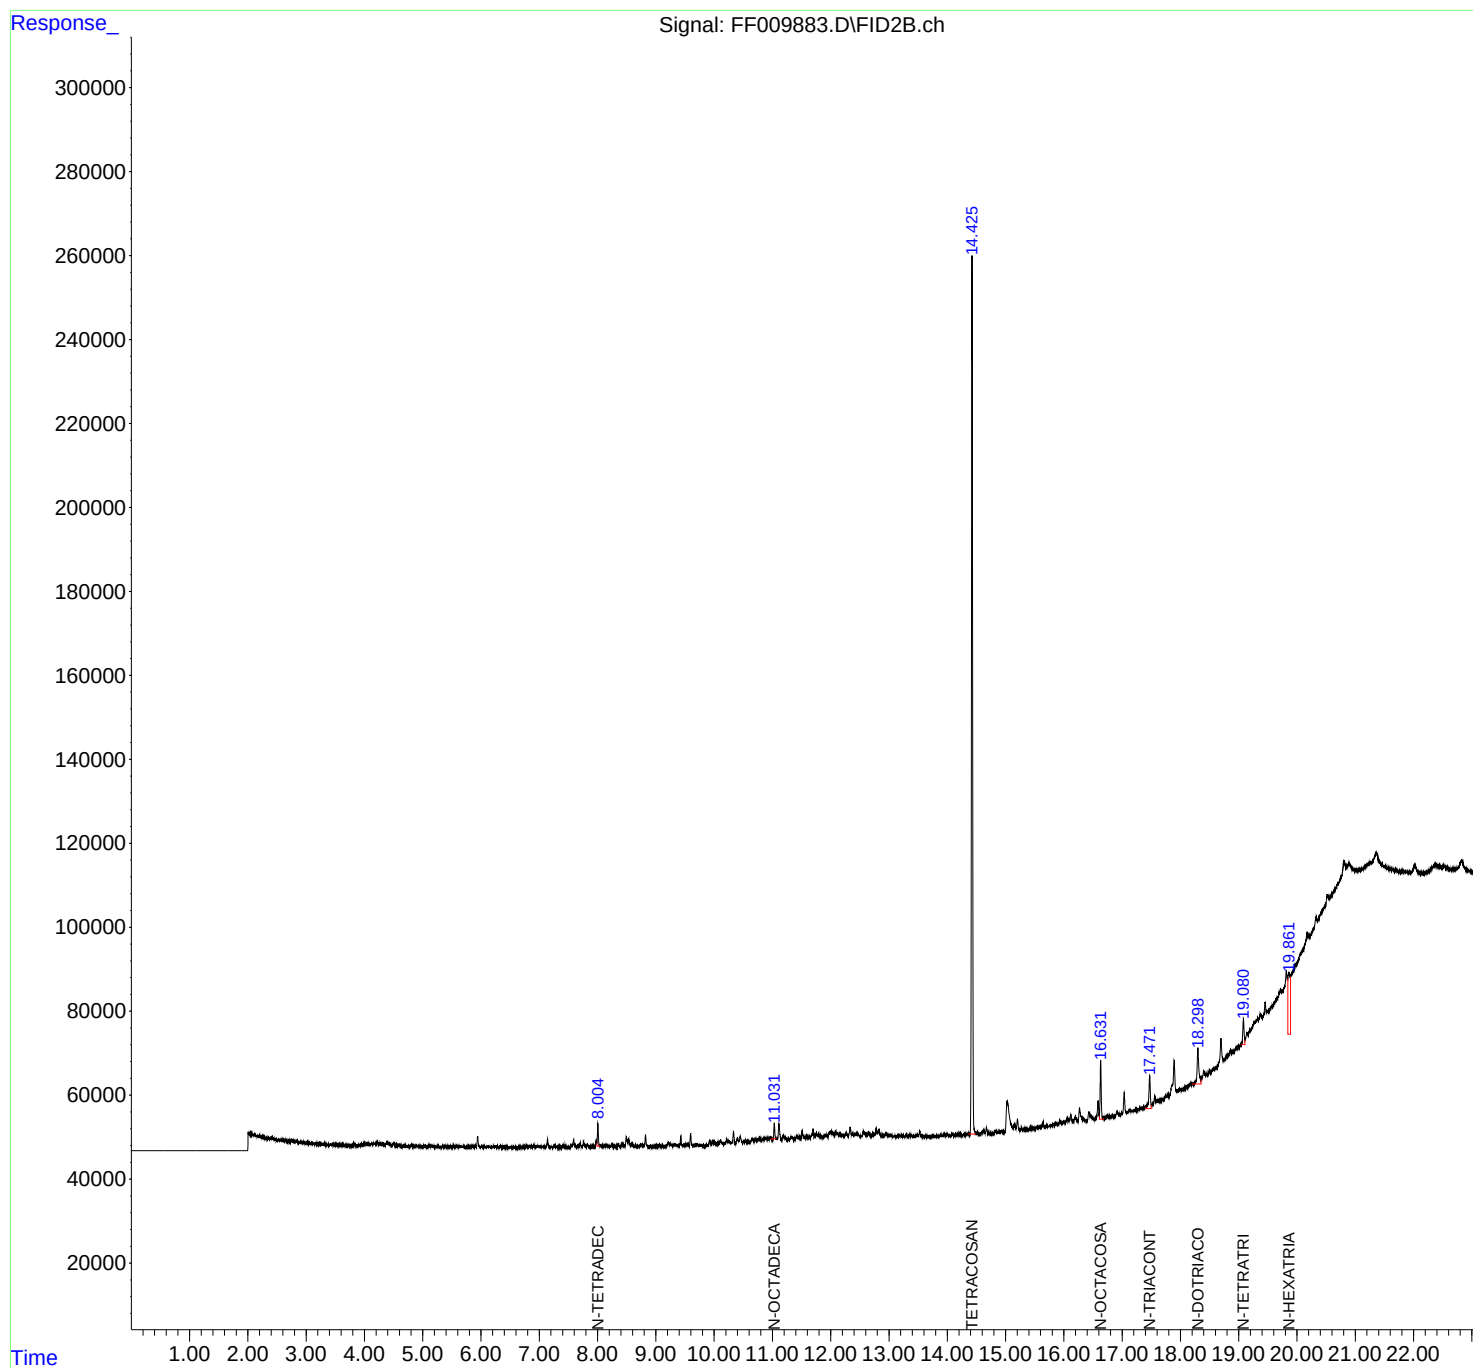


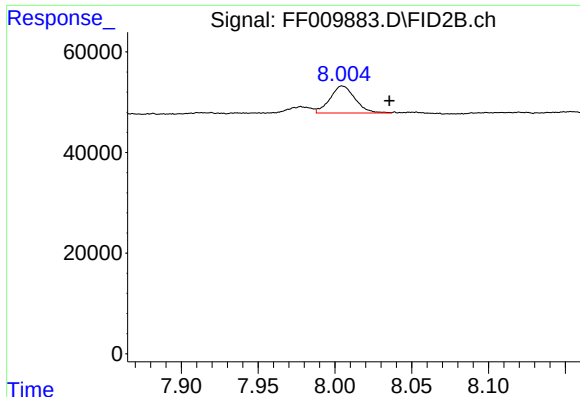

#4 N-TETRADECANE


R.T.: 8.005 min
Delta R.T.: -0.031 min
Response: 61076
Conc: 0.42 ug/ml

Instrument :
FID_F
ClientSampleId :

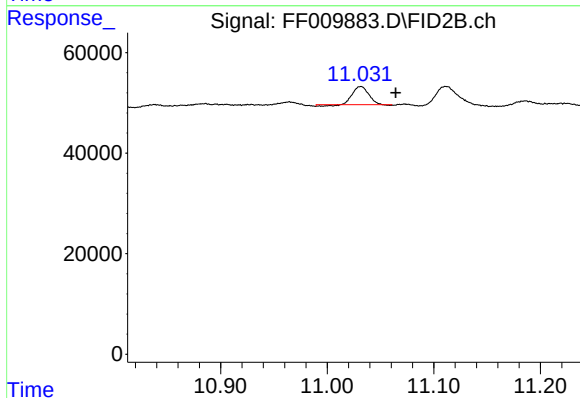


#6 N-OCTADECANE

R.T.: 11.032 min
Delta R.T.: -0.032 min
Response: 35442
Conc: 0.23 ug/ml

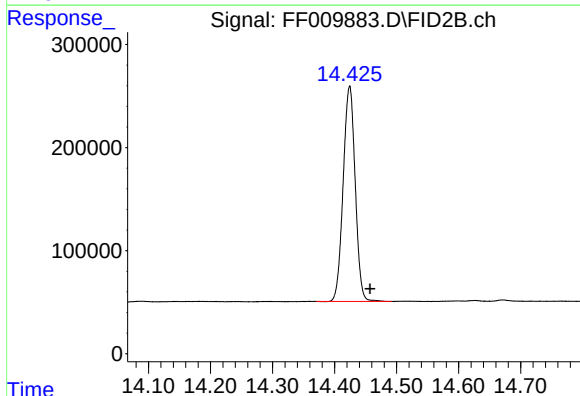


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.425 min
Delta R.T.: -0.032 min
Response: 2817344
Conc: 21.56 ug/ml

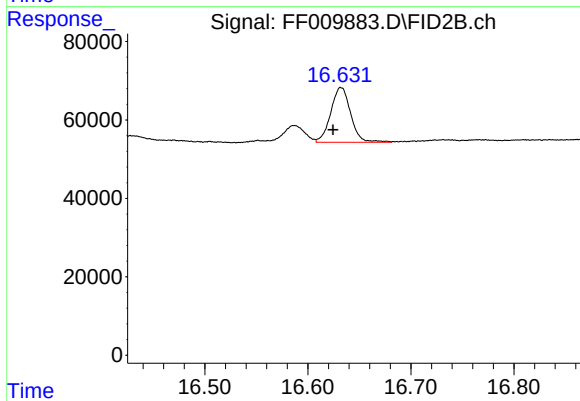

#12 N-OCTACOSANE


R.T.: 16.632 min
Delta R.T.: 0.007 min
Response: 187839
Conc: 1.29 ug/ml

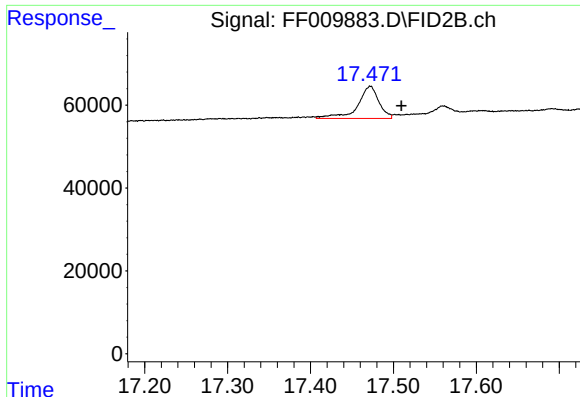

#13 N-TRIACONTANE


R.T.: 17.471 min
Delta R.T.: -0.038 min
Response: 138168
Conc: 0.97 ug/ml

Instrument :
FID_F
ClientSampleId :

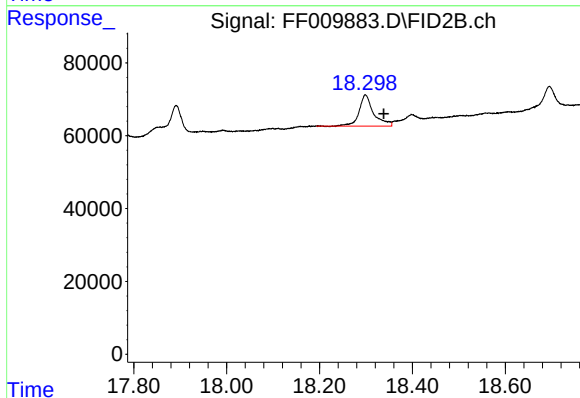


#14 N-DOTRIACONTANE

R.T.: 18.298 min
Delta R.T.: -0.040 min
Response: 186352
Conc: 1.37 ug/ml

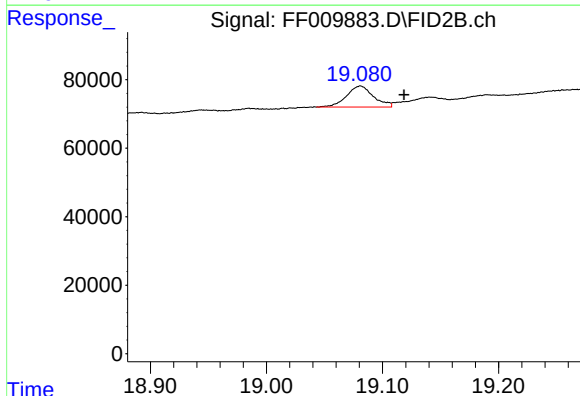

#15 N-TETRATRIACONTANE

R.T.: 19.081 min
Delta R.T.: -0.038 min
Response: 99276
Conc: 0.84 ug/ml

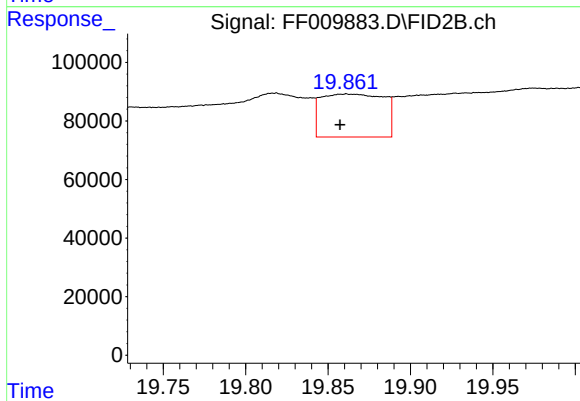

#16 N-HEXATRIACONTANE

R.T.: 19.861 min
Delta R.T.: 0.004 min
Response: 387996
Conc: 3.76 ug/ml