

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020422\
Data File : FF009884.D
Signal(s) : FID2B.ch
Acq On : 05 Feb 2022 01:18
Operator : AJ\MA
Sample : N1399-01
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 05 03:52:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

1)	N-OCTANE	2.152	120309	0.870 ug/ml
2)	N-DECANE	4.250	2448860	17.315 ug/ml
3)	N-DODECANE	6.278	29620927	206.995 ug/ml
4)	N-TETRADECANE	8.035	77629460	528.280 ug/ml
5)	N-HEXADECANE	9.626	65180433	435.717 ug/ml
7)	N-EICOSANE	12.373	974319	6.446 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF020422\
Data File : FF009884.D
Signal(s) : FID2B.ch
Acq On : 05 Feb 2022 01:18
Operator : AJ\MA
Sample : N1399-01
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 05 03:52:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF011722.M
Quant Title :
QLast Update : Tue Jan 18 02:53:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

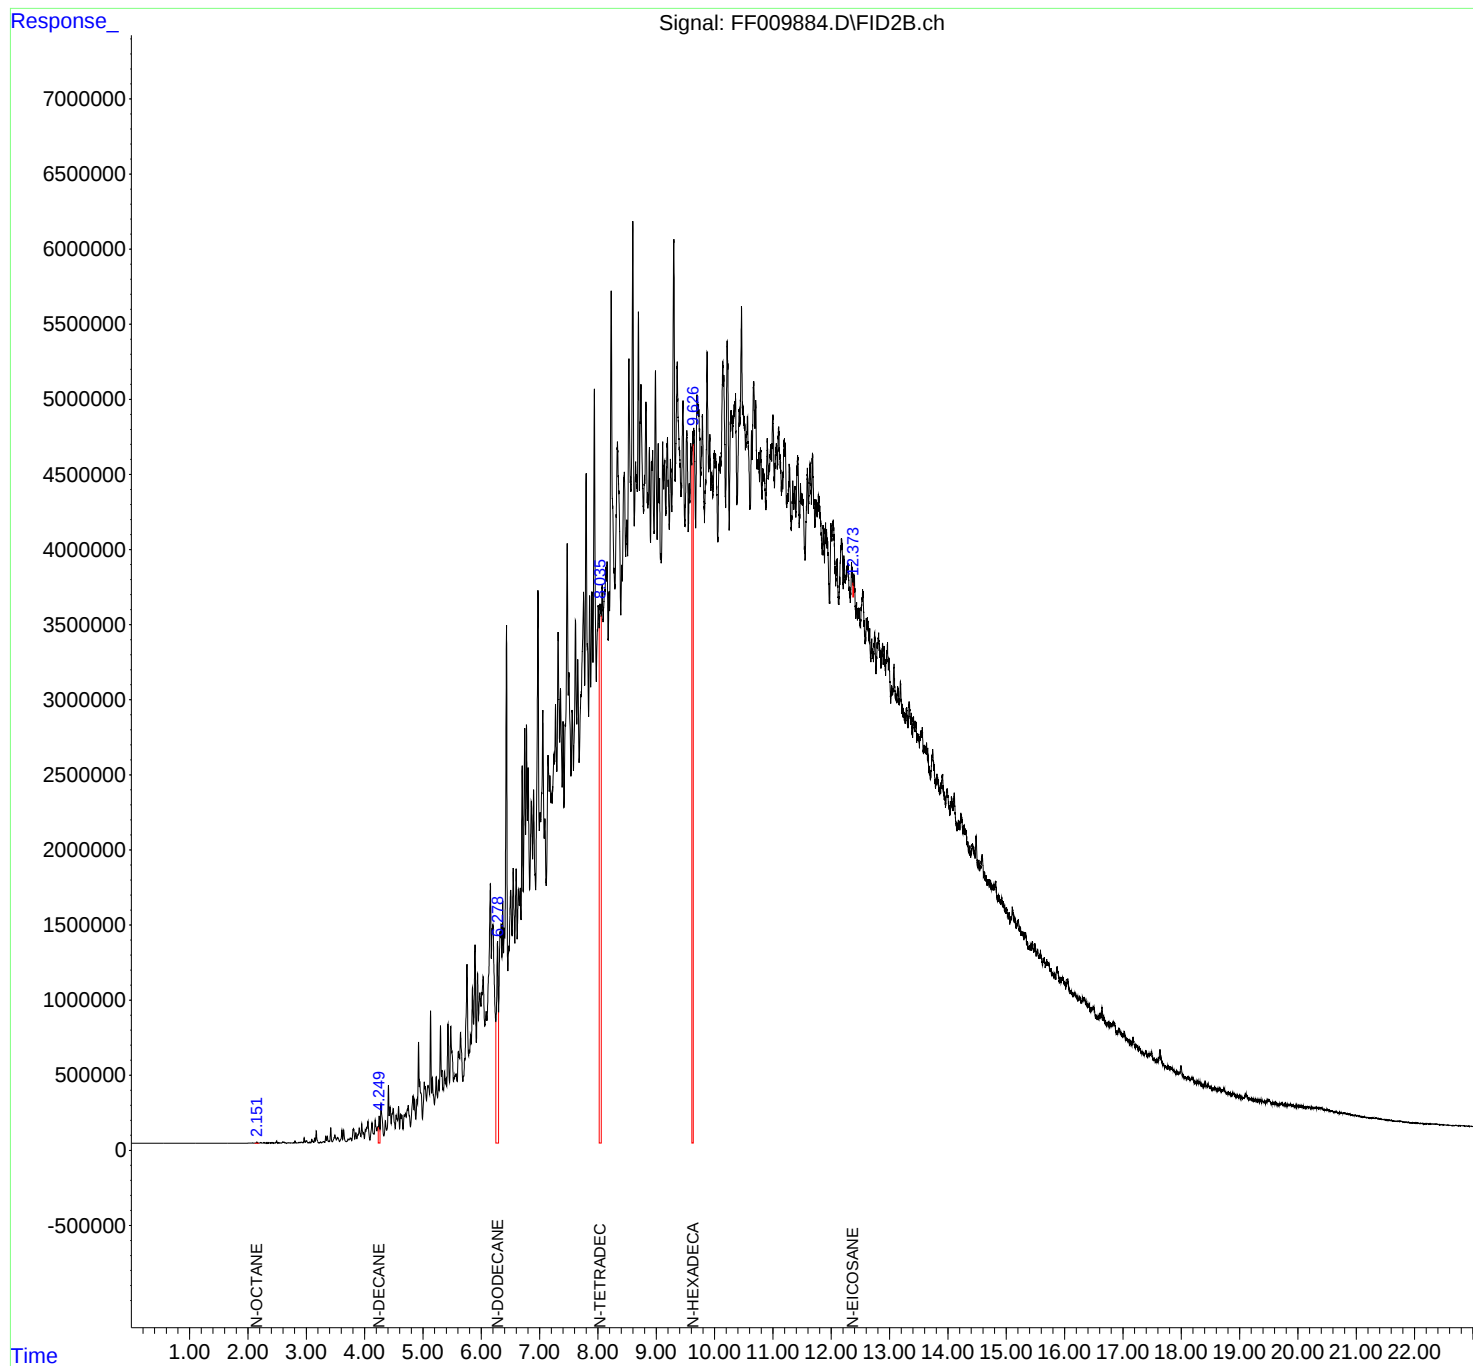


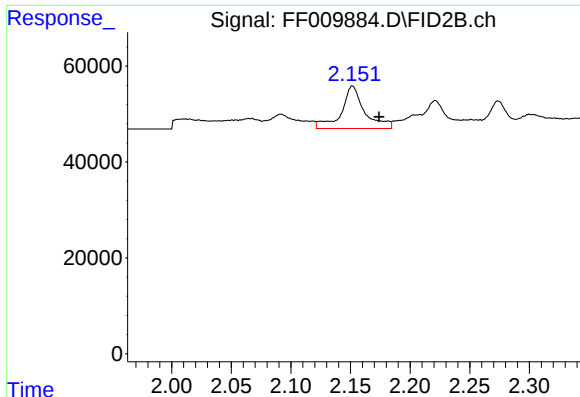

#1 N-OCTANE


R.T.: 2.152 min
Delta R.T.: -0.022 min
Response: 120309
Conc: 0.87 ug/ml

Instrument :
FID_F
ClientSampleId :

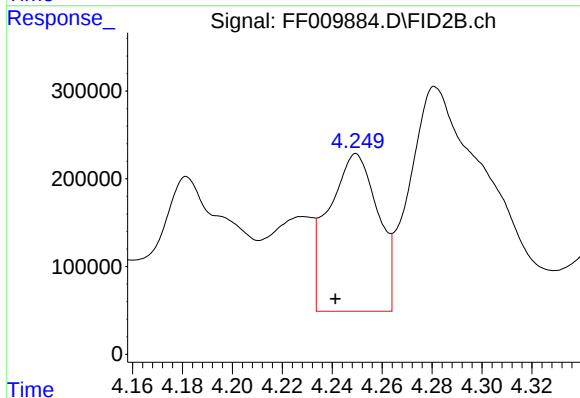


#2 N-DECANE

R.T.: 4.250 min
Delta R.T.: 0.008 min
Response: 2448860
Conc: 17.32 ug/ml

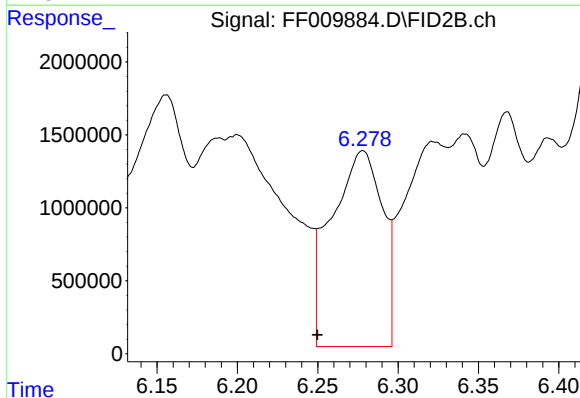


#3 N-DODECANE

R.T.: 6.278 min
Delta R.T.: 0.028 min
Response: 29620927
Conc: 207.00 ug/ml

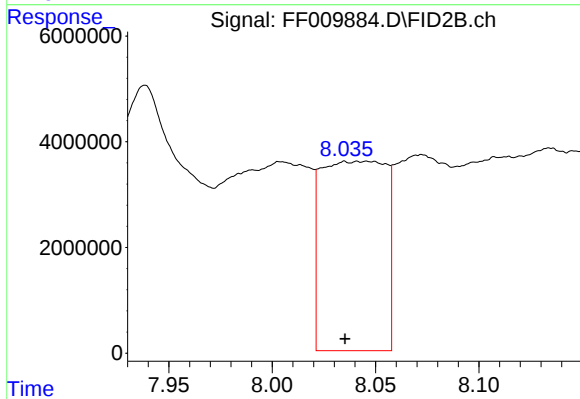

#4 N-TETRADECANE


R.T.: 8.035 min
Delta R.T.: 0.000 min
Response: 77629460
Conc: 528.28 ug/ml

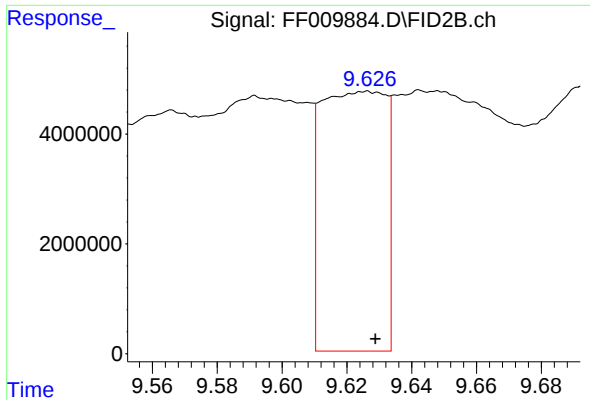

#5 N-HEXADECANE


R.T.: 9.626 min
Delta R.T.: -0.003 min
Response: 65180433
Conc: 435.72 ug/ml

Instrument :
FID_F
ClientSampleId :

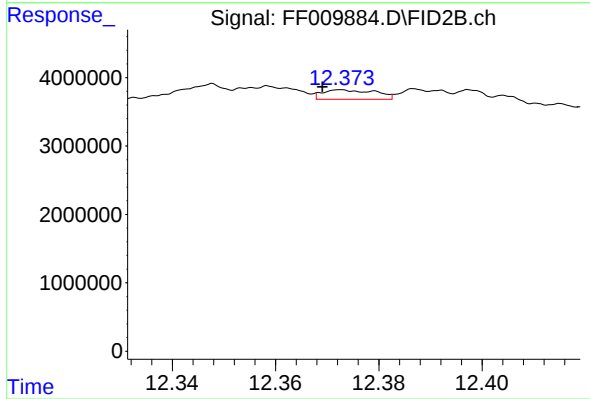

#7 N-EICOSANE

R.T.: 12.373 min
Delta R.T.: 0.004 min
Response: 974319
Conc: 6.45 ug/ml

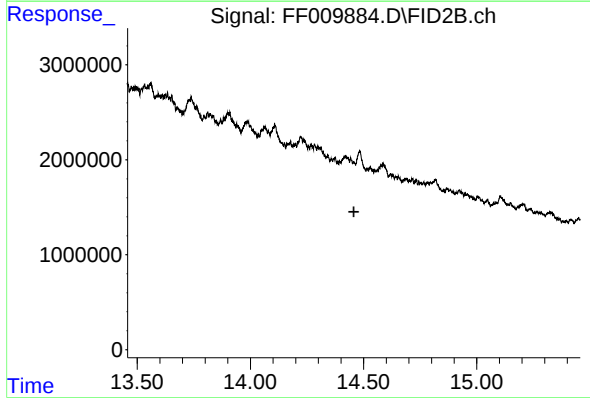

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.457 min
Delta R.T.: 0.000 min
Response: -9862436
Conc: N.D.